


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031924\
Data File : BG060676.D
Acq On : 19 Mar 2024 10:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 18 14:26:31 2024

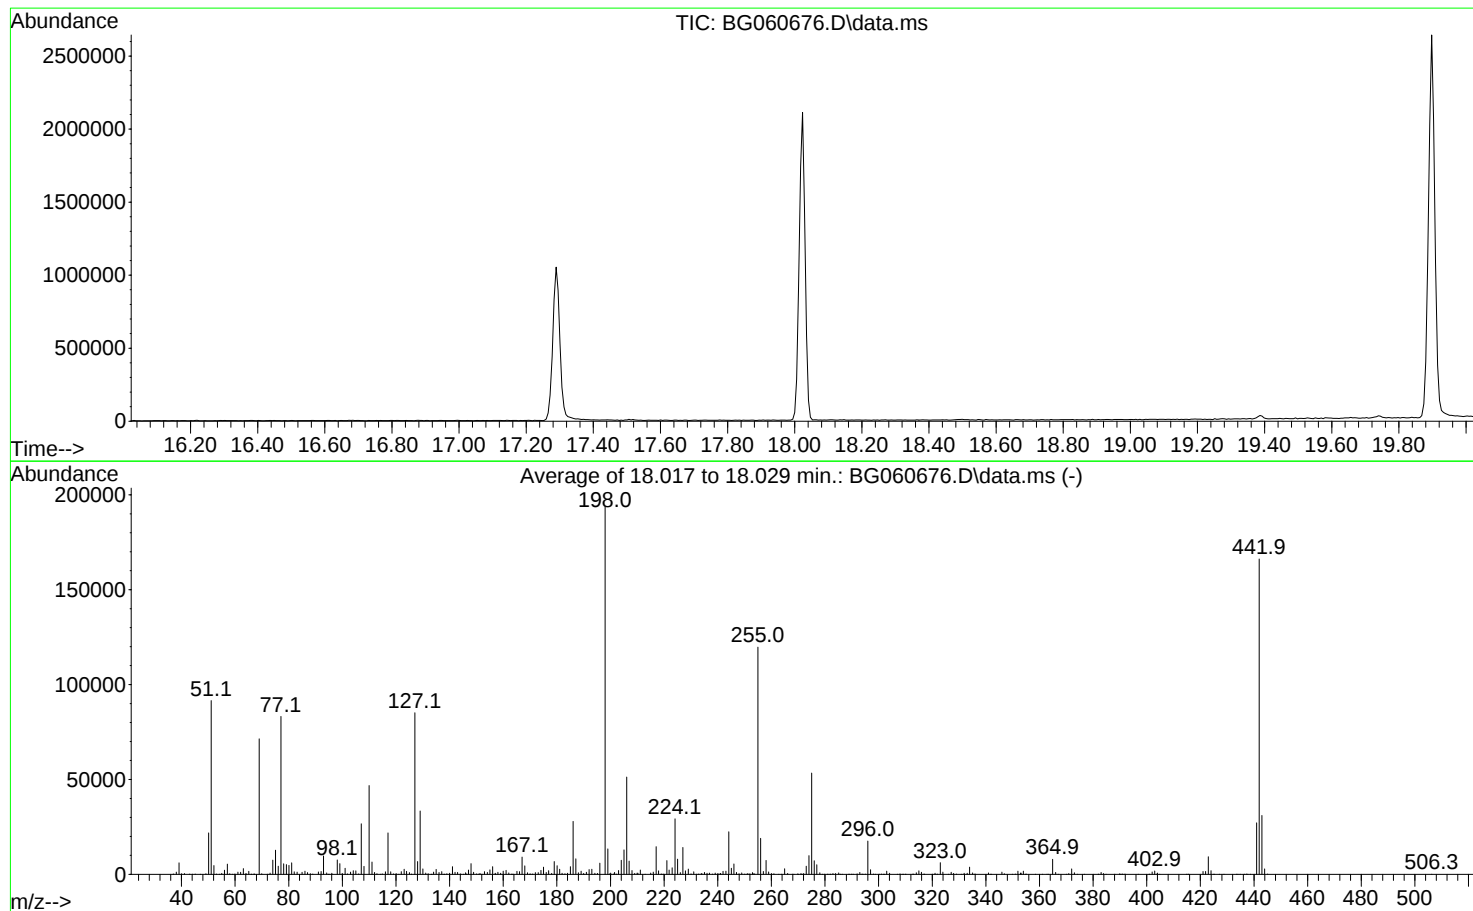




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	91536	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.8	71395	PASS
70	69	0.00	2	0.5	346	PASS
127	198	10	80	43.9	85139	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	193856	PASS
199	198	5	9	6.9	13399	PASS
275	198	10	60	27.5	53392	PASS
365	198	1	100	4.1	7930	PASS
441	198	0.01	100	14.0	27155	PASS
442	442	50	100	100.0	166235	PASS
443	442	15	24	18.6	30995	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031924\
Data File : BG060676.D
Acq On : 19 Mar 2024 10:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 20 01:46:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 18 14:26:31 2024
Response via : Initial Calibration

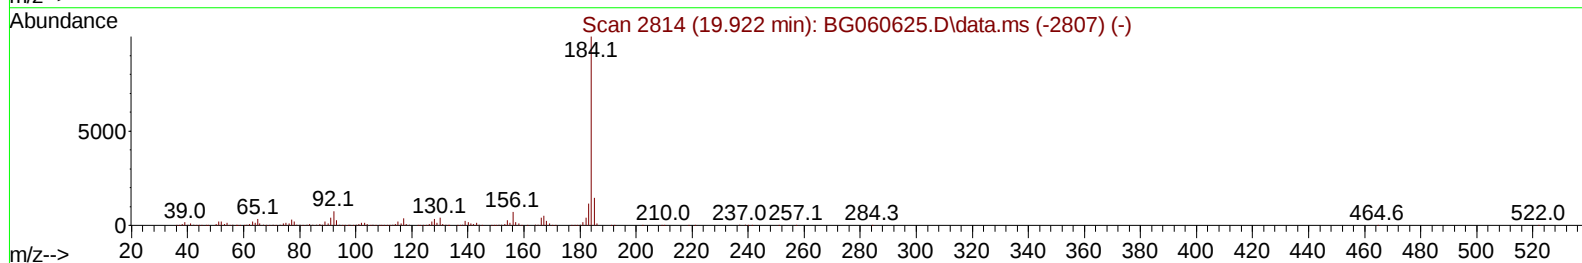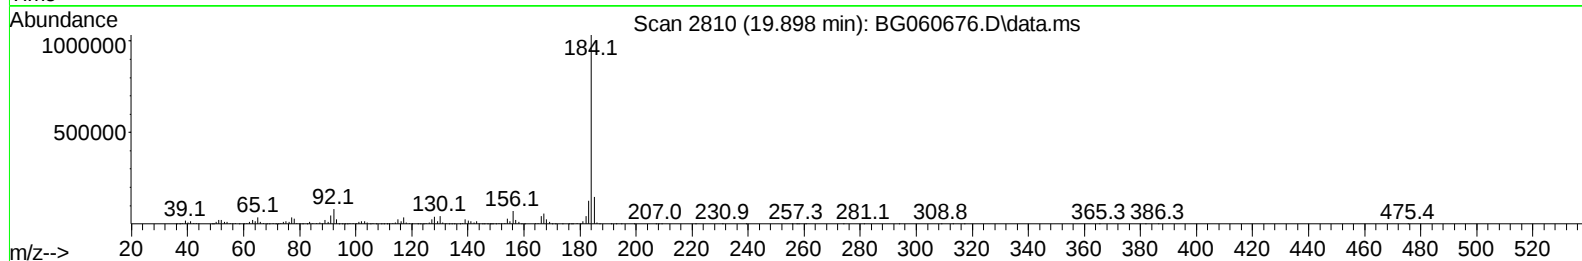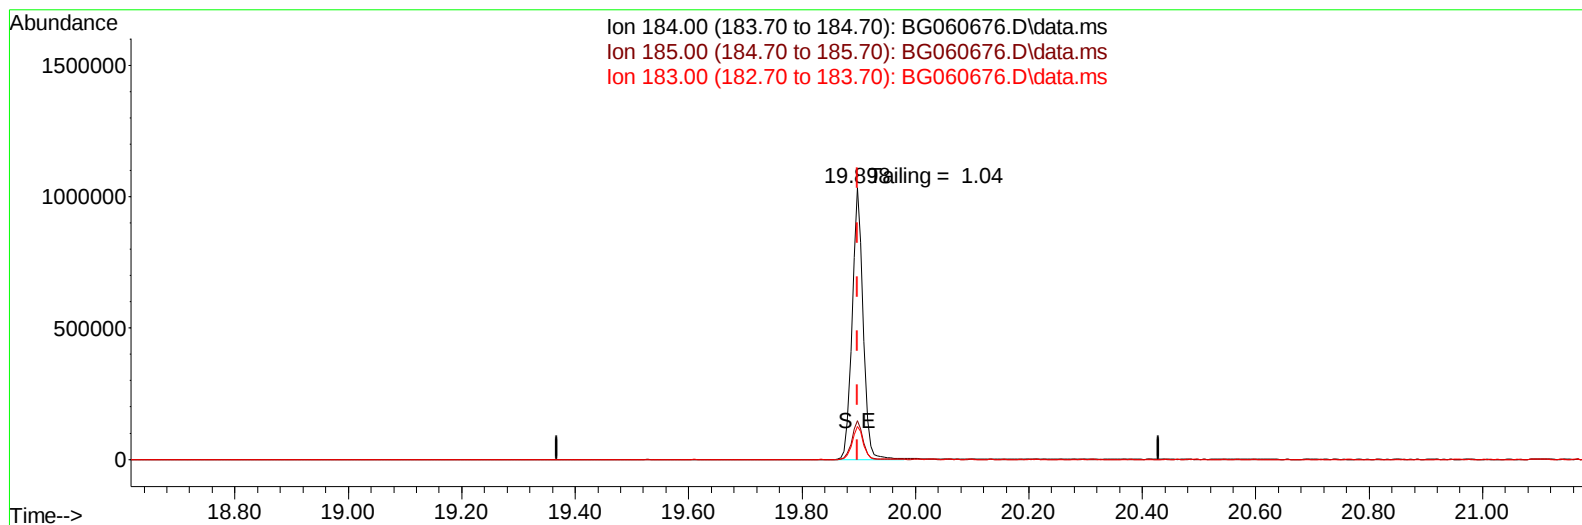

TIC: BG060676.D\data.ms

(77) Benzidine

19.898min (-0.001) 961875.67 ng

response 1388117

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	11.50	12.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/19/2024	BNA_G	<u>BG060676.D</u>
Compound Name	Response	Retention Time
DDT	467211	21.108
DDD	20145	20.65
DDE	392	20.144
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20537	487748	4.21

Instrument :
BNA_G
ClientSampleId :
DFTPP