
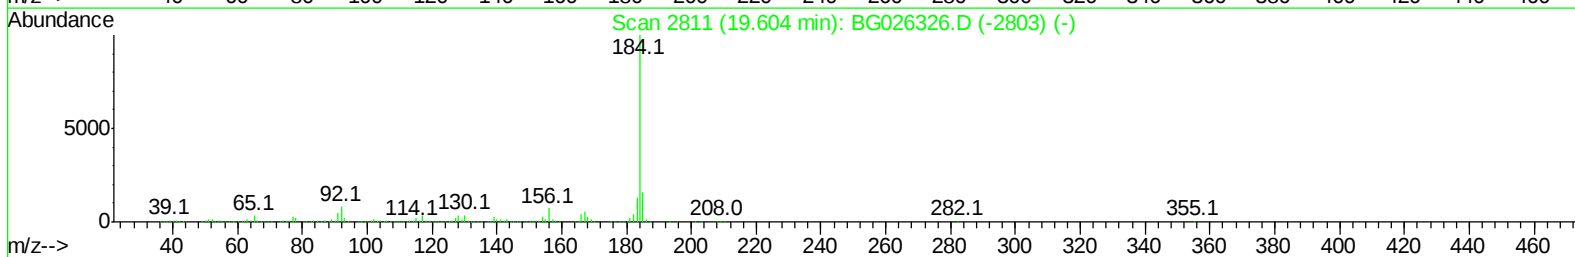
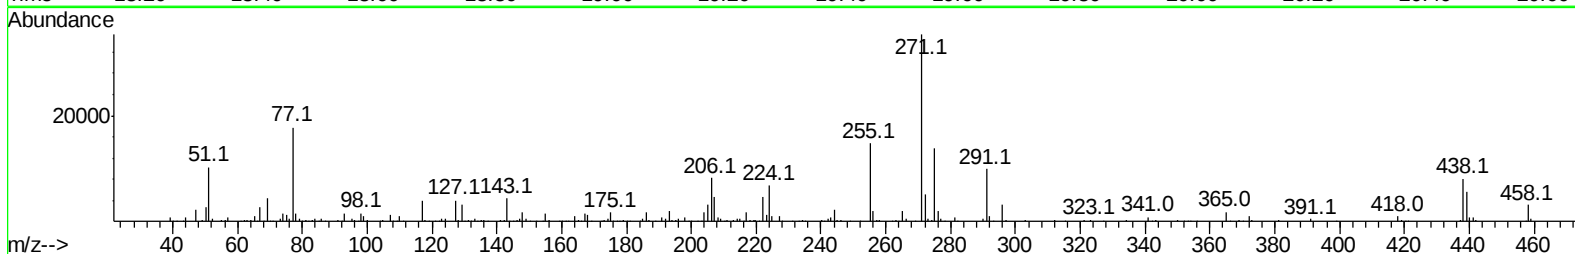


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032017\
Data File : BG026322.D
Acq On : 20 Mar 2017 11:55
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 07:21:28 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

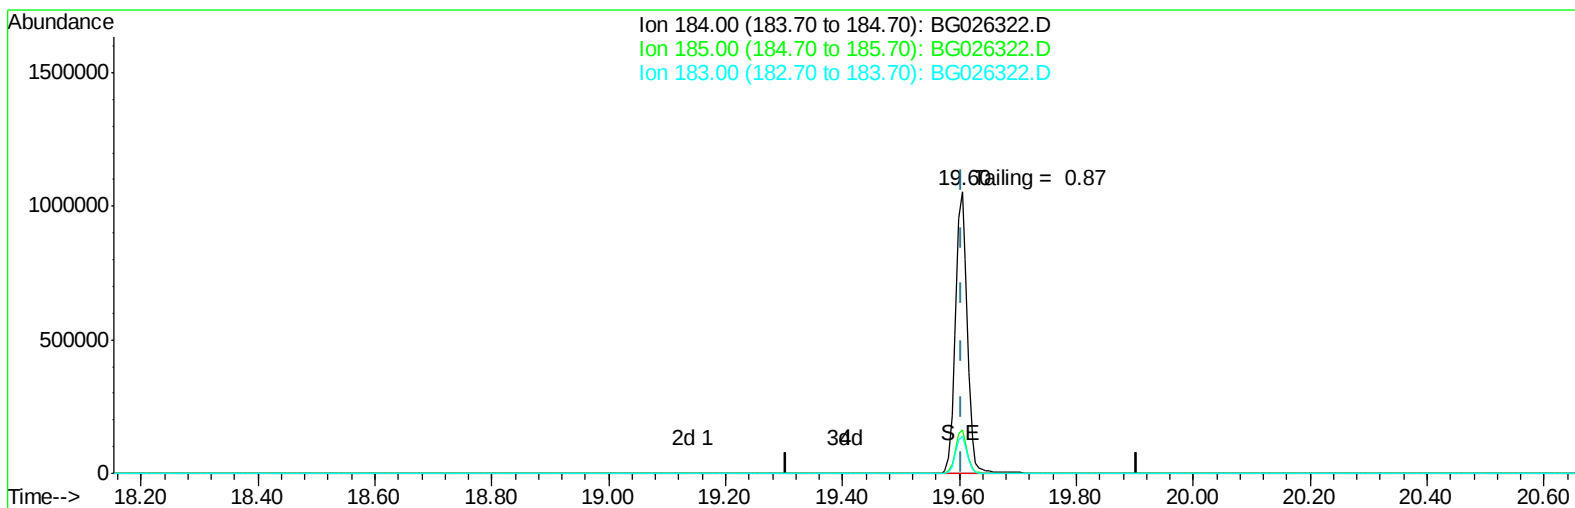

TIC: BG026322.D

(76) Benzidine




19.170min (-0.434) 56.07ng

response 116

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	351.40#
183.00	13.80	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032017\
Data File : BG026322.D
Acq On : 20 Mar 2017 11:55
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 07:21:28 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

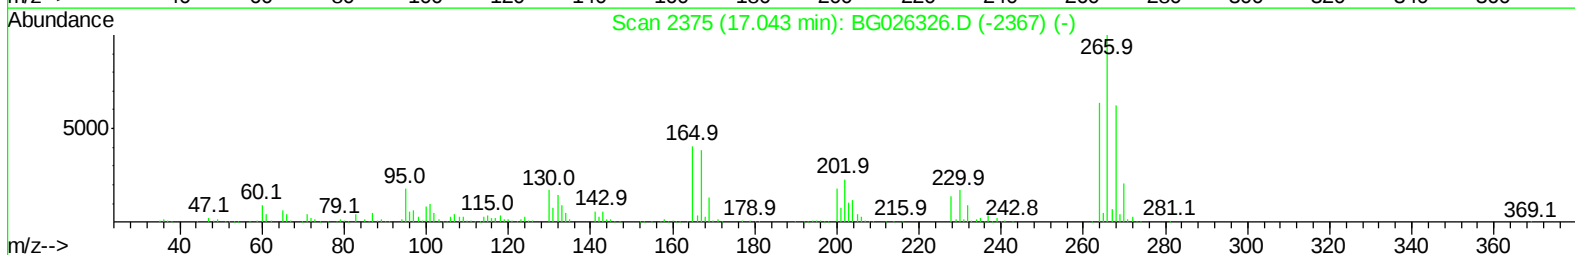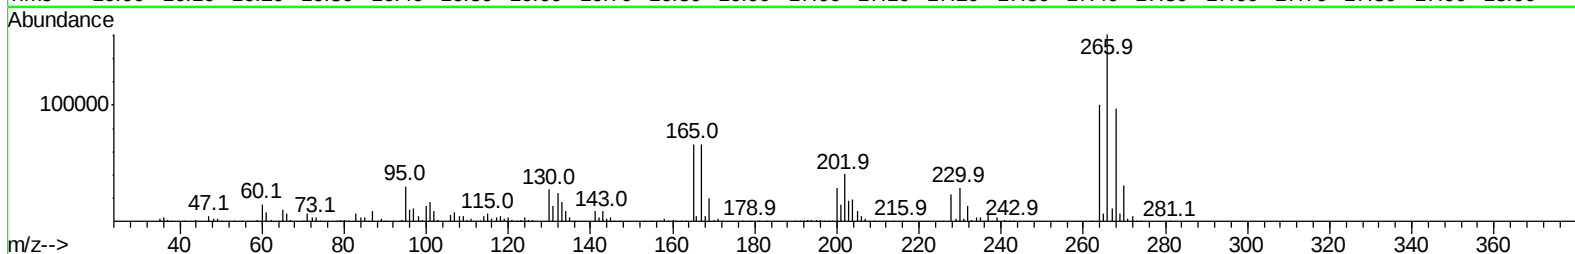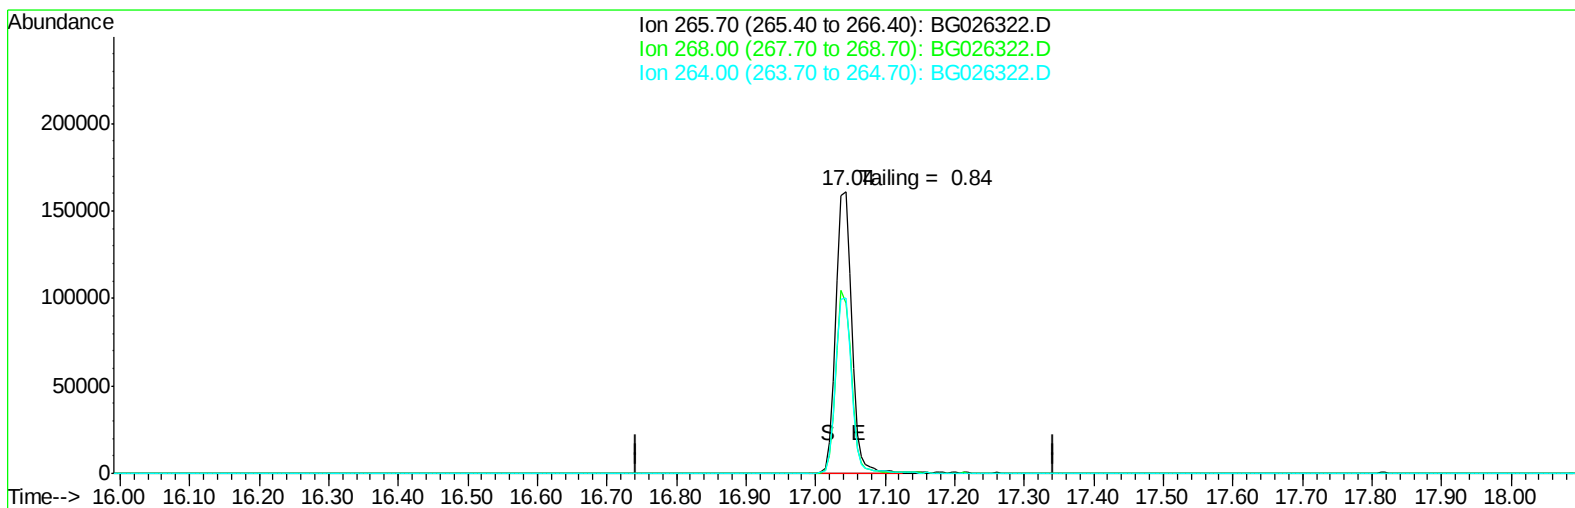

TIC: BG026322.D

(69) Pentachlorophenol (C)

17.043min (-17.043) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	60.70	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00