


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032017\
 Data File : BG026322.D
 Acq On : 20 Mar 2017 11:55
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 20 17:43:27 2017

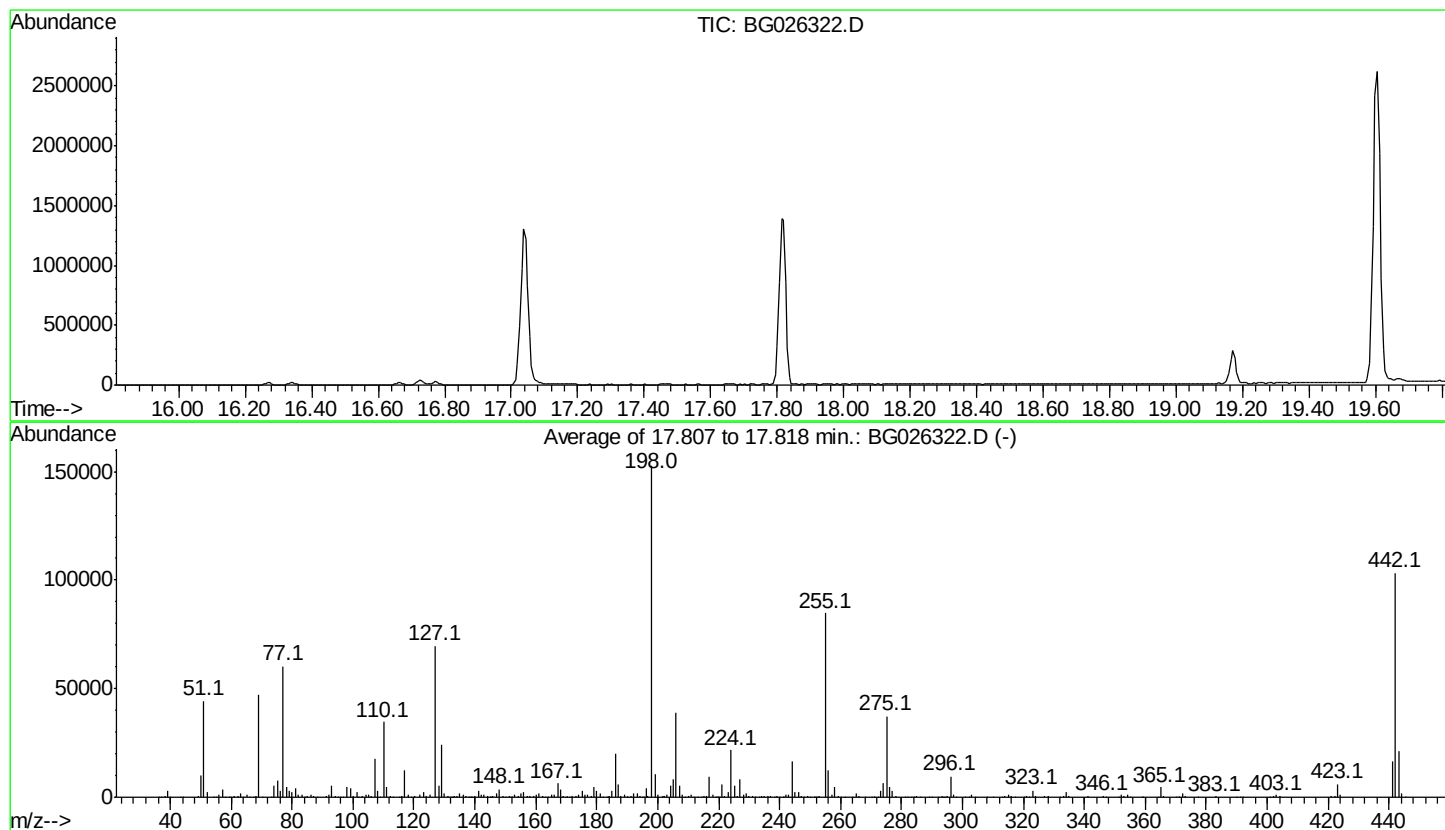

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	44341	PASS
68	69	0.00	2	0.8	374	PASS
69	198	0.00	100	31.0	47336	PASS
70	69	0.00	2	0.1	45	PASS
127	198	10	80	45.6	69602	PASS
197	198	0.00	2	0.6	881	PASS
198	198	100	100	100.0	152765	PASS
199	198	5	9	6.9	10616	PASS
275	198	10	60	24.4	37341	PASS
365	198	1	100	3.0	4644	PASS
441	442	0.01	24	15.7	16286	PASS
442	198	50	100	67.7	103432	PASS
443	442	15	24	20.5	21210	PASS