
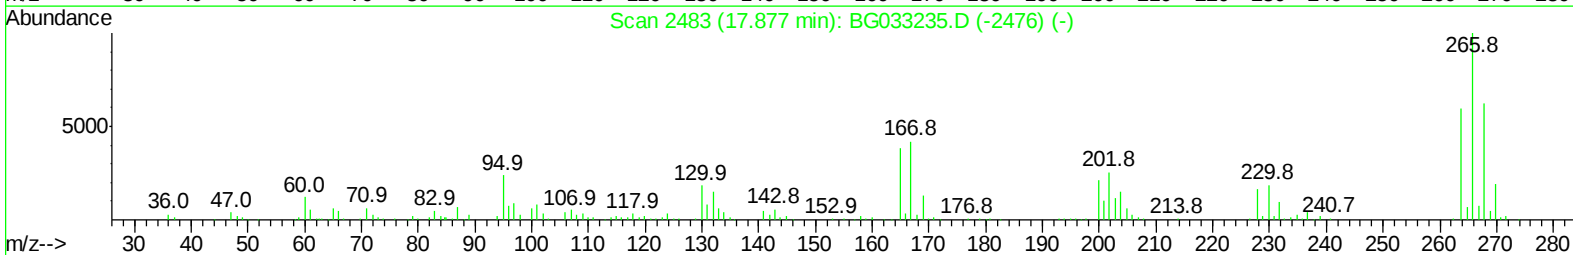
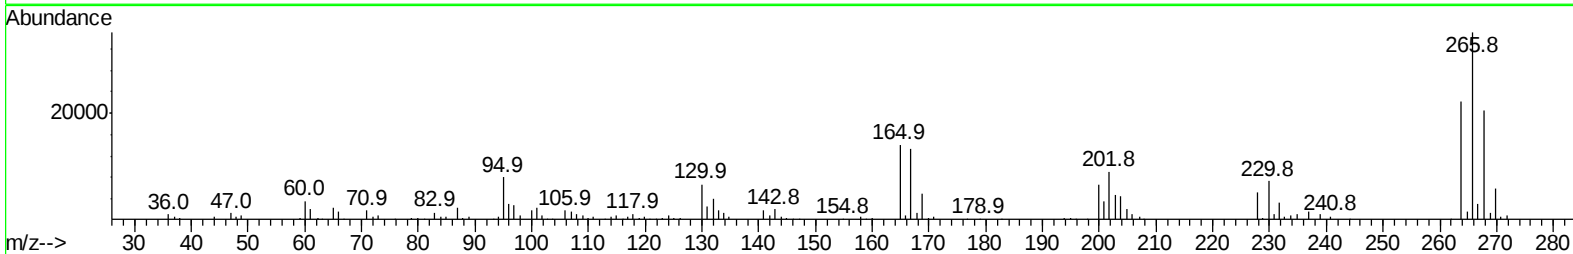


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG032018\
Data File : BG033275.D
Acq On : 20 Mar 2018 21:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 04:03:23 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 19 16:48:53 2018
Response via : Initial Calibration

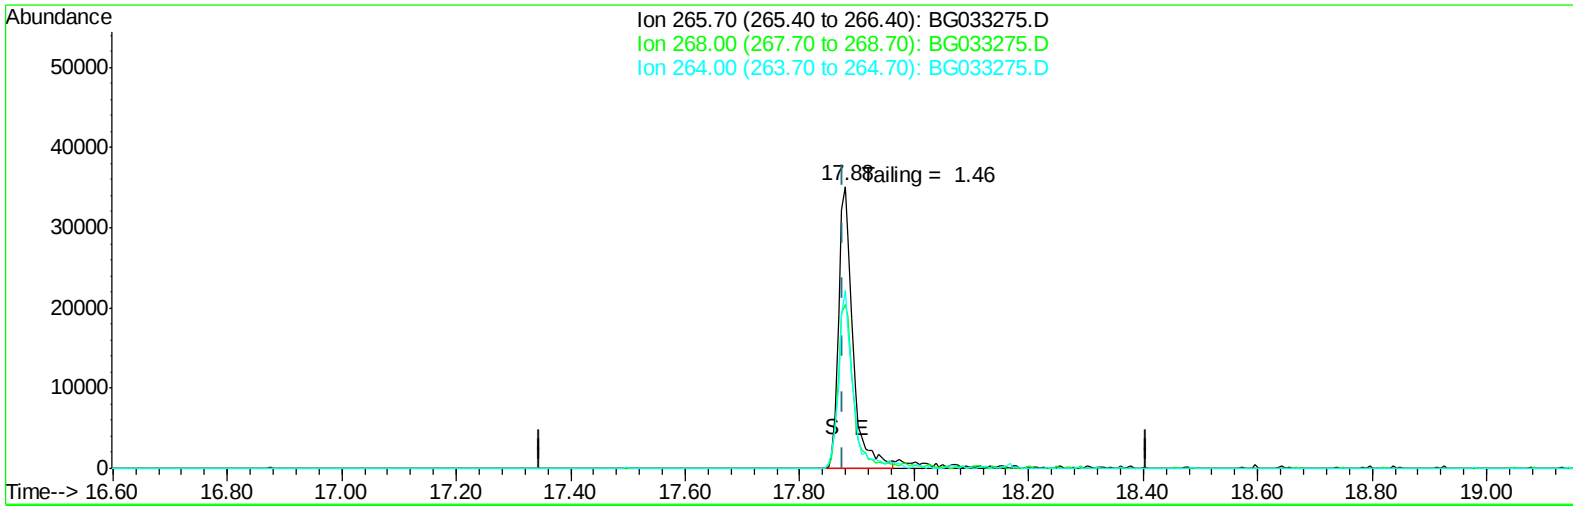

TIC: BG033275.D

(69) Pentachlorophenol (C)




17.879min (+0.003) 13989.39ng m

response 61645

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.13
264.00	62.00	63.26
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG032018\
Data File : BG033275.D
Acq On : 20 Mar 2018 21:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 04:03:23 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 19 16:48:53 2018
Response via : Initial Calibration

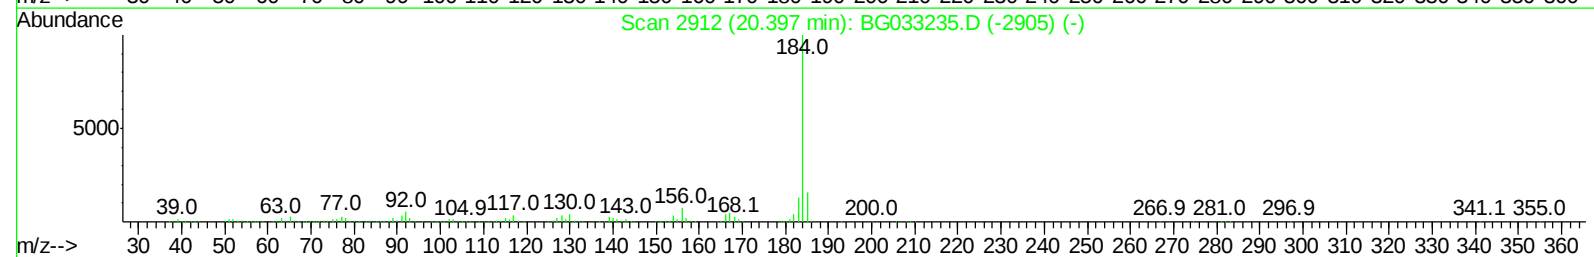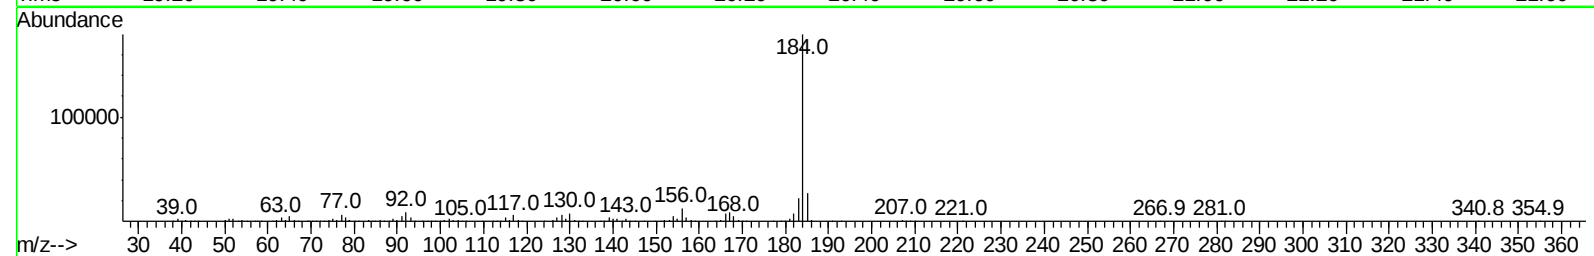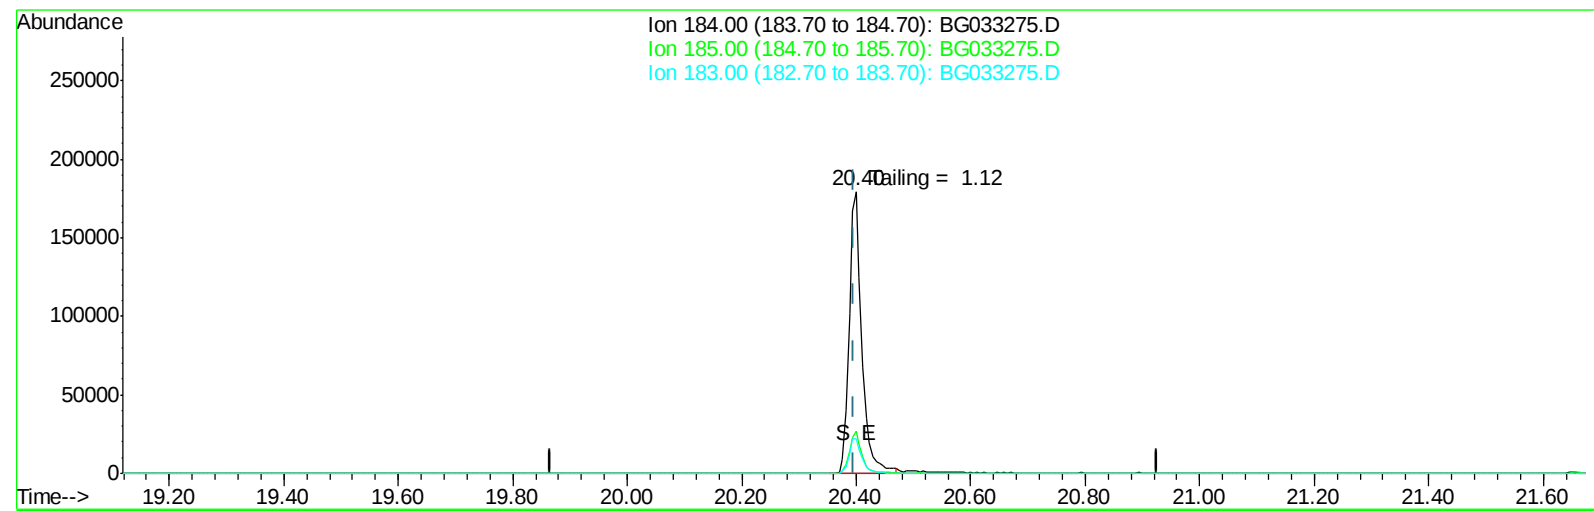

TIC: BG033275.D

(76) Benzidine

20.400min (+0.003) 0.00ng

response 278435

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.99
183.00	13.30	12.36
0.00	0.00	0.00