

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG032018\
 Data File : BG033285.D
 Acq On : 21 Mar 2018 3:20
 Operator : SJ/JU
 Sample : J1977-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP

Quant Time: Mar 21 06:38:42 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 19 16:48:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.90	152	35141	20.00	ng	0.00
21) Naphthalene-d8	11.78	136	149649	20.00	ng	0.00
38) Acenaphthene-d10	15.51	164	117041	20.00	ng	0.00
63) Phenanthrene-d10	18.24	188	320264	20.00	ng	0.00
75) Chrysene-d12	22.60	240	319830	20.00	ng	0.00
86) Perylene-d12	26.39	264	329078	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.31	112	321093	171.33	ng	0.00
7) Phenol-d6	8.00	99	439547	136.50	ng	0.00
23) Nitrobenzene-d5	10.09	82	354229	108.75	ng	0.00
41) 2,4,6-Tribromophenol	16.98	330	259426	148.20	ng	0.00
44) 2-Fluorobiphenyl	14.14	172	831098	102.51	ng	0.00
78) Terphenyl-d14	20.76	244	1657953	110.86	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG032018\
Data File : BG033285.D
Acq On : 21 Mar 2018 3:20
Operator : SJ/JU
Sample : J1977-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP

Quant Time: Mar 21 06:38:42 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 19 16:48:53 2018
Response via : Initial Calibration

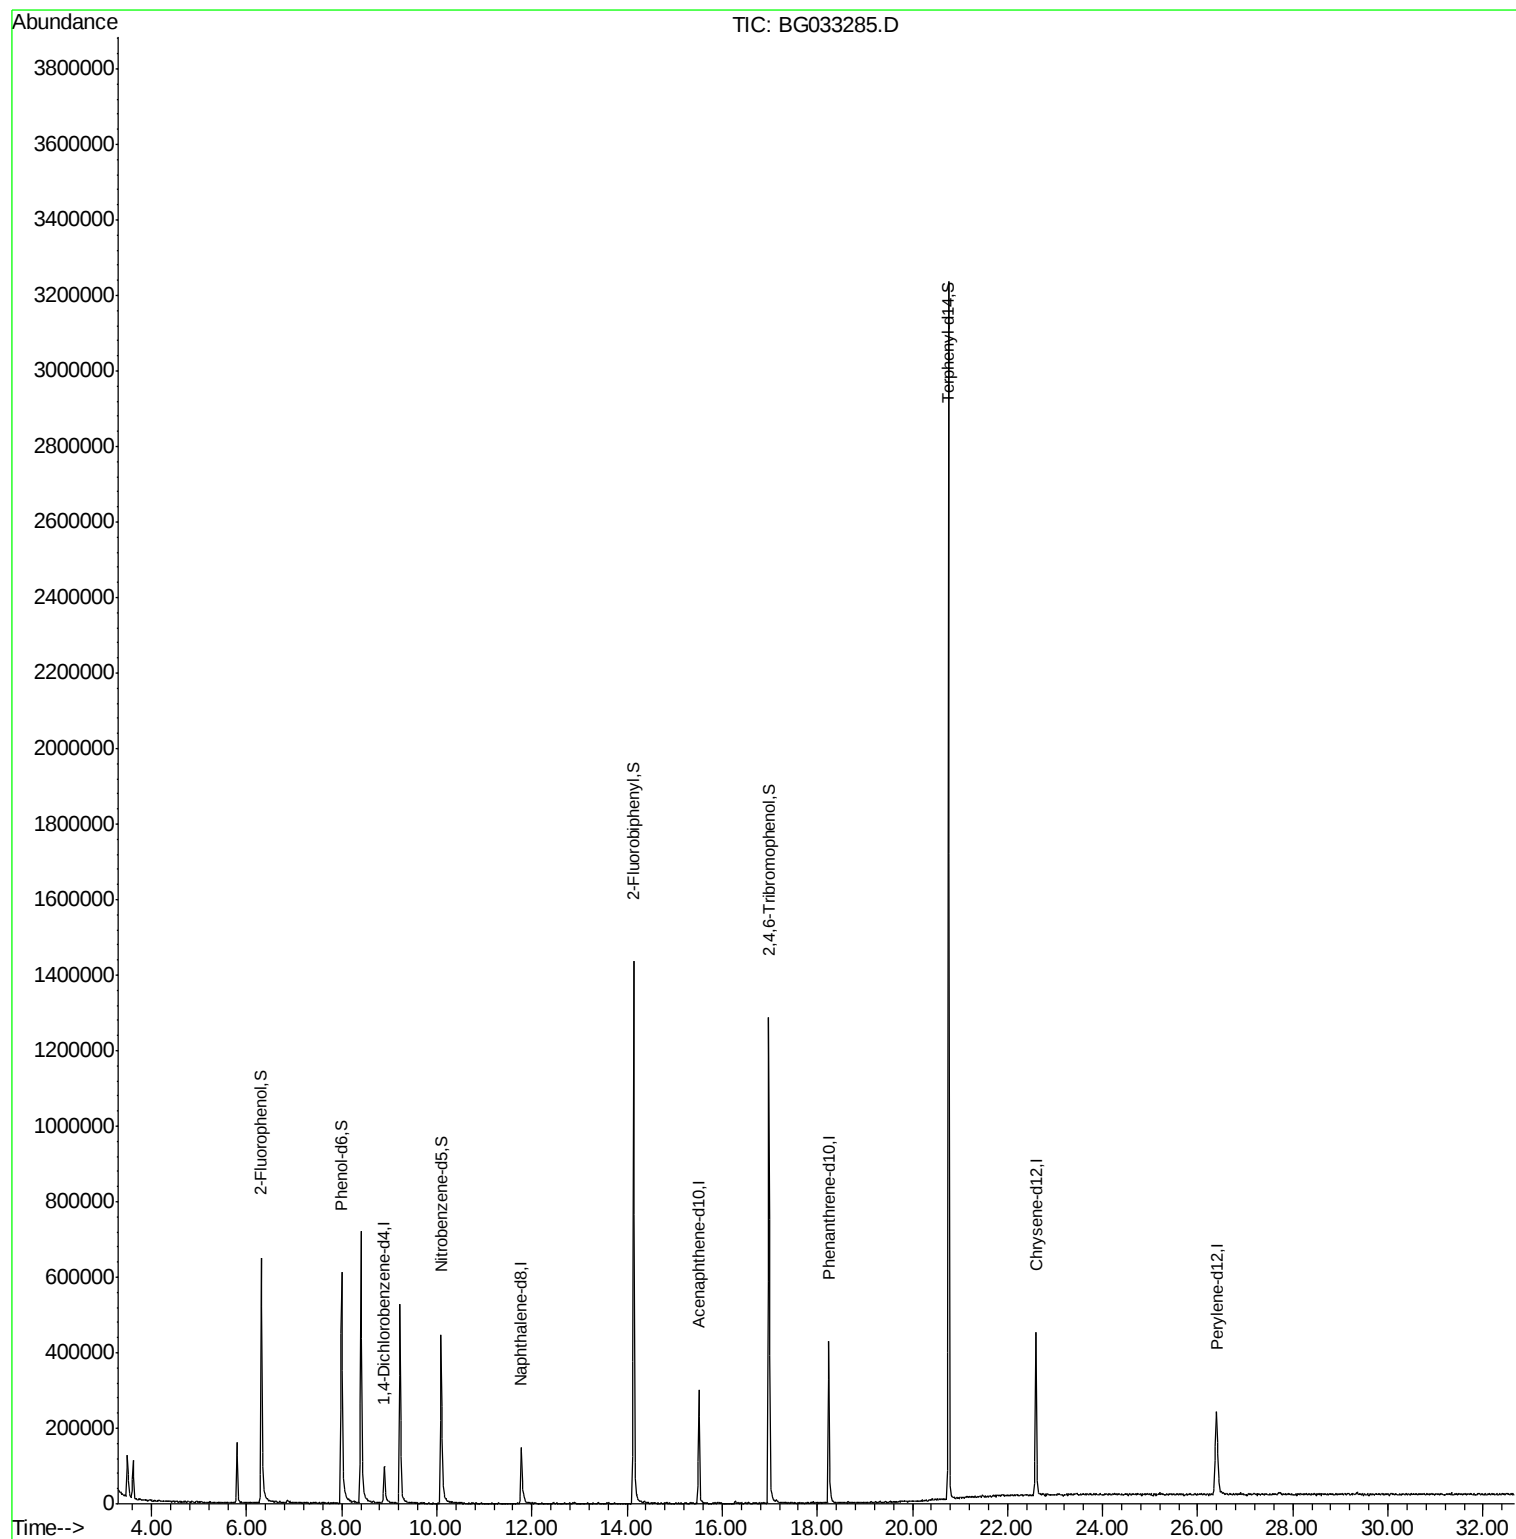






#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.90 min Scan# 954
Delta R.T. -0.00 min
Lab File: BG033285.D
Acq: 21 Mar 2018 3:20

Instrument :
BNA_G
ClientSampleId :
SP




Tot Ion:152 Resp: 35141
Ion Ratio Lower Upper
152 100
150 165.3 126.6 189.8
115 62.9 53.0 79.4

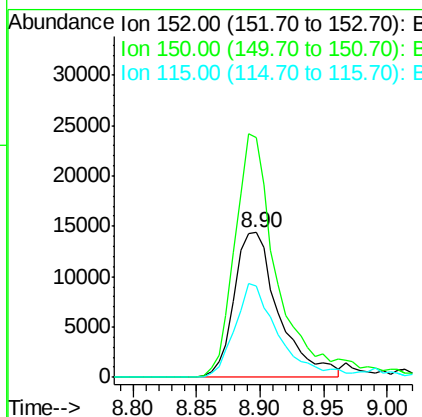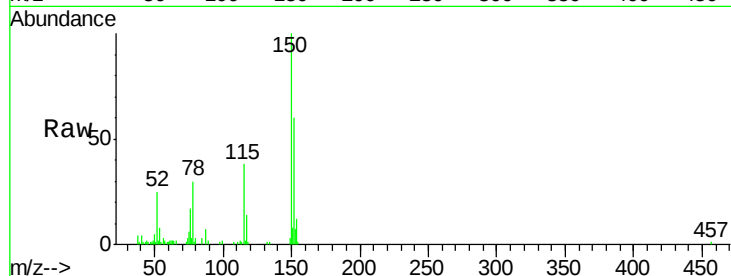


#5

2-Fluorophenol
Concen: 171.335 ng
RT: 6.31 min Scan# 514
Delta R.T. -0.00 min
Lab File: BG033285.D
Acq: 21 Mar 2018 3:20

Tgt Ion:112 Resp: 321093
Ion Ratio Lower Upper
112 100
64 68.8 56.3 84.5
63 39.5 30.1 45.1

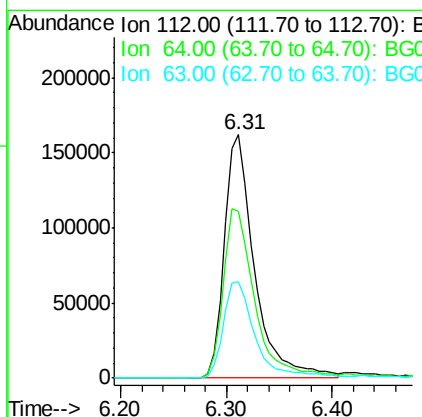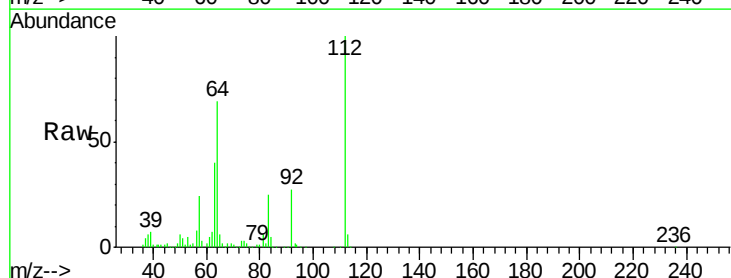

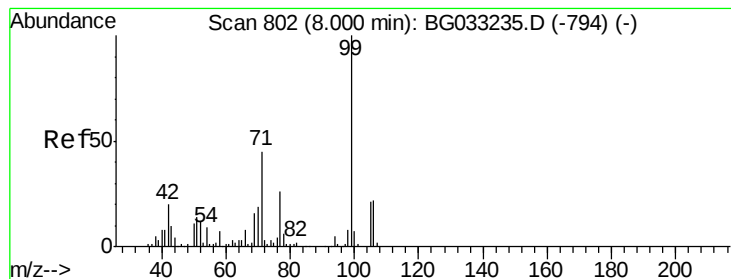

#7

Phenol-d6

Concen: 136.504 ng

RT: 8.00 min Scan# 801

Delta R.T. -0.00 min

Lab File: BG033285.D

Acq: 21 Mar 2018 3:20

Instrument :

BNA_G

ClientSampleId :

SP


Tot Ion: 99 Resp: 439547

Ion Ratio Lower Upper




99 100

42 19.8 14.1 21.1

71 42.2 26.1 39.1#

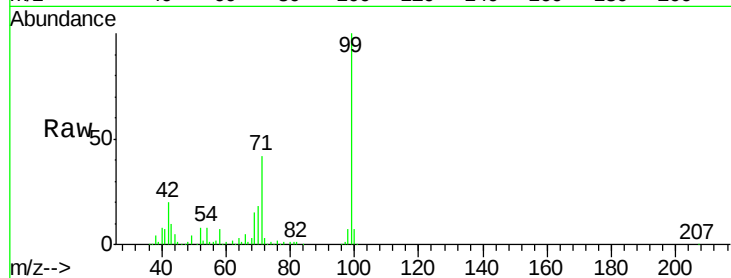

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

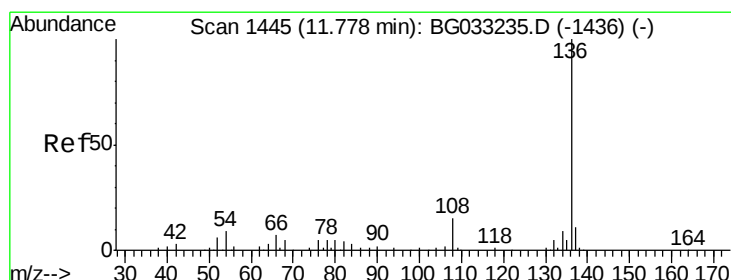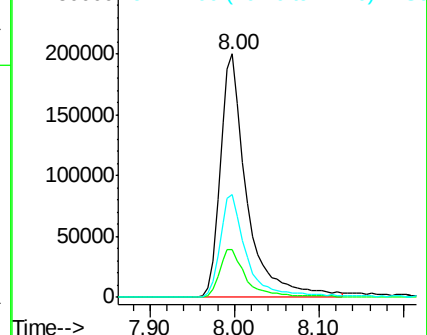

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.78 min Scan# 1444

Delta R.T. -0.01 min

Lab File: BG033285.D

Acq: 21 Mar 2018 3:20

Tgt Ion: 136 Resp: 149649


Ion Ratio Lower Upper

136 100



137 9.7 9.2 13.8


54 10.5 10.3 15.5

68 4.8 4.5 6.7

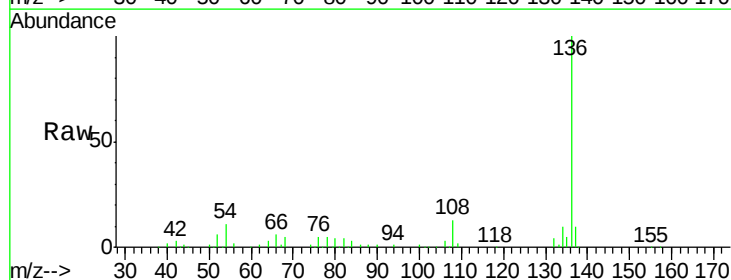

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

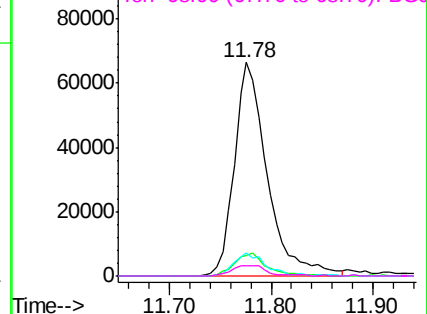

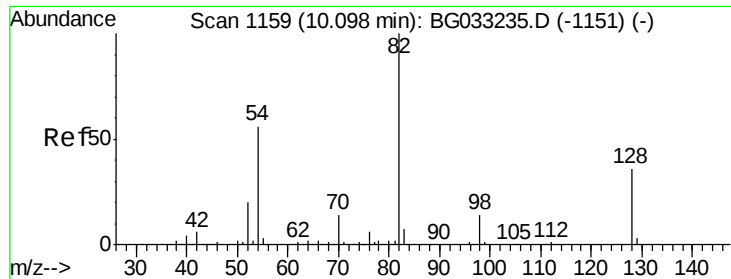

#23

Nitrobenzene-d5

Concen: 108.753 ng

RT: 10.09 min Scan# 1157

Delta R.T. -0.01 min

Lab File: BG033285.D

Acq: 21 Mar 2018 3:20

Instrument :

BNA_G

ClientSampled :

SP


Tot Ion: 82 Resp: 354229

Ion Ratio Lower Upper




82 100

128 35.1 29.7 44.5

54 57.4 43.1 64.7

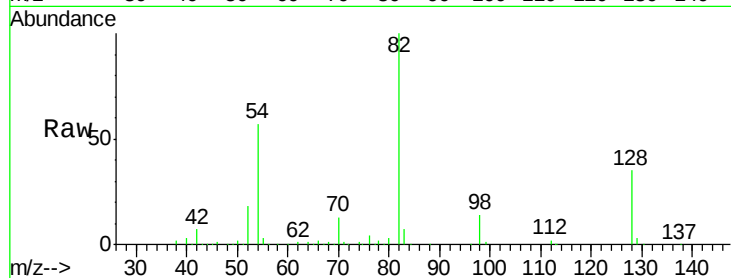

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

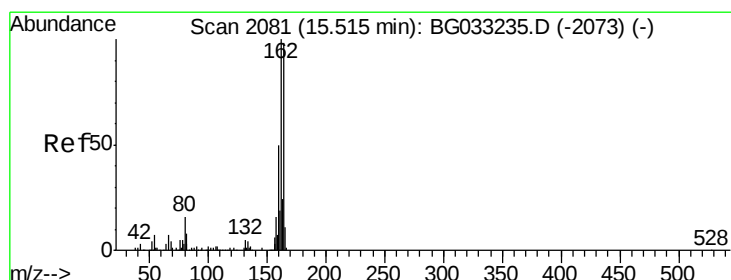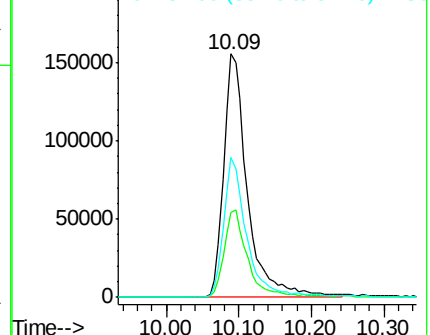

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 15.51 min Scan# 2079

Delta R.T. -0.01 min

Lab File: BG033285.D

Acq: 21 Mar 2018 3:20


Tgt Ion: 164 Resp: 117041

Ion Ratio Lower Upper



164 100


162 101.8 78.8 118.2

160 45.5 35.4 53.0

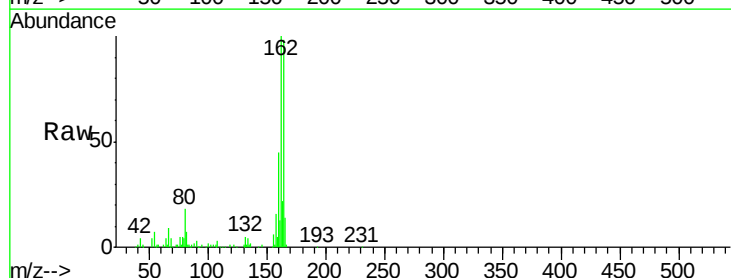

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

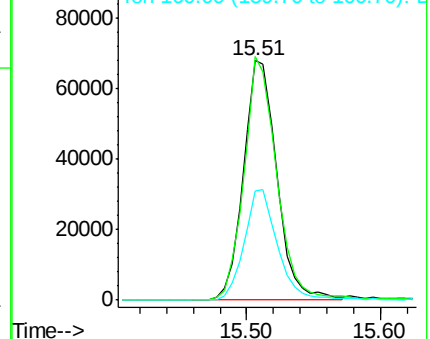


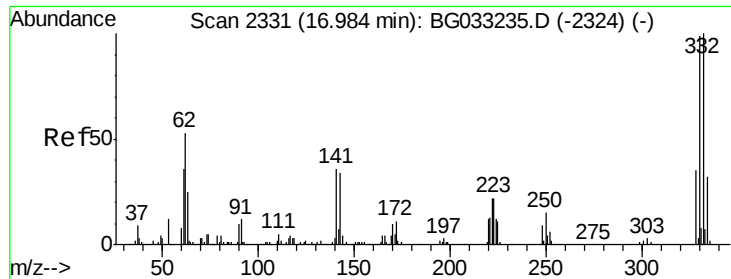

#41
 2,4,6-Tribromophenol
 Concen: 148.202 ng
 RT: 16.98 min Scan# 2330
 Delta R.T. -0.00 min
 Lab File: BG033285.D
 Acq: 21 Mar 2018 3:20

Instrument :
 BNA_G
 ClientSampleId :
 SP

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.5	77.0	115.6
141	36.5	25.2	37.8



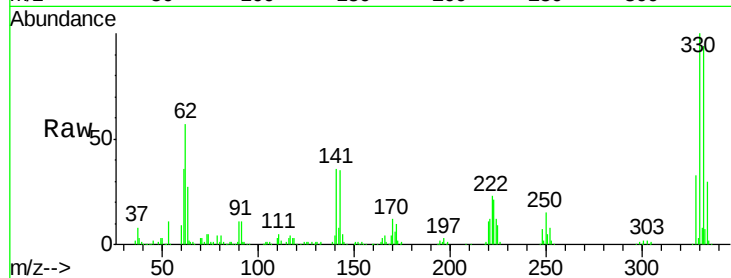


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

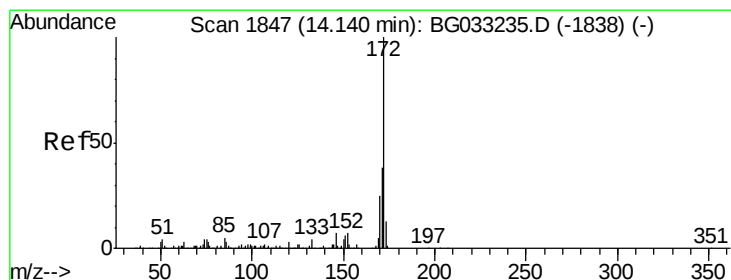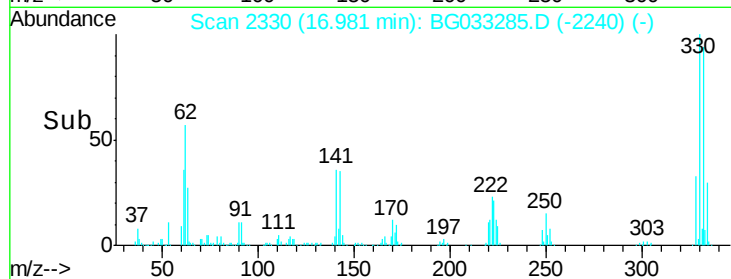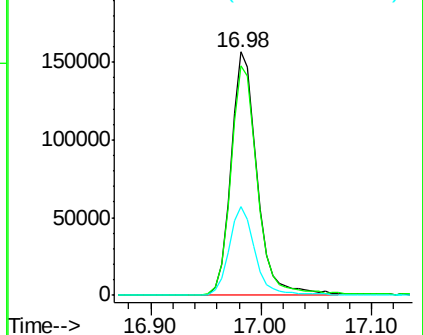

#44
 2-Fluorobiphenyl
 Concen: 102.511 ng
 RT: 14.14 min Scan# 1846
 Delta R.T. -0.00 min
 Lab File: BG033285.D
 Acq: 21 Mar 2018 3:20

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.2	30.0	45.0
170	24.4	19.5	29.3


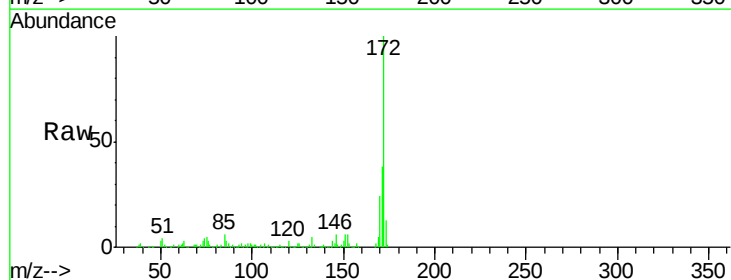



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

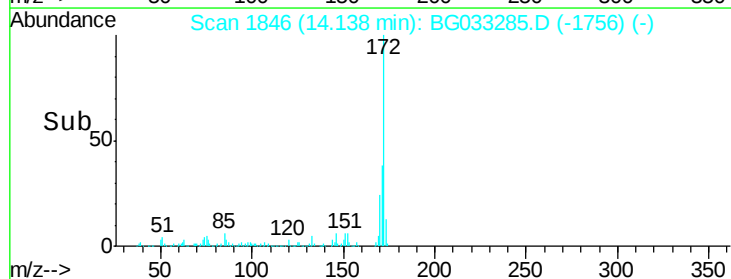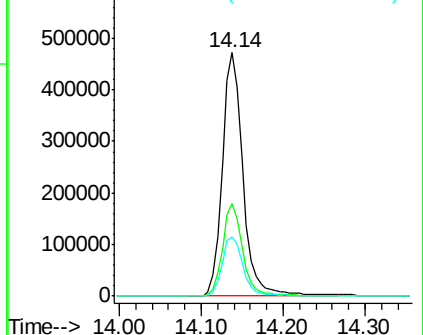



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.24 min Scan# 2544

Delta R.T. -0.00 min

Lab File: BG033285.D

Acq: 21 Mar 2018 3:20

Instrument :

BNA_G

ClientSampleId :

SP


Tot Ion:188 Resp: 320264

Ion Ratio Lower Upper

188 100

94 5.3 6.9 10.3#




80 7.4 7.7 11.5#

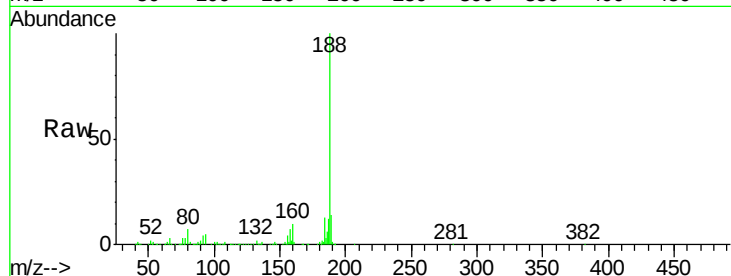

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

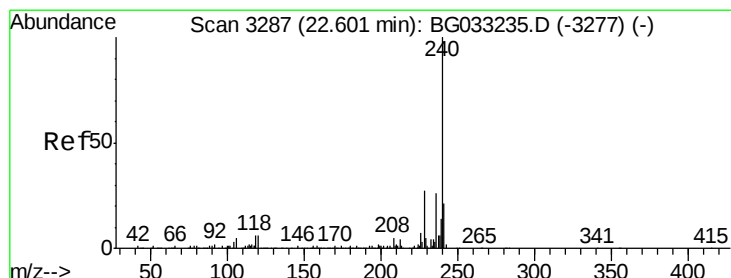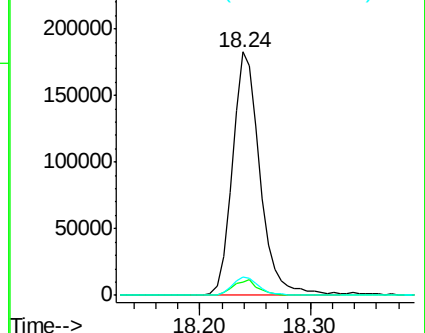

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.60 min Scan# 3286

Delta R.T. -0.00 min

Lab File: BG033285.D

Acq: 21 Mar 2018 3:20


Tgt Ion:240 Resp: 319830

Ion Ratio Lower Upper

240 100

120 6.3 6.8 10.2#



236 26.8 20.9 31.3

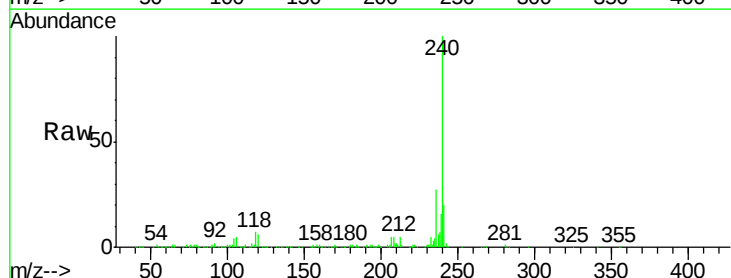


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

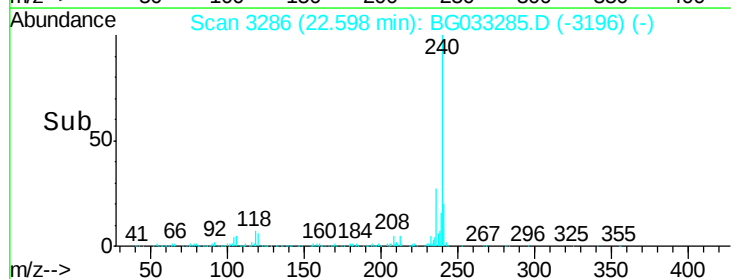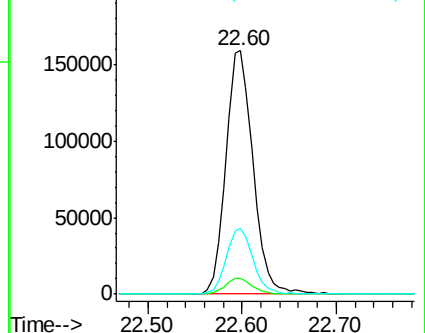

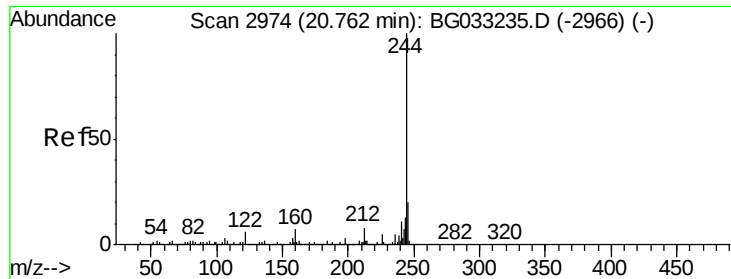

#78

Terphenyl-d14

Concen: 110.862 ng

RT: 20.76 min Scan# 2973

Delta R.T. -0.00 min

Lab File: BG033285.D

Acq: 21 Mar 2018 3:20

Instrument :

BNA_G

ClientSampleId :

SP


Tot Ion:244 Resp: 1657953

Ion Ratio Lower Upper

244 100

212 9.1 5.8 8.8#




122 7.3 7.0 10.4

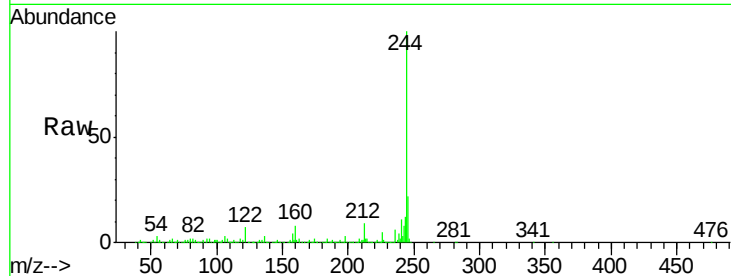

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

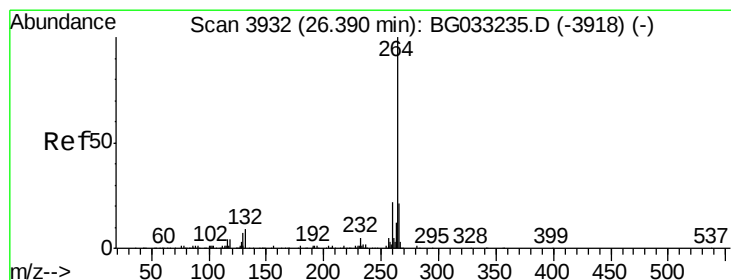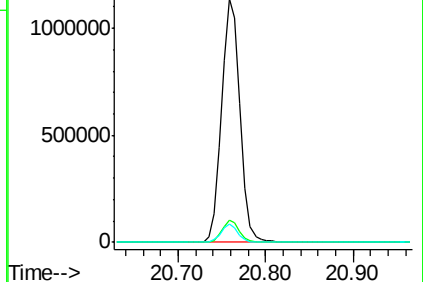

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.39 min Scan# 3932

Delta R.T. -0.00 min

Lab File: BG033285.D

Acq: 21 Mar 2018 3:20


Tgt Ion:264 Resp: 329078

Ion Ratio Lower Upper

264 100

260 24.2 17.4 26.0

265 19.3 17.7 26.5

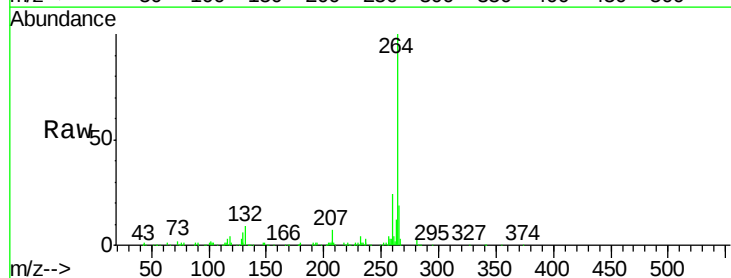

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

