


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG032018\
 Data File : BG033263.D
 Acq On : 20 Mar 2018 8:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 19 16:48:53 2018

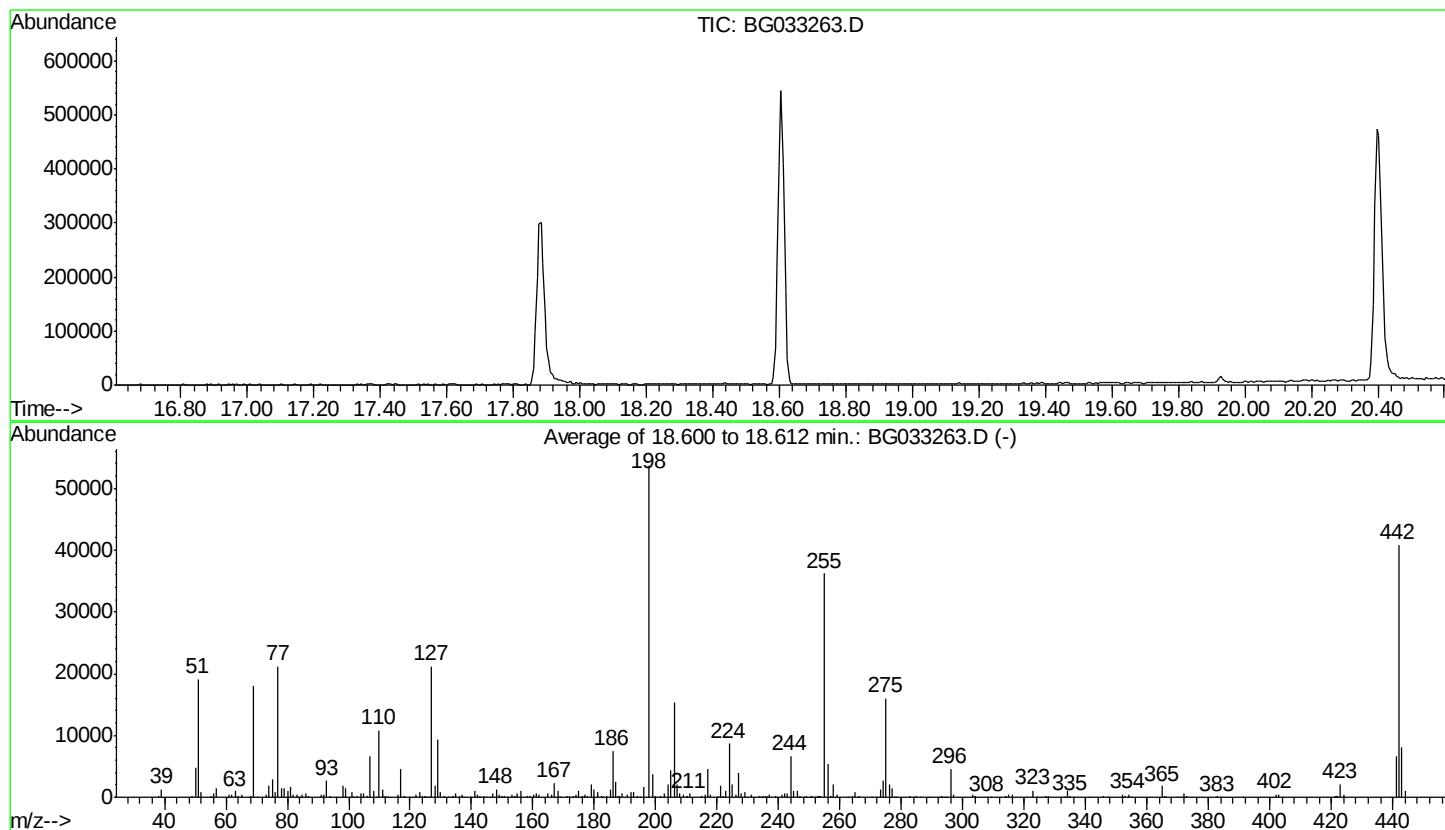

AutoFind: Scans 2606, 2607, 2608; Background Corrected with Scan 2599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	19091	PASS
68	69	0.00	2	0.7	132	PASS
69	198	0.00	100	33.7	18065	PASS
70	69	0.00	2	0.3	61	PASS
127	198	10	80	39.5	21181	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53680	PASS
199	198	5	9	6.9	3707	PASS
275	198	10	60	29.7	15961	PASS
365	198	1	100	3.4	1815	PASS
441	443	0.01	100	81.7	6579	PASS
442	198	50	100	76.2	40906	PASS
443	442	15	24	19.7	8049	PASS