


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG032018\
 Data File : BG033275.D
 Acq On : 20 Mar 2018 21:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 19 16:48:53 2018

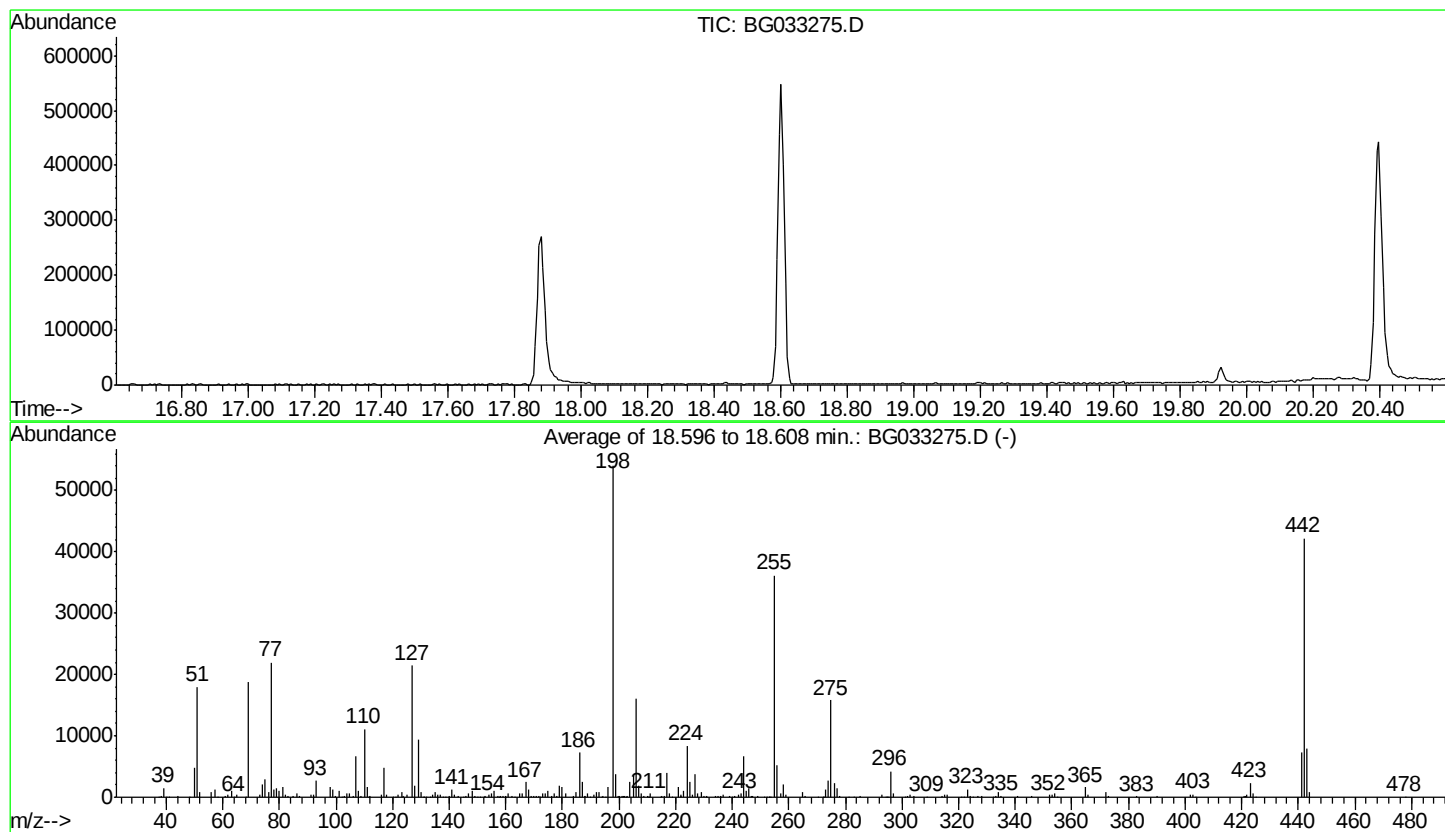

AutoFind: Scans 2605, 2606, 2607; Background Corrected with Scan 2598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	17937	PASS
68	69	0.00	2	0.5	93	PASS
69	198	0.00	100	34.6	18690	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.7	21472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54026	PASS
199	198	5	9	7.1	3847	PASS
275	198	10	60	29.2	15773	PASS
365	198	1	100	3.0	1597	PASS
441	443	0.01	100	91.1	7312	PASS
442	198	50	100	78.1	42189	PASS
443	442	15	24	19.0	8028	PASS