
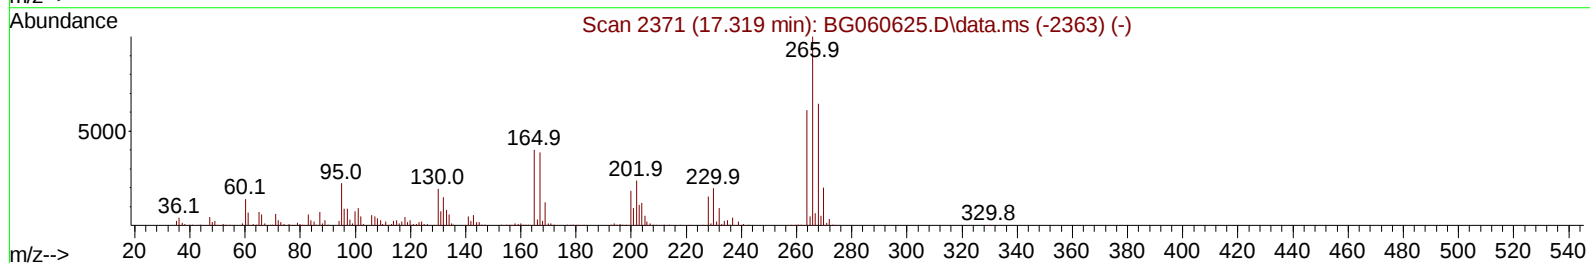
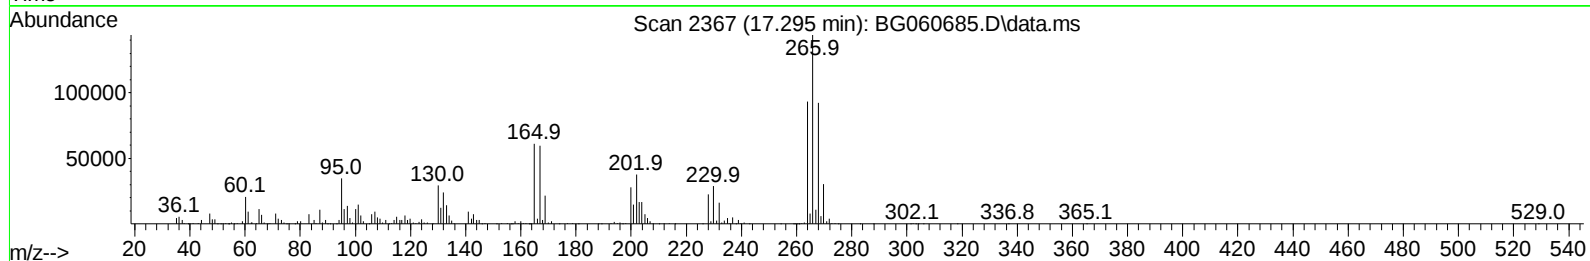


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032024\
Data File : BG060685.D
Acq On : 20 Mar 2024 10:23
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 01:47:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 18 14:26:31 2024
Response via : Initial Calibration

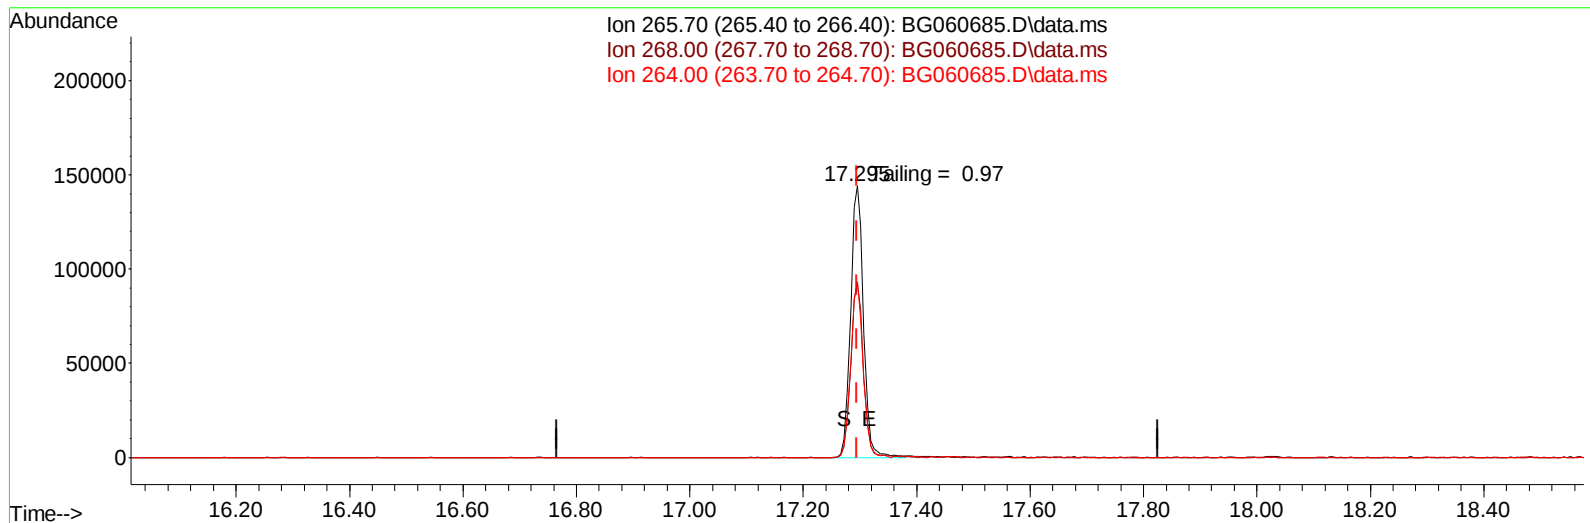

TIC: BG060685.D\data.ms

(70) Pentachlorophenol (C)




17.295min (+ 0.000) 20962.20 ng

response 227408

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.12
264.00	61.10	64.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032024\
Data File : BG060685.D
Acq On : 20 Mar 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 01:47:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 18 14:26:31 2024
Response via : Initial Calibration

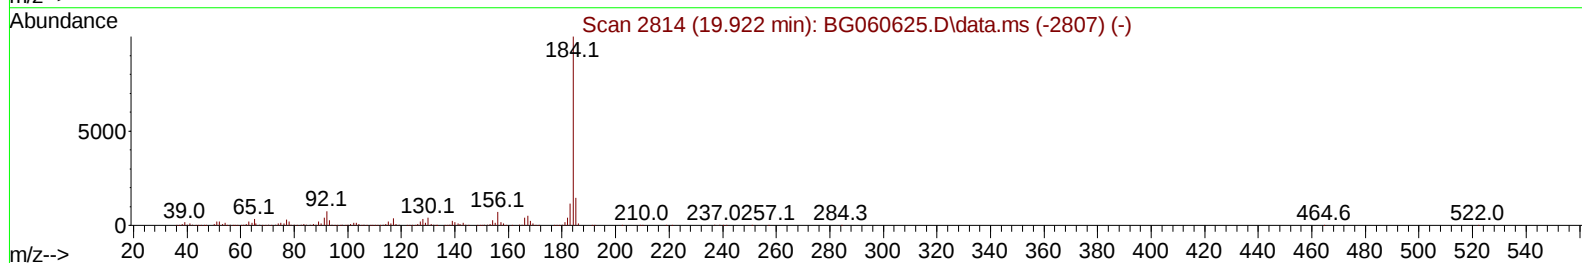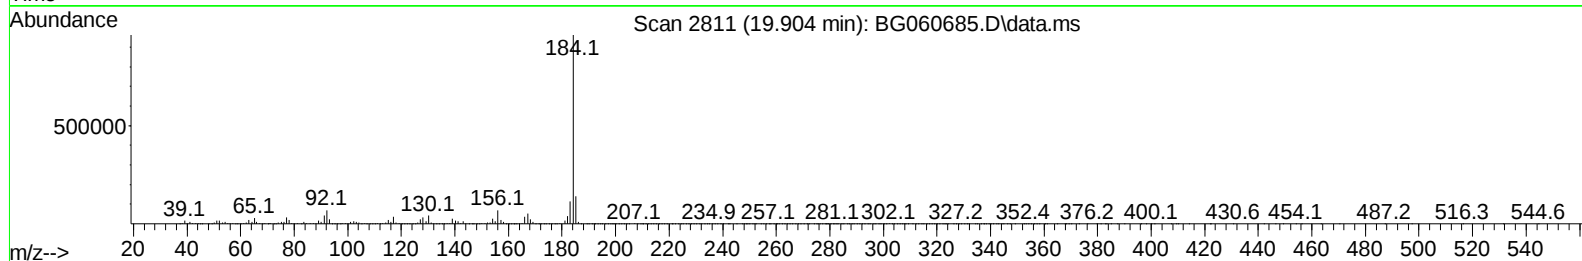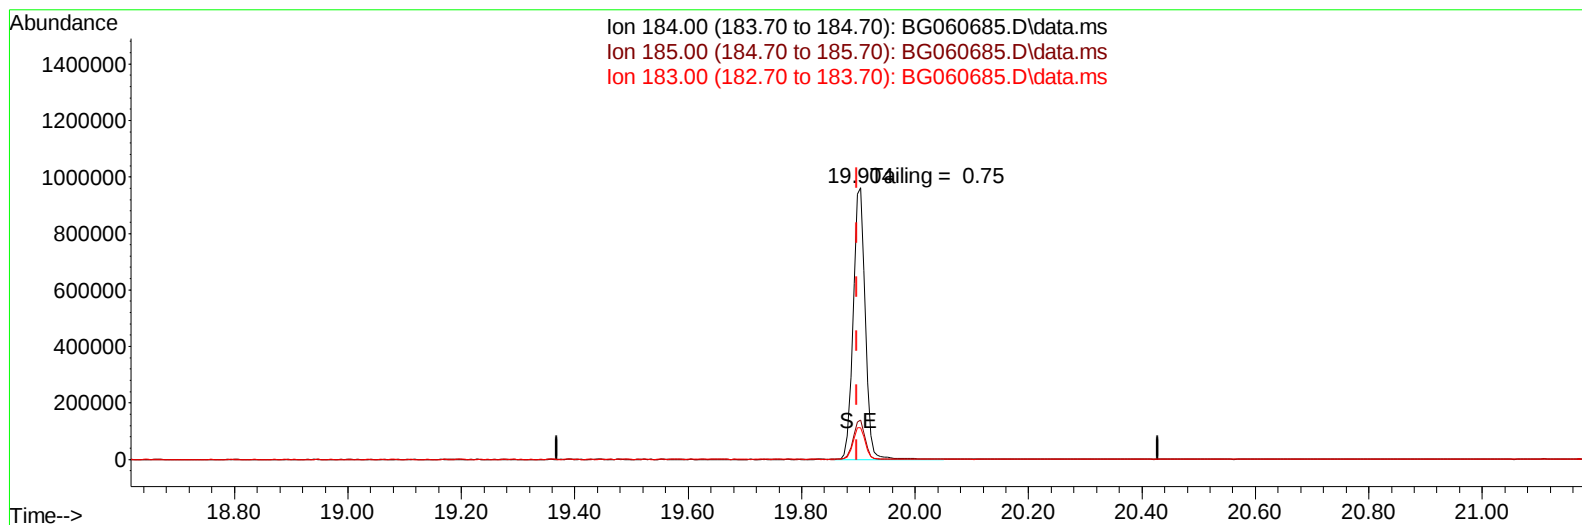

TIC: BG060685.D\data.ms

(77) Benzidine**19.904min (+ 0.006) 241142.46 ng****response 1427395**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.52
183.00	11.50	11.79
0.00	0.00	0.00