


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032024\
Data File : BG060685.D
Acq On : 20 Mar 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 18 14:26:31 2024

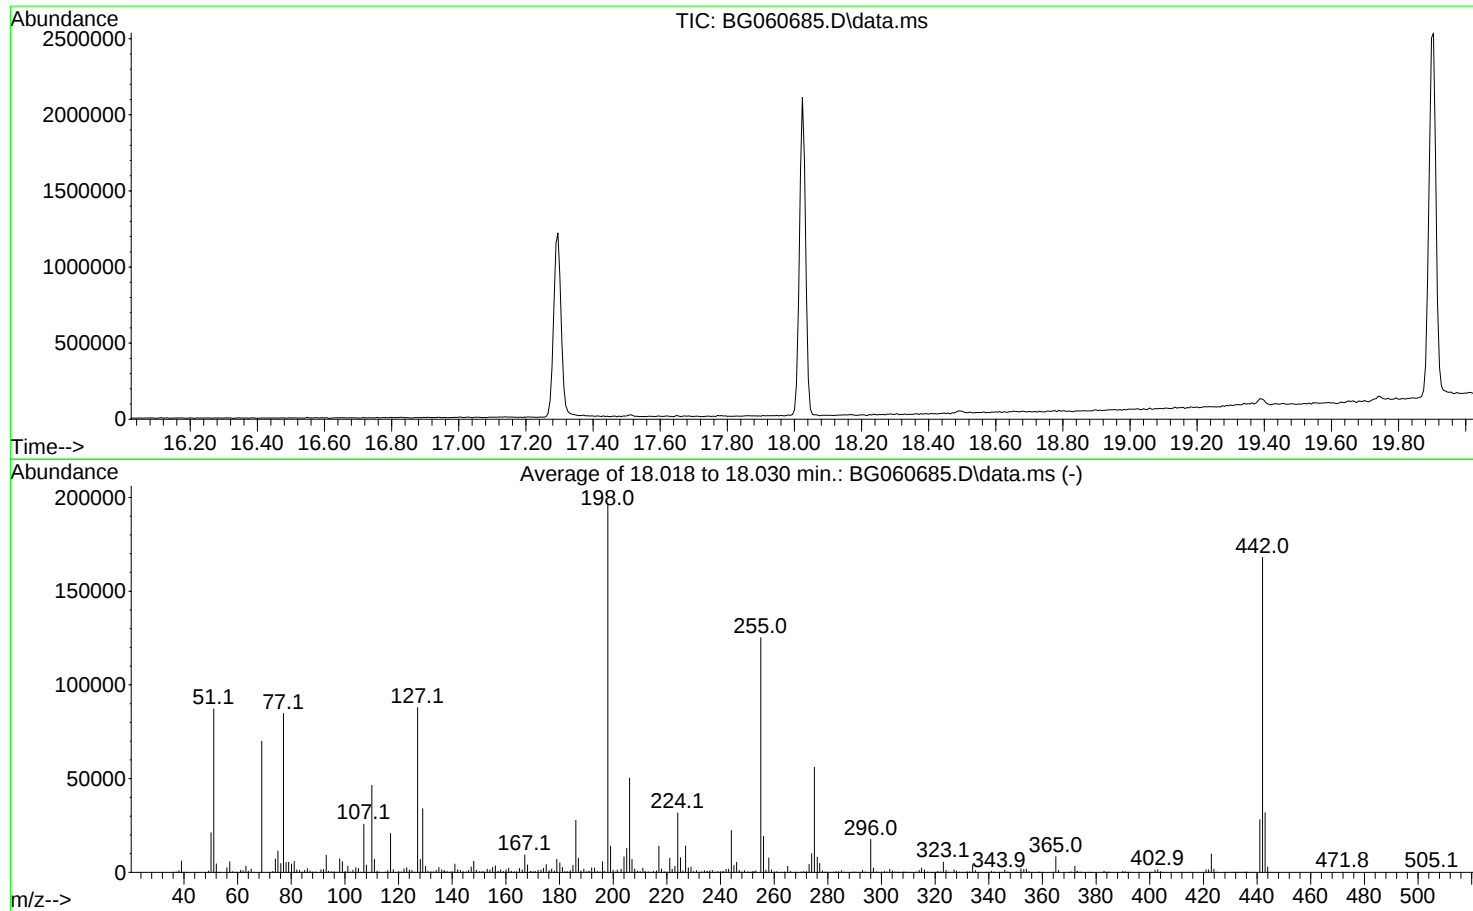




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	87235	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	69875	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.8	87885	PASS
197	198	0.00	2	0.3	512	PASS
198	198	100	100	100.0	196224	PASS
199	198	5	9	7.1	14028	PASS
275	198	10	60	28.6	56043	PASS
365	198	1	100	4.3	8377	PASS
441	198	0.01	100	14.3	28125	PASS
442	442	50	100	100.0	168021	PASS
443	442	15	24	19.0	31877	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032024\
Data File : BG060685.D
Acq On : 20 Mar 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 21 01:47:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 18 14:26:31 2024
Response via : Initial Calibration

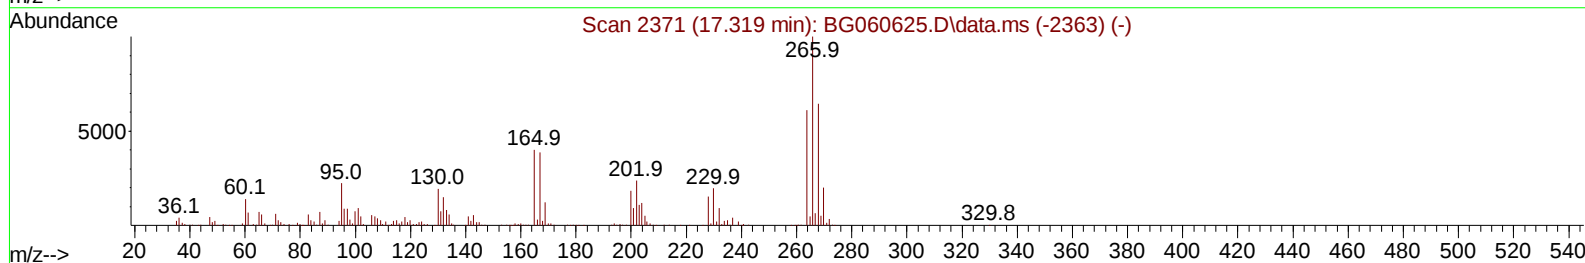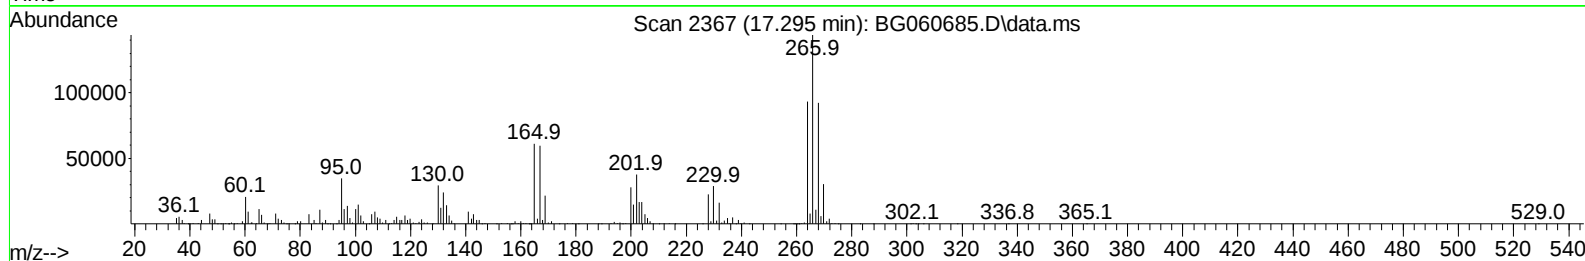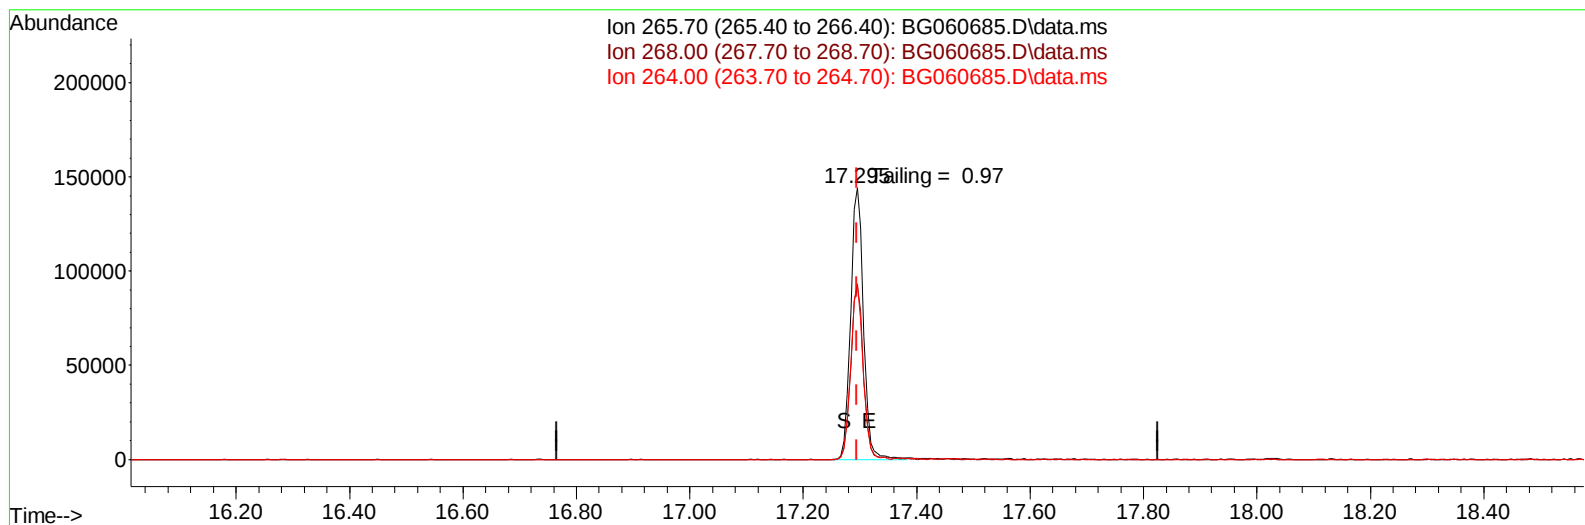

TIC: BG060685.D\data.ms

(70) Pentachlorophenol (C)

17.295min (+ 0.000) 20962.20 ng




response 227408

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	64.12
264.00	61.10	64.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032024\
Data File : BG060685.D
Acq On : 20 Mar 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 21 01:47:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 18 14:26:31 2024
Response via : Initial Calibration

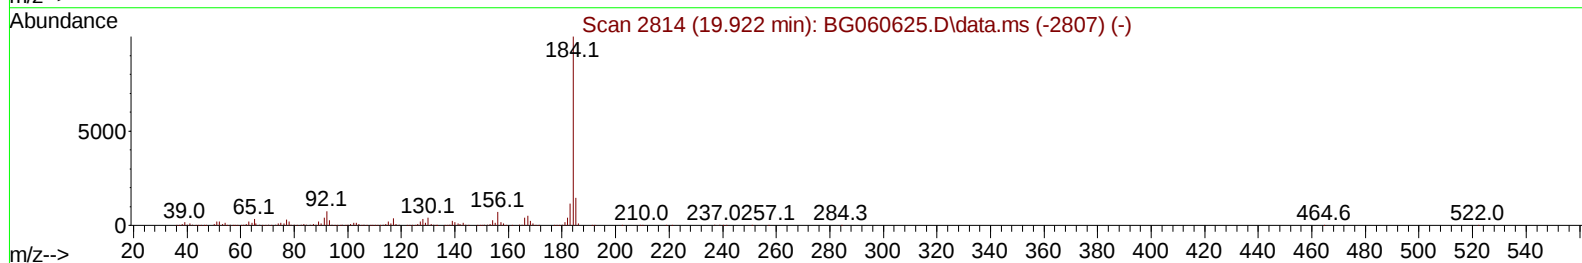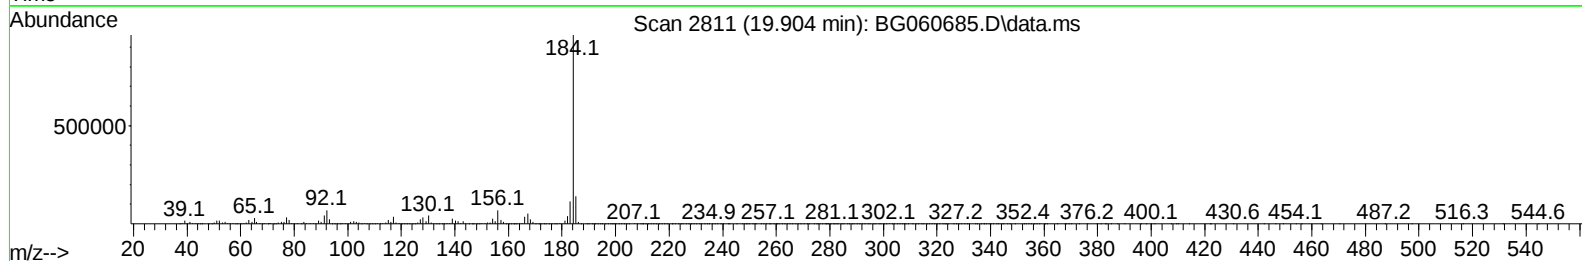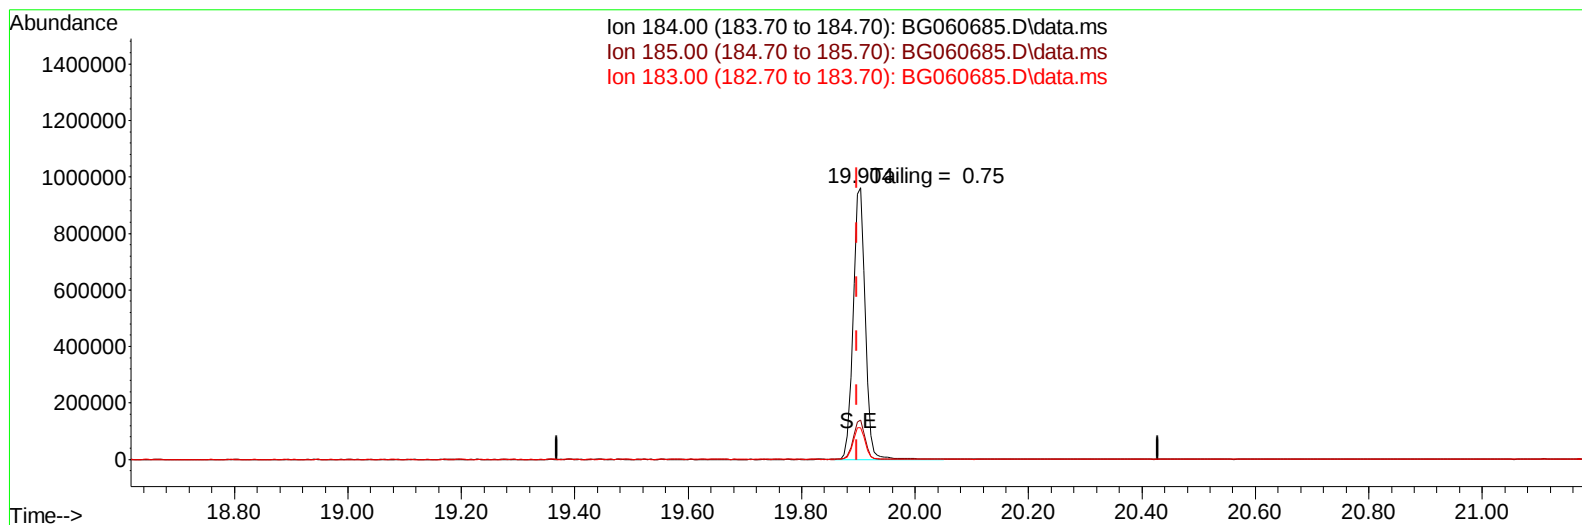

TIC: BG060685.D\data.ms

(77) Benzidine**19.904min (+ 0.006) 241142.46 ng****response 1427395**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.52
183.00	11.50	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/20/2024	BNA_G	<u>BG060685.D</u>
Compound Name	Response	Retention Time
DDT	554074	21.109
DDD	34886	20.656
DDE	0	20.144
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34886	588960	5.92

Instrument :
BNA_G
ClientSampleId :
DFTPP