

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021460.D
 Acq On : 22 Mar 2016 1:40
 Operator : UM/SJ
 Sample : H1835-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T28MSD

Quant Time: Mar 22 02:22:43 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 22 01:42:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	9977	20.00	ng/ul	0.00
18) Naphthalene-d8	10.88	136	47695	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	30229	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.42	188	70962	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	84794	20.00	ng/ul	-0.01
86) Perylene-d12	24.90	264	81576	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	214	0.96	ng/uL	0.00
5) Phenol-d5	7.34	99	6790	7.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	15342	27.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	16292	22.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	15318	18.96	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	11082	30.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.97	143	12119	29.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	19882	27.19	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	1571	1.64	ng/ul	0.00
44) Dimethylphthalate-d6	14.09	166	80434	31.96	ng/ul	0.00
47) Acenaphthylene-d8	14.39	160	97424	31.40	ng/ul	0.00
52) 4-Nitrophenol-d4	15.08	143	2688	6.68	ng/ul	0.02
58) Fluorene-d10	15.67	176	70683	31.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	12223	26.07	ng/ul	0.00
71) Anthracene-d10	17.52	188	117233	33.71	ng/ul	0.00
79) Pyrene-d10	19.80	212	137576	34.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.68	264	144572	38.40	ng/ul	0.00

Target Compounds


						Qvalue
6) Phenol	7.36	94	7134	7.15	ng/ul	91
10) 2-Chlorophenol	7.68	128	16503	22.42	ng/ul	91
15) N-Nitroso-di-n-propylamine	8.87	70	21062	28.82	ng/ul#	97
33) 4-Chloro-3-methylphenol	12.24	107	23306	25.14	ng/ul#	93
50) Acenaphthene	14.75	153	64343	30.35	ng/ul	100
53) 4-Nitrophenol	15.10	109	2855	6.84	ng/ul	87
55) 2,4-Dinitrotoluene	15.05	165	23645	30.22	ng/ul	86
69) Pentachlorophenol	17.09	266	7959	34.42	ng/ul	98
80) Pyrene	19.83	202	170766	33.80	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021460.D
Acq On : 22 Mar 2016 1:40
Operator : UM/SJ
Sample : H1835-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T28MSD

Quant Time: Mar 22 02:22:43 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 22 01:42:49 2016
Response via : Initial Calibration

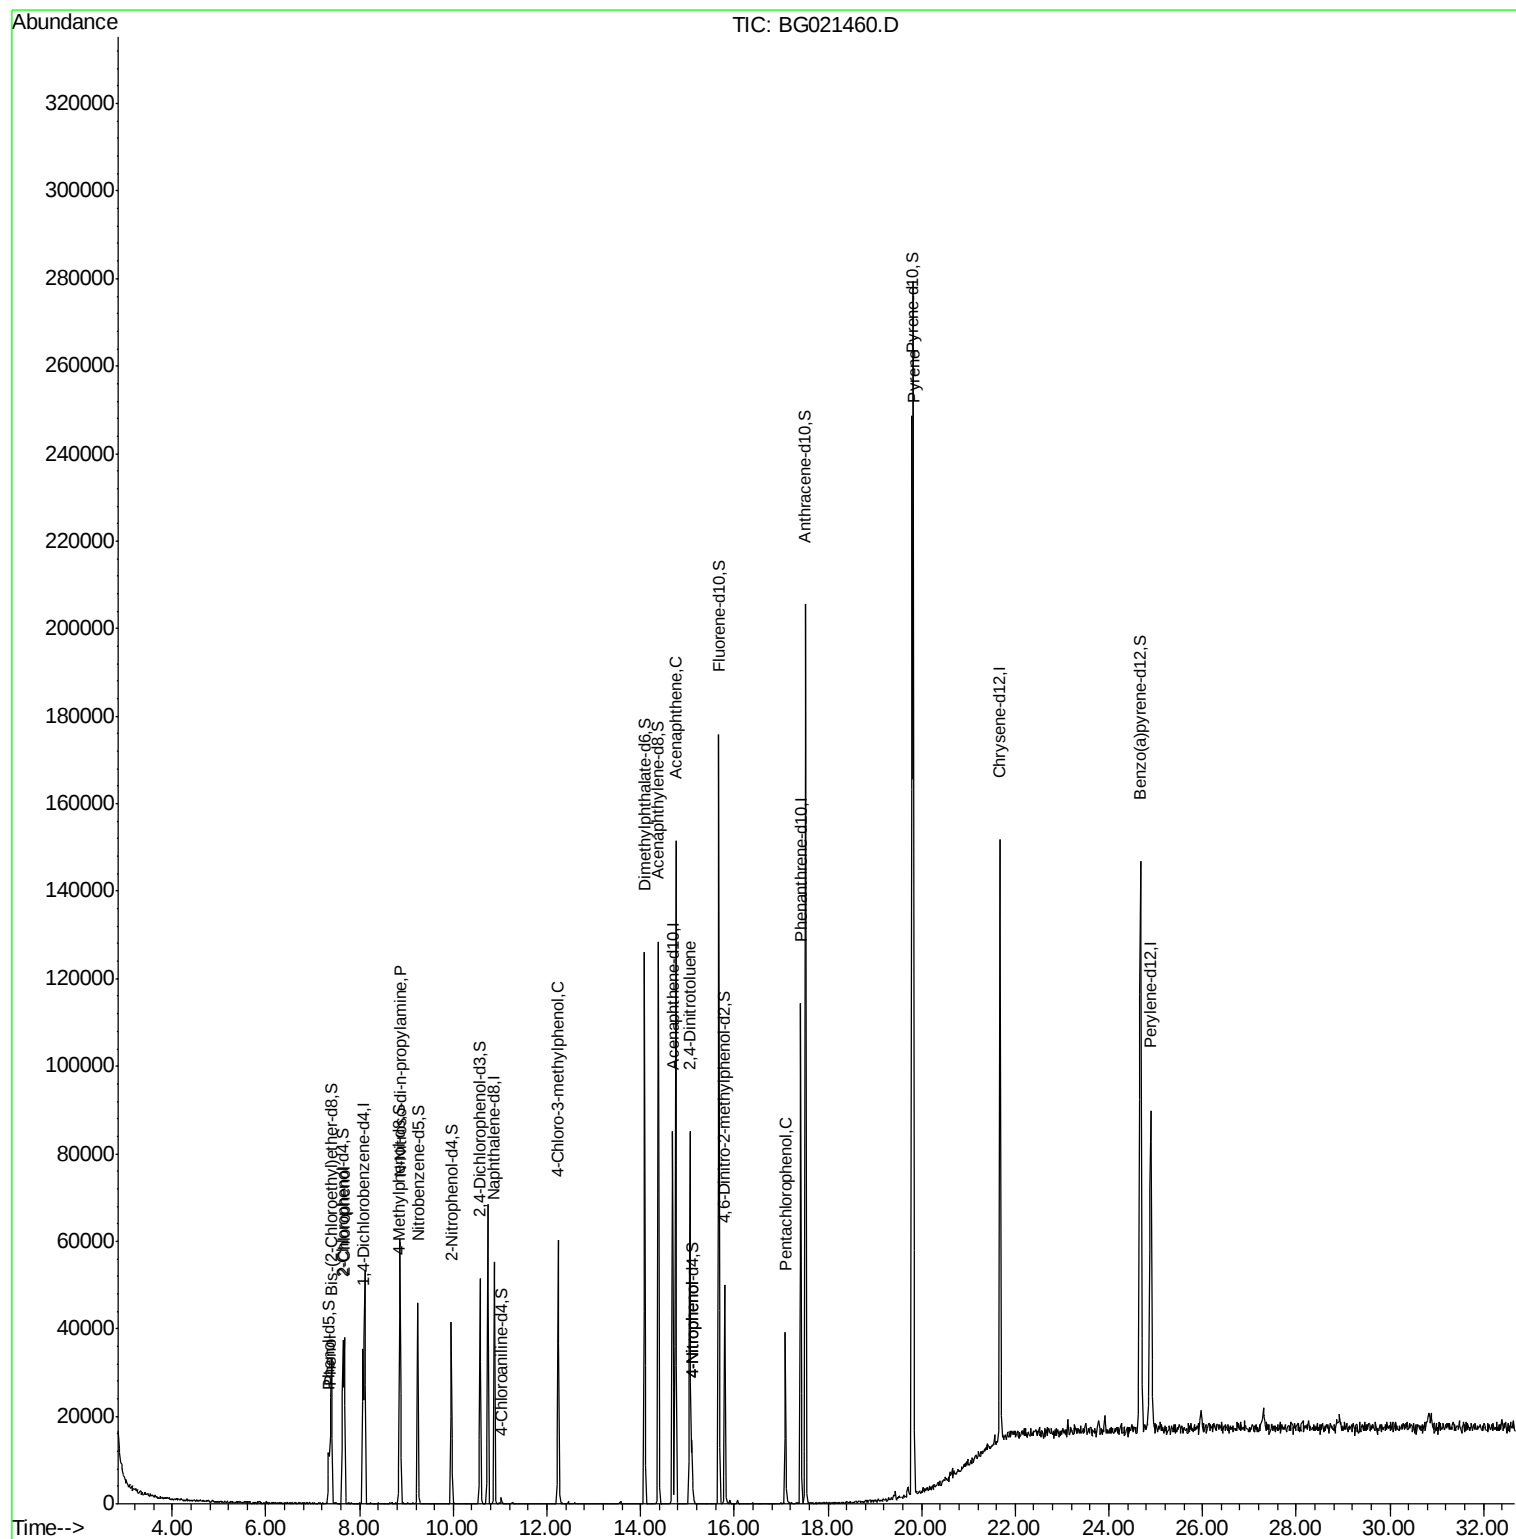

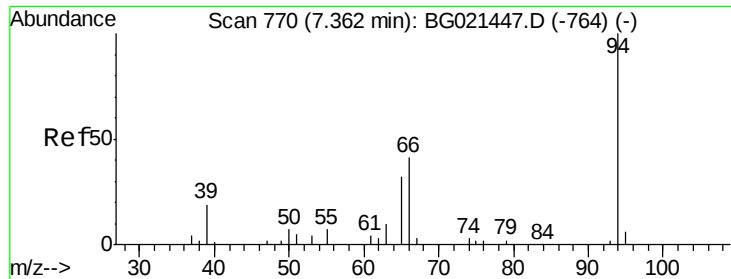

#6

Phenol

Concen: 7.15 ng/ul

RT: 7.36 min Scan# 770

Delta R.T. 0.00 min

Lab File: BG021460.D

Acq: 22 Mar 2016 1:40

Instrument :

BNA_G

ClientSampleId :

A4T28MSD


Tgt Ion: 94 Resp: 7134

Ion Ratio Lower Upper




94 100

65 28.2 26.1 39.1

66 37.6 35.0 52.4

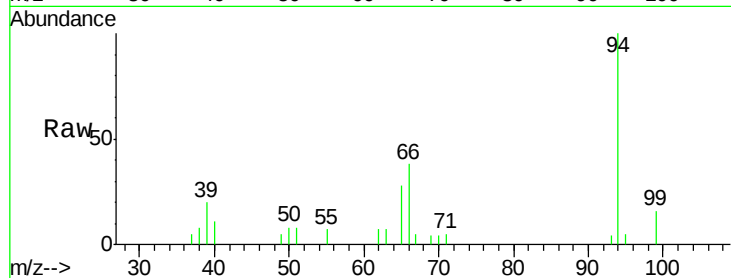

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

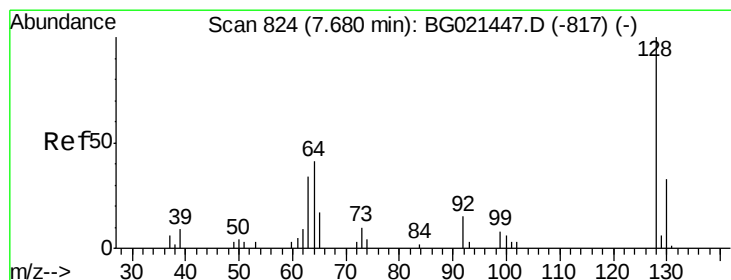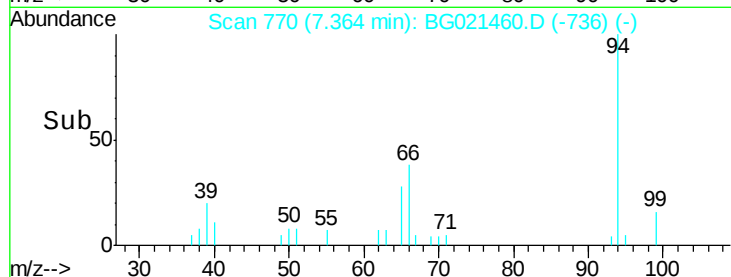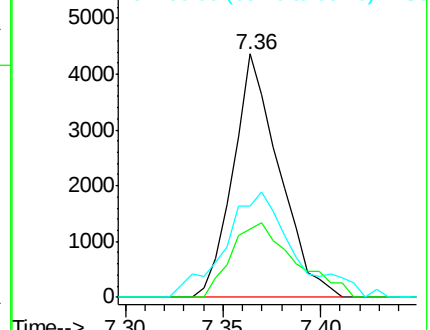

#10

2-Chlorophenol

Concen: 22.42 ng/ul

RT: 7.68 min Scan# 823

Delta R.T. -0.00 min

Lab File: BG021460.D

Acq: 22 Mar 2016 1:40


Tgt Ion: 128 Resp: 16503

Ion Ratio Lower Upper



128 100


64 51.7 47.0 70.6

130 30.4 27.8 41.6

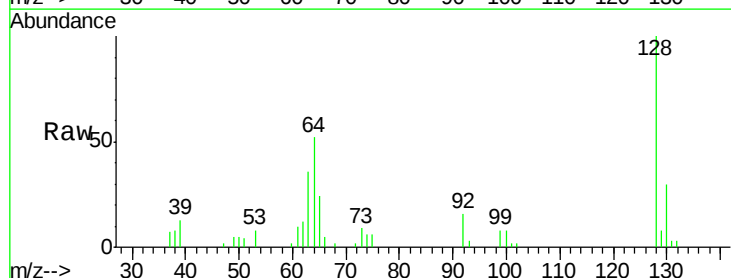

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 130.00 (129.70 to 130.70): E

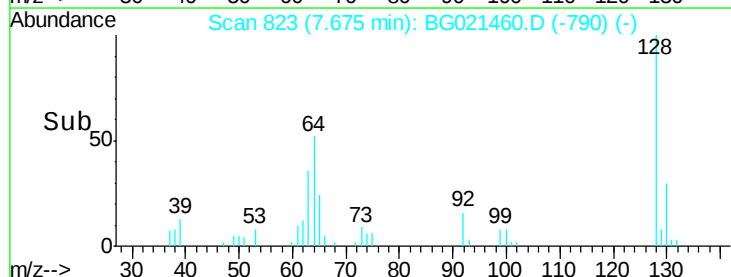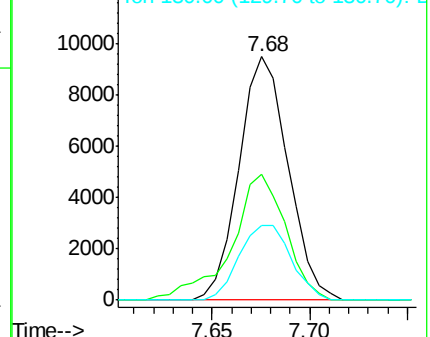


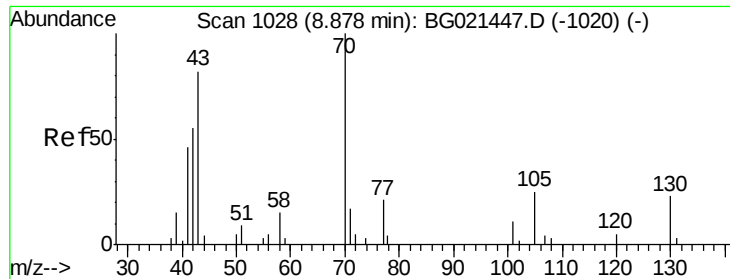




#15
N-Nitroso-di-n-propylamine
Concen: 28.82 ng/ul
RT: 8.87 min Scan# 1027
Delta R.T. -0.00 min
Lab File: BG021460.D
Acq: 22 Mar 2016 1:40

Instrument :
BNA_G
ClientSampleId :
A4T28MSD

Tgt Ion: 70 Resp: 21062
Ion Ratio Lower Upper
70 100
42 54.9 43.4 65.0
101 9.2 6.5 9.7
130 21.0 13.8 20.6#

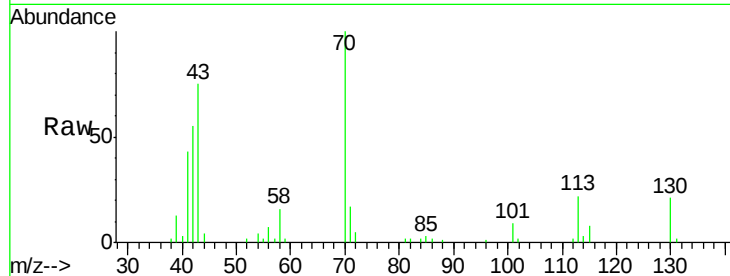


Abundance Ion 70.00 (69.70 to 70.70): BG021447.D (-1020) (-)
Ion 42.00 (41.70 to 42.70): BG021447.D (-1020) (-)
Ion 101.00 (100.70 to 101.70): BG021447.D (-1020) (-)
Ion 130.00 (129.70 to 130.70): BG021447.D (-1020) (-)

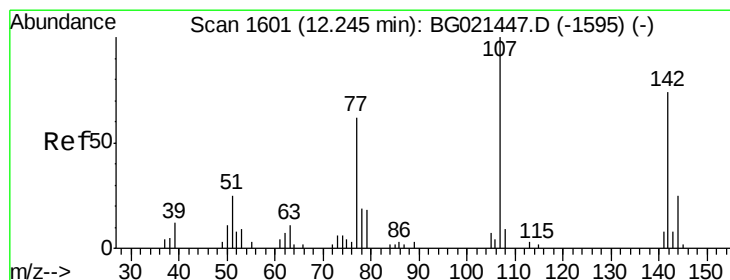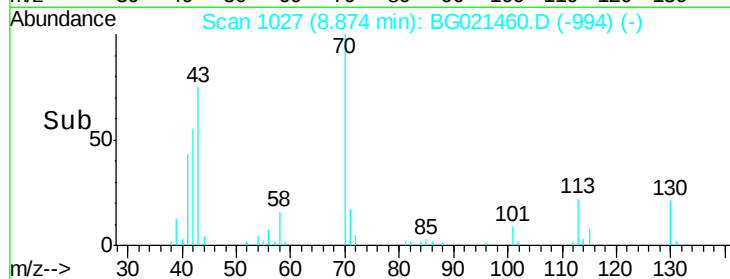
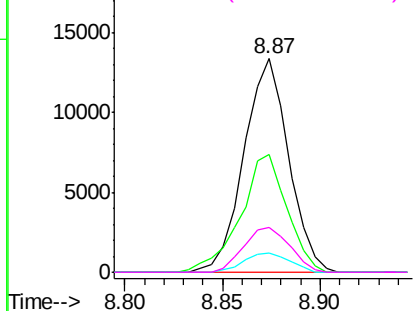



#33
4-Chloro-3-methylphenol
Concen: 25.14 ng/ul
RT: 12.24 min Scan# 1600
Delta R.T. -0.00 min
Lab File: BG021460.D
Acq: 22 Mar 2016 1:40

Tgt Ion: 107 Resp: 23306
Ion Ratio Lower Upper
107 100
144 26.1 17.2 25.8#
142 69.6 52.0 78.0

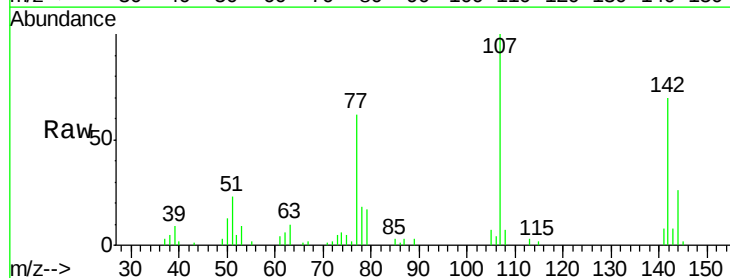

Abundance Ion 107.00 (106.70 to 107.70): BG021447.D (-1595) (-)
Ion 144.00 (143.70 to 144.70): BG021447.D (-1595) (-)
Ion 142.00 (141.70 to 142.70): BG021447.D (-1595) (-)

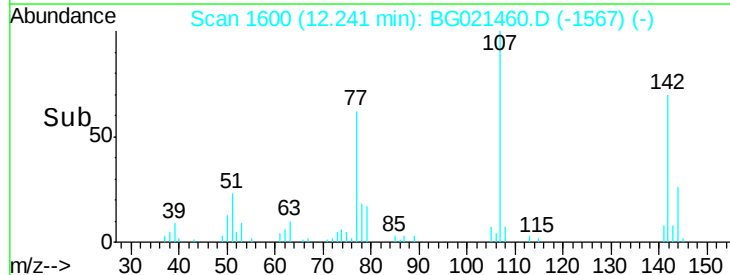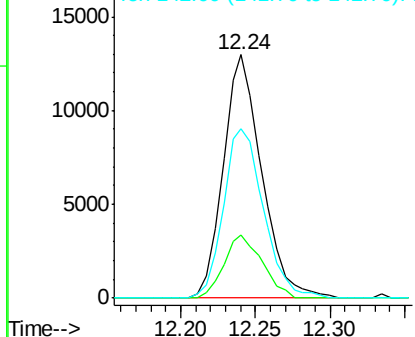

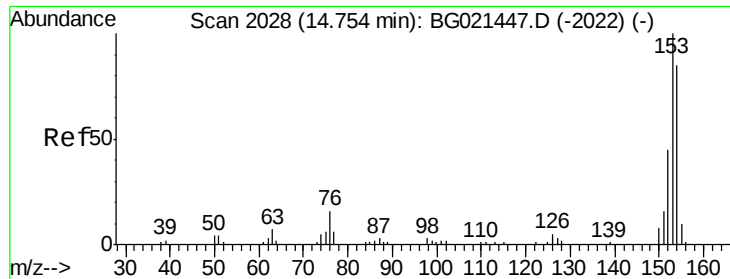

#50

Acenaphthene

Concen: 30.35 ng/ul

RT: 14.75 min Scan# 2027

Delta R.T. -0.00 min

Lab File: BG021460.D

Acq: 22 Mar 2016 1:40

Instrument :

BNA_G

ClientSampleId :

A4T28MSD


Tgt Ion:153 Resp: 64343

Ion Ratio Lower Upper

153 100

152 45.3 36.5 54.7




154 84.3 67.3 100.9

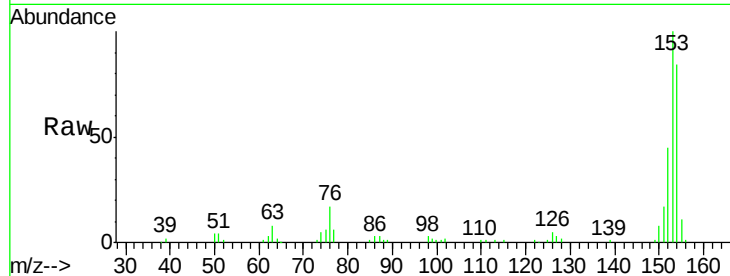

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

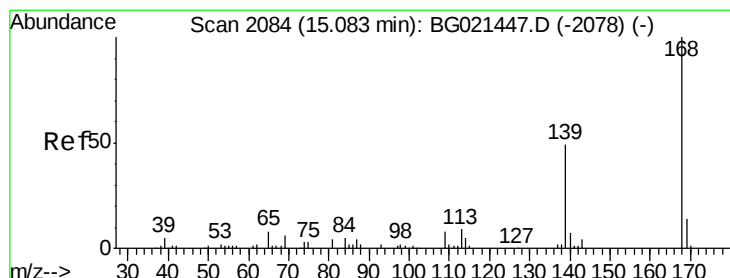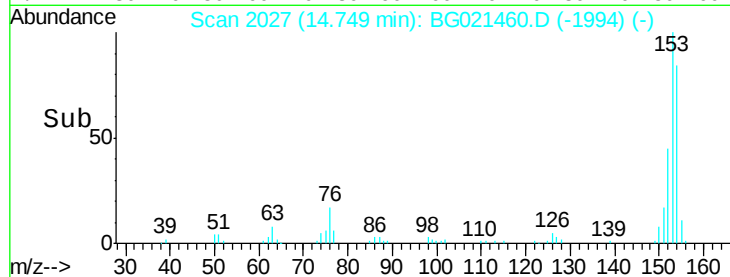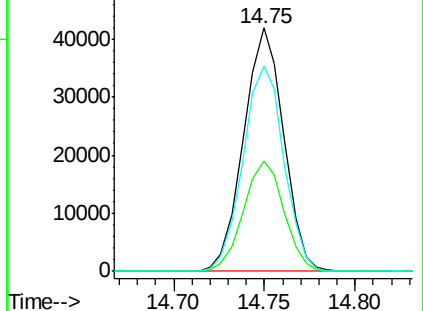

#53

4-Nitrophenol

Concen: 6.84 ng/ul

RT: 15.10 min Scan# 2086

Delta R.T. 0.01 min

Lab File: BG021460.D

Acq: 22 Mar 2016 1:40


Tgt Ion:109 Resp: 2855

Ion Ratio Lower Upper

109 100

139 104.3 75.9 113.9



65 141.8 99.8 149.8

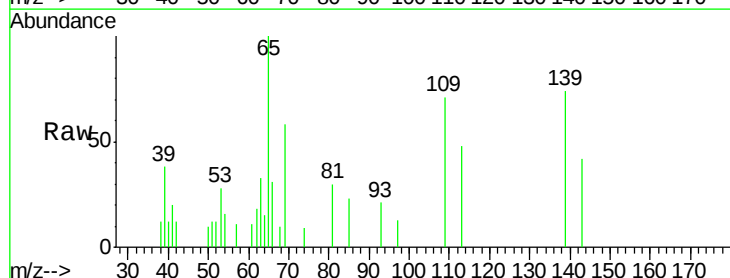


Abundance Ion 109.00 (108.70 to 109.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BGC



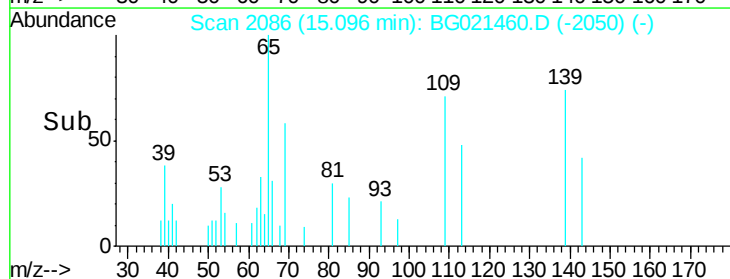
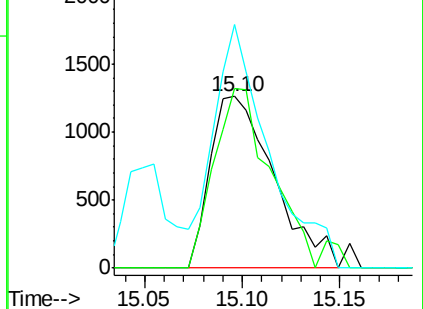


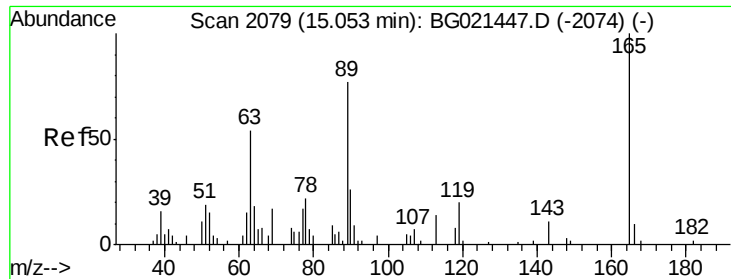

#55
 2,4-Dinitrotoluene
 Concen: 30.22 ng/ul
 RT: 15.05 min Scan# 2079
 Delta R.T. 0.00 min
 Lab File: BG021460.D
 Acq: 22 Mar 2016 1:40




Instrument :
 BNA_G
 ClientSampleId :
 A4T28MSD


Tgt Ion	Ratio	Lower	Upper
165	100		
63	49.1	48.1	72.1
182	2.6	2.2	3.2

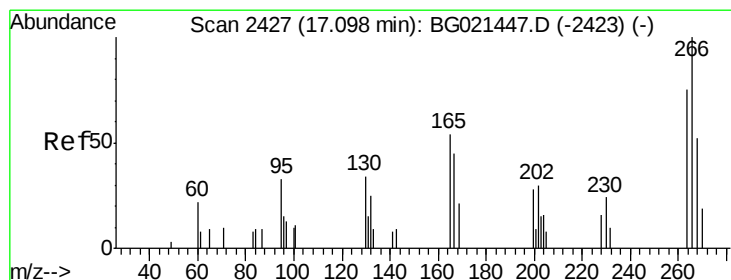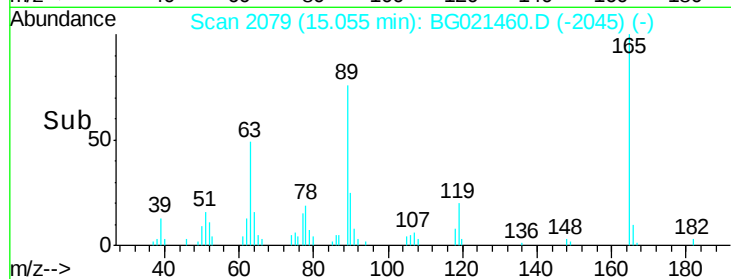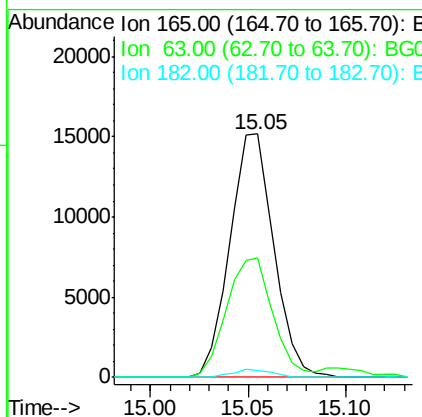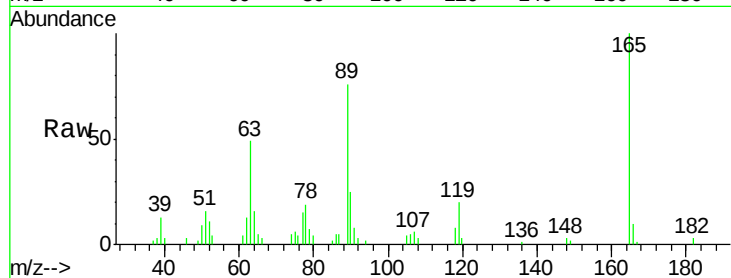

#69
 Pentachlorophenol
 Concen: 34.42 ng/ul
 RT: 17.09 min Scan# 2426
 Delta R.T. -0.00 min
 Lab File: BG021460.D
 Acq: 22 Mar 2016 1:40

Tgt Ion	Ratio	Lower	Upper
266	100		
264	69.7	56.7	85.1
268	65.6	50.6	76.0

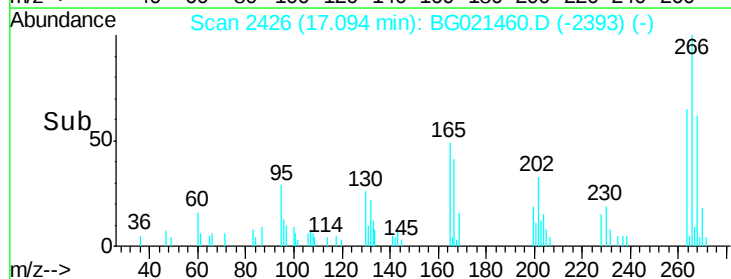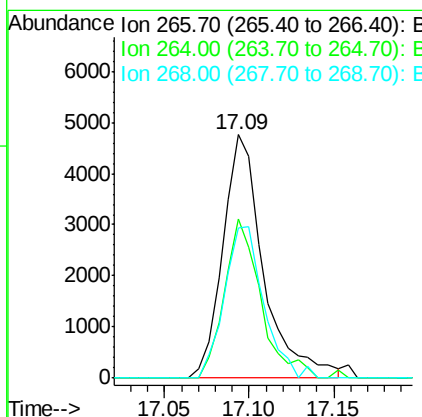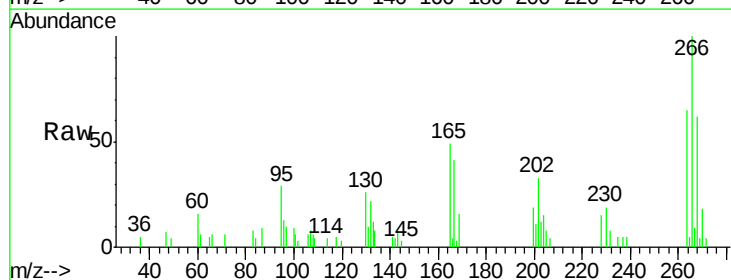

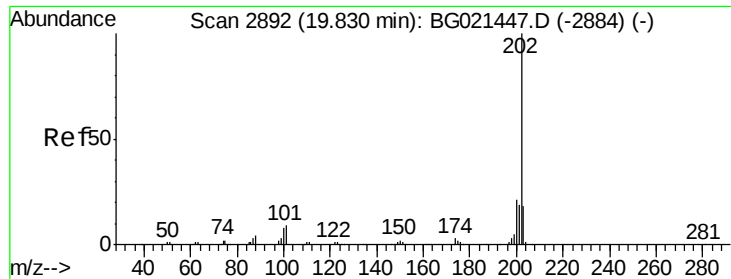

#80
 Pyrene
 Concen: 33.80 ng/ul
 RT: 19.83 min Scan# 2891
 Delta R.T. -0.00 min
 Lab File: BG021460.D
 Acq: 22 Mar 2016 1:40

Instrument :
 BNA_G
 ClientSampleId :
 A4T28MSD

Tgt Ion: 202 Resp: 170766
 Ion Ratio Lower Upper
 202 100
 101 9.6 9.8 14.8#
 100 9.1 9.3 13.9#

