

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021451.D
 Acq On : 21 Mar 2016 19:46
 Operator : UM/SJ
 Sample : H1835-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.309	78	80	82	rVB3	552	423	0.11%	0.014%
2	3.385	90	93	96	rVB2	476	514	0.13%	0.017%
3	3.579	123	126	134	rVB3	1648	3115	0.81%	0.102%
4	3.638	134	136	138	rBV3	422	433	0.11%	0.014%
5	3.820	163	167	168	rBV2	397	499	0.13%	0.016%
6	3.944	186	188	190	rBV2	515	430	0.11%	0.014%
7	4.231	235	237	242	rVB2	424	468	0.12%	0.015%
8	4.361	255	259	261	rVB3	544	703	0.18%	0.023%
9	4.631	302	305	308	rBV2	384	566	0.15%	0.019%
10	4.713	317	319	321	rVV2	812	652	0.17%	0.021%
11	4.772	324	329	331	rVB2	407	583	0.15%	0.019%
12	5.430	439	441	444	rBV2	470	559	0.15%	0.018%
13	5.542	457	460	463	rVB2	495	623	0.16%	0.020%
14	5.600	467	470	473	rVB	306	386	0.10%	0.013%
15	5.647	473	478	481	rBV	619	658	0.17%	0.022%
16	5.700	485	487	488	rBV	405	403	0.10%	0.013%
17	5.835	505	510	511	rVV2	419	673	0.18%	0.022%
18	6.164	563	566	569	rBB	496	703	0.18%	0.023%
19	6.200	569	572	574	rBV	486	663	0.17%	0.022%
20	6.405	604	607	608	rBB	429	399	0.10%	0.013%
21	6.423	608	610	612	rBB	474	410	0.11%	0.013%
22	6.482	619	620	623	rBV	388	386	0.10%	0.013%
23	7.287	756	757	762	rBV	405	585	0.15%	0.019%
24	7.345	762	767	771	rVV	7909	13071	3.40%	0.428%
25	7.398	771	776	784	rVB	33121	55309	14.40%	1.810%
26	7.557	802	803	808	rBB	350	409	0.11%	0.013%
27	7.645	812	818	829	rBB	33664	57506	14.97%	1.882%
28	8.074	885	891	901	rBB	35166	59286	15.44%	1.940%
29	8.850	1018	1023	1030	rBB	27103	45424	11.83%	1.486%
30	9.243	1083	1090	1099	rBB	46312	79500	20.70%	2.602%
31	9.966	1206	1213	1220	rBV2	41162	71568	18.64%	2.342%
32	10.571	1310	1316	1327	rBB	49167	87050	22.67%	2.849%
33	10.882	1362	1369	1376	rBV	54603	95103	24.76%	3.112%
34	11.029	1391	1394	1399	rBB	861	1030	0.27%	0.034%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021451.D
 Acq On : 21 Mar 2016 19:46
 Operator : UM/SJ
 Sample : H1835-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	12.457	1634	1637	1640	rBB	690	778	0.20%	0.025%
36	14.090	1909	1915	1921	rBV	118765	164394	42.81%	5.380%
37	14.384	1958	1965	1972	rBV	122303	191539	49.88%	6.268%
38	14.684	2010	2016	2024	rBB2	81872	130130	33.89%	4.258%
39	15.089	2081	2085	2093	rBB2	5991	9417	2.45%	0.308%
40	15.677	2178	2185	2192	rBB	172471	253913	66.12%	8.309%
41	15.794	2200	2205	2215	rBV	48089	76697	19.97%	2.510%
42	15.912	2222	2225	2228	rBB	988	1221	0.32%	0.040%
43	17.210	2445	2446	2450	rBB	392	429	0.11%	0.014%
44	17.422	2476	2482	2491	rBB	98842	150281	39.13%	4.918%
45	17.522	2493	2499	2509	rBV	202361	306105	79.71%	10.017%
46	17.921	2560	2567	2568	rBV2	376	737	0.19%	0.024%
47	18.004	2578	2581	2586	rBV	391	843	0.22%	0.028%
48	18.244	2620	2622	2624	rBV	401	398	0.10%	0.013%
49	18.315	2632	2634	2638	rVB	431	528	0.14%	0.017%
50	18.438	2652	2655	2658	rBV	676	777	0.20%	0.025%
51	18.479	2658	2662	2663	rVV	665	504	0.13%	0.016%
52	18.497	2663	2665	2668	rVV2	563	475	0.12%	0.016%
53	18.609	2681	2684	2686	rBV	436	414	0.11%	0.014%
54	18.662	2692	2693	2696	rBV2	394	407	0.11%	0.013%
55	18.908	2729	2735	2736	rBV2	408	552	0.14%	0.018%
56	19.108	2766	2769	2773	rBV2	467	730	0.19%	0.024%
57	19.226	2785	2789	2790	rBV2	518	443	0.12%	0.014%
58	19.237	2790	2791	2794	rVV2	731	409	0.11%	0.013%
59	19.314	2803	2804	2807	rBV2	524	515	0.13%	0.017%
60	19.367	2809	2813	2817	rVB2	679	989	0.26%	0.032%
61	19.443	2822	2826	2829	rVB2	1673	2432	0.63%	0.080%
62	19.543	2840	2843	2844	rBV2	429	523	0.14%	0.017%
63	19.584	2848	2850	2854	rBV2	409	542	0.14%	0.018%
64	19.613	2854	2855	2858	rBV2	544	624	0.16%	0.020%
65	19.643	2858	2860	2865	rVB3	516	673	0.18%	0.022%
66	19.690	2865	2868	2871	rBV2	2115	2122	0.55%	0.069%
67	19.801	2880	2887	2896	rBV2	263168	380636	99.12%	12.456%
68	19.866	2896	2898	2900	rBV	682	574	0.15%	0.019%
69	19.884	2900	2901	2902	rBV	907	489	0.13%	0.016%
70	20.001	2919	2921	2922	rBV2	798	439	0.11%	0.014%
71	20.019	2922	2924	2926	rVV2	742	668	0.17%	0.022%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021451.D
 Acq On : 21 Mar 2016 19:46
 Operator : UM/SJ
 Sample : H1835-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	20.095	2935	2937	2938	rBV	1184	653	0.17%	0.021%
73	20.119	2938	2941	2943	rBV3	1257	1239	0.32%	0.041%
74	20.142	2943	2945	2947	rBV2	788	835	0.22%	0.027%
75	20.219	2955	2958	2959	rBV3	1119	1007	0.26%	0.033%
76	20.236	2959	2961	2962	rVV2	693	419	0.11%	0.014%
77	20.301	2968	2972	2974	rBV4	937	1213	0.32%	0.040%
78	20.383	2982	2986	2987	rBV4	842	1163	0.30%	0.038%
79	20.442	2995	2996	3000	rVB3	1540	1026	0.27%	0.034%
80	20.765	3049	3051	3052	rBV2	1287	957	0.25%	0.031%
81	20.824	3058	3061	3063	rVB3	1521	1419	0.37%	0.046%
82	20.877	3068	3070	3072	rBV2	1702	1658	0.43%	0.054%
83	21.682	3201	3207	3214	rVB	125548	205329	53.47%	6.719%
84	24.684	3708	3718	3730	rVB	145264	384028	100.00%	12.567%
85	24.901	3748	3755	3768	rVB2	71709	189580	49.37%	6.204%
86	30.912	4776	4778	4779	rBV	2717	1841	0.48%	0.060%


Sum of corrected areas: 3055804

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021451.D
Acq On : 21 Mar 2016 19:46
Operator : UM/SJ
Sample : H1835-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T13

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

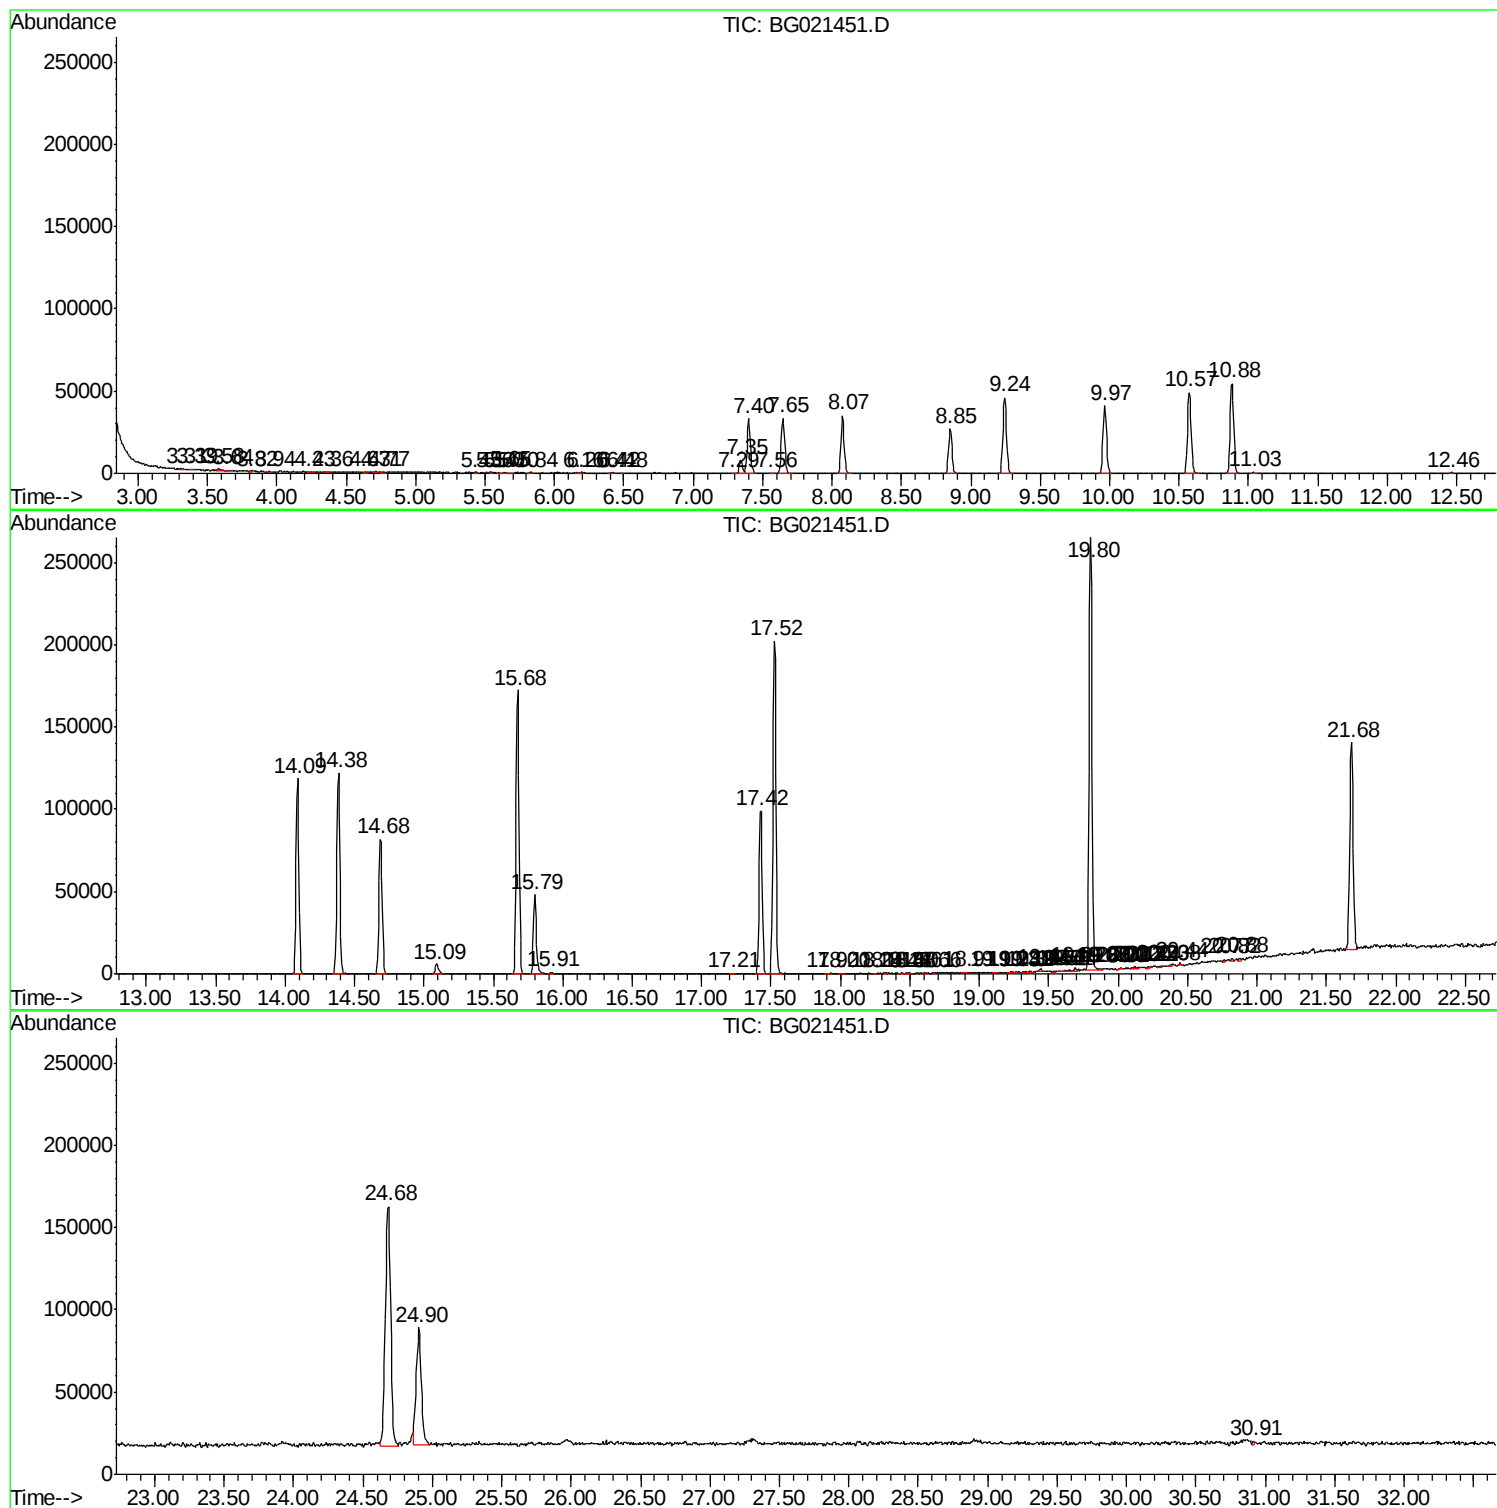

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021451.D
Acq On : 21 Mar 2016 19:46
Operator : UM/SJ
Sample : H1835-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T13

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021451.D
Acq On : 21 Mar 2016 19:46
Operator : UM/SJ
Sample : H1835-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T13

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc