

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021454.D
 Acq On : 21 Mar 2016 21:44
 Operator : UM/SJ
 Sample : H1835-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T20

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.104	44	45	47	rBV2	565	452	0.13%	0.014%
2	3.280	74	75	78	rBV3	1006	965	0.28%	0.030%
3	3.568	122	124	128	rBV2	511	542	0.16%	0.017%
4	3.950	188	189	193	rVB2	416	460	0.13%	0.014%
5	4.044	203	205	208	rBV3	384	371	0.11%	0.012%
6	4.103	213	215	219	rBV3	541	823	0.24%	0.026%
7	4.185	227	229	232	rVB2	409	437	0.13%	0.014%
8	4.221	232	235	237	rBV	333	425	0.12%	0.013%
9	4.579	295	296	301	rBV2	427	542	0.16%	0.017%
10	4.843	339	341	343	rVB2	546	479	0.14%	0.015%
11	5.008	368	369	372	rBV	479	368	0.11%	0.011%
12	5.125	386	389	390	rVB2	449	421	0.12%	0.013%
13	5.513	454	455	458	rVB	497	433	0.13%	0.014%
14	5.537	458	459	462	rBV	411	455	0.13%	0.014%
15	5.572	464	465	471	rBV2	434	686	0.20%	0.021%
16	5.807	503	505	508	rVB	473	520	0.15%	0.016%
17	5.842	508	511	512	rBV	668	675	0.20%	0.021%
18	5.866	512	515	517	rVV2	517	575	0.17%	0.018%
19	6.071	548	550	552	rVB	515	387	0.11%	0.012%
20	6.118	555	558	562	rVV	572	843	0.24%	0.026%
21	6.177	566	568	571	rVV2	531	559	0.16%	0.017%
22	6.230	574	577	578	rVV2	423	458	0.13%	0.014%
23	6.253	578	581	584	rVB	330	474	0.14%	0.015%
24	6.400	602	606	607	rVV2	471	595	0.17%	0.019%
25	6.418	607	609	612	rVV2	586	607	0.18%	0.019%
26	6.453	612	615	619	rVV	485	626	0.18%	0.020%
27	6.518	623	626	629	rVB	400	504	0.15%	0.016%
28	6.547	629	631	633	rBV	406	483	0.14%	0.015%
29	6.577	633	636	638	rVB2	341	382	0.11%	0.012%
30	6.770	666	669	672	rVB2	478	718	0.21%	0.022%
31	6.794	672	673	676	rBV	400	458	0.13%	0.014%
32	6.911	690	693	695	rBB2	405	390	0.11%	0.012%
33	7.041	714	715	719	rBV2	407	440	0.13%	0.014%
34	7.158	733	735	738	rVB	386	369	0.11%	0.012%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021454.D
 Acq On : 21 Mar 2016 21:44
 Operator : UM/SJ
 Sample : H1835-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T20

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	7.346	761	767	771	rBV	9873	16854	4.88%	0.526%
36	7.399	771	776	784	rVV	36345	59834	17.33%	1.867%
37	7.646	811	818	826	rBB	37098	62744	18.17%	1.958%
38	7.775	837	840	843	rBV	454	592	0.17%	0.018%
39	8.016	877	881	883	rBB	322	360	0.10%	0.011%
40	8.075	883	891	900	rBB	38491	64895	18.79%	2.025%
41	8.345	936	937	940	rBV	347	424	0.12%	0.013%
42	8.850	1017	1023	1031	rBB2	31351	54843	15.88%	1.711%
43	9.244	1083	1090	1099	rBB	51641	89209	25.84%	2.784%
44	9.967	1206	1213	1220	rBB	45072	80837	23.41%	2.522%
45	10.572	1310	1316	1328	rBB	55291	100026	28.97%	3.121%
46	10.883	1362	1369	1376	rBB	60583	106708	30.90%	3.330%
47	11.030	1390	1394	1398	rBB	906	1225	0.35%	0.038%
48	12.458	1633	1637	1639	rBB2	614	813	0.24%	0.025%
49	14.091	1909	1915	1921	rBV	135156	197713	57.26%	6.169%
50	14.385	1958	1965	1972	rBV	150502	228971	66.31%	7.145%
51	14.685	2010	2016	2023	rBB3	98234	155385	45.00%	4.849%
52	15.096	2081	2086	2093	rBV3	4742	8803	2.55%	0.275%
53	15.678	2178	2185	2192	rBB	192365	293705	85.06%	9.165%
54	15.795	2200	2205	2213	rBV	42941	66888	19.37%	2.087%
55	15.860	2213	2216	2218	rVB	444	505	0.15%	0.016%
56	15.919	2222	2226	2229	rBB	1210	1373	0.40%	0.043%
57	17.423	2476	2482	2490	rBB	114023	166913	48.34%	5.208%
58	17.523	2492	2499	2507	rBV2	203507	299893	86.85%	9.358%
59	17.581	2507	2509	2513	rVB	612	722	0.21%	0.023%
60	17.934	2566	2569	2571	rBB	401	445	0.13%	0.014%
61	17.975	2574	2576	2578	rBV	403	451	0.13%	0.014%
62	18.028	2582	2585	2586	rBV	409	386	0.11%	0.012%
63	18.263	2622	2625	2628	rBB2	504	627	0.18%	0.020%
64	18.369	2640	2643	2647	rBV2	419	538	0.16%	0.017%
65	18.627	2685	2687	2689	rVB	588	419	0.12%	0.013%
66	18.668	2689	2694	2695	rVB	376	369	0.11%	0.012%
67	18.774	2711	2712	2717	rBV	416	585	0.17%	0.018%
68	18.815	2717	2719	2721	rVB2	508	428	0.12%	0.013%
69	18.927	2736	2738	2739	rVB	585	365	0.11%	0.011%
70	19.062	2758	2761	2765	rVB2	404	662	0.19%	0.021%
71	19.221	2783	2788	2790	rVV2	490	651	0.19%	0.020%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021454.D
 Acq On : 21 Mar 2016 21:44
 Operator : UM/SJ
 Sample : H1835-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T20

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	19.250	2792	2793	2796	rVB2	493	450	0.13%	0.014%
73	19.279	2796	2798	2801	rVB2	659	560	0.16%	0.017%
74	19.309	2801	2803	2804	rVB	521	366	0.11%	0.011%
75	19.356	2804	2811	2814	rBV2	730	1472	0.43%	0.046%
76	19.438	2822	2825	2831	rVB4	2276	2978	0.86%	0.093%
77	19.550	2843	2844	2846	rVB	561	362	0.10%	0.011%
78	19.567	2846	2847	2850	rVB2	738	573	0.17%	0.018%
79	19.650	2859	2861	2863	rVB2	446	376	0.11%	0.012%
80	19.685	2863	2867	2871	rBV2	1191	2229	0.65%	0.070%
81	19.732	2871	2875	2877	rBV2	630	904	0.26%	0.028%
82	19.802	2880	2887	2896	rBV	241772	345282	100.00%	10.774%
83	19.885	2900	2901	2906	rVB3	617	784	0.23%	0.024%
84	19.937	2907	2910	2911	rBV2	589	633	0.18%	0.020%
85	19.973	2914	2916	2917	rBV	680	495	0.14%	0.015%
86	20.055	2928	2930	2931	rBV2	990	884	0.26%	0.028%
87	20.114	2939	2940	2944	rBV3	1007	1243	0.36%	0.039%
88	20.155	2944	2947	2948	rVB3	1467	1216	0.35%	0.038%
89	20.184	2948	2952	2955	rBV2	1219	2222	0.64%	0.069%
90	20.237	2959	2961	2962	rBV2	681	439	0.13%	0.014%
91	20.302	2970	2972	2973	rBV2	1007	802	0.23%	0.025%
92	20.355	2979	2981	2982	rVB2	1319	764	0.22%	0.024%
93	20.396	2986	2988	2991	rBV2	953	1448	0.42%	0.045%
94	20.519	3007	3009	3011	rBV2	1094	800	0.23%	0.025%
95	20.684	3035	3037	3038	rBV2	1218	860	0.25%	0.027%
96	21.395	3156	3158	3160	rBV3	2296	2371	0.69%	0.074%
97	21.677	3200	3206	3212	rBV	123042	204562	59.24%	6.383%
98	24.673	3708	3716	3728	rVB	126923	343602	99.51%	10.722%
99	24.902	3745	3755	3766	rVB2	70041	200677	58.12%	6.262%
100	27.687	4227	4229	4230	rBV2	2483	1329	0.38%	0.041%


Sum of corrected areas: 3204766

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021454.D
Acq On : 21 Mar 2016 21:44
Operator : UM/SJ
Sample : H1835-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T20

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

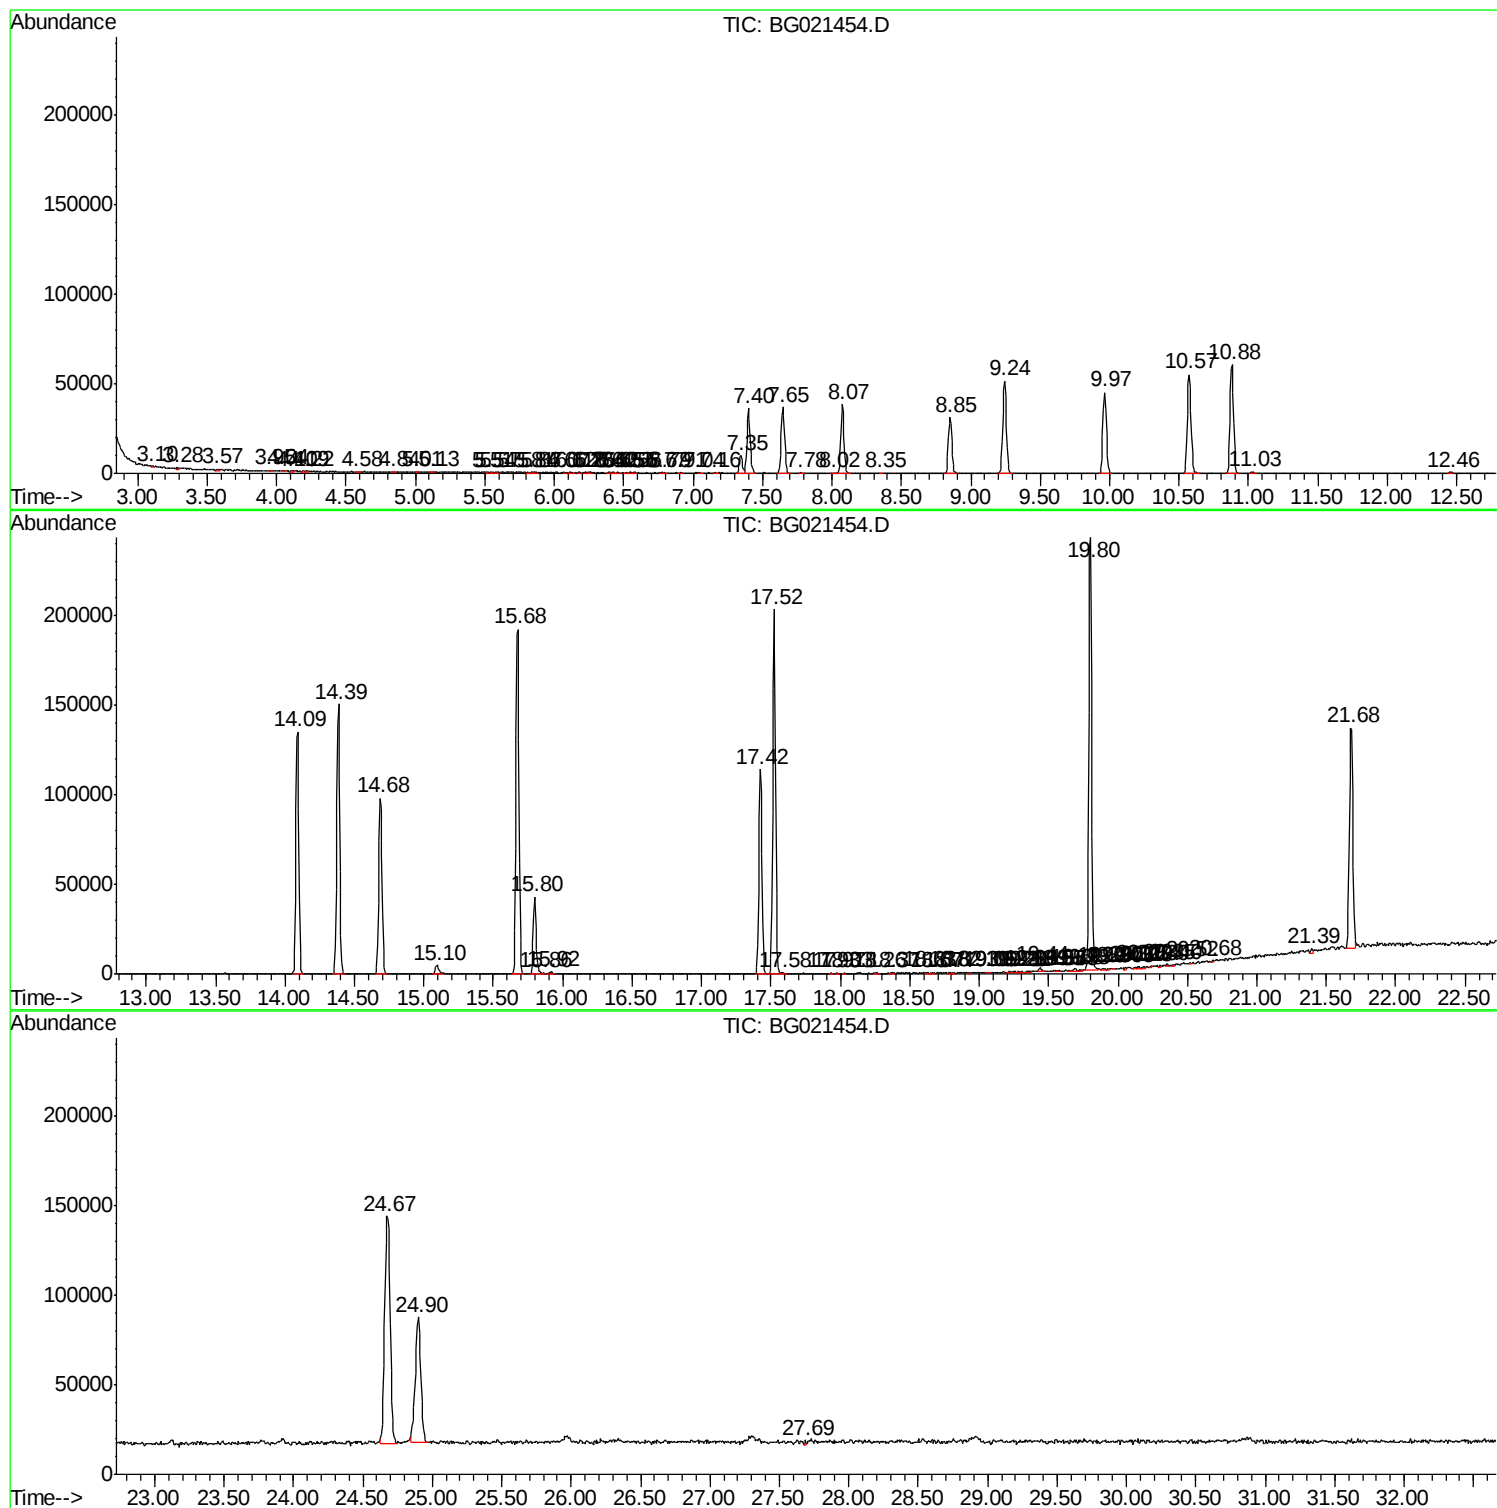

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021454.D
Acq On : 21 Mar 2016 21:44
Operator : UM/SJ
Sample : H1835-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T20

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021454.D
Acq On : 21 Mar 2016 21:44
Operator : UM/SJ
Sample : H1835-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T20

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc