

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021457.D
 Acq On : 21 Mar 2016 23:42
 Operator : UM/SJ
 Sample : H1835-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.349	85	87	91	rBV3	480	599	0.16%	0.018%
2	3.860	172	174	175	rBV2	645	387	0.10%	0.012%
3	3.948	187	189	194	rVB2	768	888	0.23%	0.027%
4	4.001	196	198	200	rVV2	833	513	0.13%	0.016%
5	4.048	204	206	210	rBV3	393	439	0.11%	0.013%
6	4.142	219	222	225	rBV2	652	686	0.18%	0.021%
7	4.342	254	256	259	rVB2	476	556	0.15%	0.017%
8	4.459	275	276	279	rVB3	487	437	0.11%	0.013%
9	4.489	279	281	282	rBV2	559	419	0.11%	0.013%
10	4.506	282	284	286	rVV2	574	565	0.15%	0.017%
11	4.924	351	355	357	rBV2	425	502	0.13%	0.015%
12	4.941	357	358	362	rVB2	523	504	0.13%	0.015%
13	5.388	429	434	436	rBV	364	559	0.15%	0.017%
14	5.505	452	454	457	rVB2	421	480	0.13%	0.015%
15	5.964	531	532	536	rVB	575	544	0.14%	0.017%
16	5.999	536	538	540	rBV	437	479	0.12%	0.015%
17	6.028	540	543	547	rBV2	396	417	0.11%	0.013%
18	6.146	559	563	564	rVV	356	430	0.11%	0.013%
19	6.163	564	566	568	rVB2	589	436	0.11%	0.013%
20	6.322	590	593	595	rBV	396	401	0.10%	0.012%
21	6.381	599	603	604	rBV	468	537	0.14%	0.016%
22	6.510	621	625	626	rBV	358	392	0.10%	0.012%
23	7.203	742	743	748	rVB2	355	400	0.10%	0.012%
24	7.268	752	754	758	rVB2	483	698	0.18%	0.021%
25	7.344	761	767	771	rBV	7860	11999	3.13%	0.367%
26	7.397	771	776	783	rVB	31401	50465	13.16%	1.545%
27	7.515	793	796	798	rBV	340	433	0.11%	0.013%
28	7.562	801	804	807	rVB	362	458	0.12%	0.014%
29	7.644	813	818	826	rBV	32243	53388	13.93%	1.635%
30	8.073	883	891	897	rBB	37955	61370	16.01%	1.879%
31	8.132	897	901	903	rBV	343	461	0.12%	0.014%
32	8.848	1016	1023	1032	rBB	25784	44267	11.55%	1.356%
33	9.242	1084	1090	1098	rBB	44285	74203	19.36%	2.272%
34	9.959	1207	1212	1219	rBB2	37934	66391	17.32%	2.033%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021457.D
 Acq On : 21 Mar 2016 23:42
 Operator : UM/SJ
 Sample : H1835-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	10.570	1310	1316	1326	rBV	48903	85923	22.41%	2.631%
36	10.881	1362	1369	1378	rBB	59202	103977	27.12%	3.184%
37	11.028	1389	1394	1399	rBB	1324	1863	0.49%	0.057%
38	12.456	1634	1637	1640	rBB	658	862	0.22%	0.026%
39	13.572	1824	1827	1830	rBB2	952	1116	0.29%	0.034%
40	14.089	1909	1915	1921	rBV	134032	189520	49.43%	5.804%
41	14.383	1958	1965	1971	rBV	132064	203723	53.14%	6.239%
42	14.683	2010	2016	2023	rBB2	92259	150077	39.15%	4.596%
43	15.094	2082	2086	2094	rBB3	5158	8804	2.30%	0.270%
44	15.676	2178	2185	2191	rBV	179741	275867	71.96%	8.448%
45	15.793	2200	2205	2218	rBB	53527	81539	21.27%	2.497%
46	15.911	2222	2225	2229	rBB	1295	1363	0.36%	0.042%
47	16.069	2249	2252	2255	rBB	1346	1510	0.39%	0.046%
48	17.427	2477	2483	2489	rBV	126280	186549	48.66%	5.713%
49	17.521	2492	2499	2510	rBB	207133	316171	82.47%	9.682%
50	17.850	2553	2555	2558	rBB	544	445	0.12%	0.014%
51	17.920	2564	2567	2571	rBB	390	476	0.12%	0.015%
52	18.232	2617	2620	2621	rVV	378	387	0.10%	0.012%
53	18.261	2624	2625	2628	rBV	545	428	0.11%	0.013%
54	18.373	2637	2644	2646	rBV2	347	547	0.14%	0.017%
55	18.942	2737	2741	2743	rVB	417	586	0.15%	0.018%
56	18.978	2743	2747	2749	rBV2	601	693	0.18%	0.021%
57	19.089	2762	2766	2767	rBV	351	466	0.12%	0.014%
58	19.254	2791	2794	2796	rVB3	693	629	0.16%	0.019%
59	19.277	2796	2798	2800	rBV	678	654	0.17%	0.020%
60	19.436	2819	2825	2829	rBV2	2074	3604	0.94%	0.110%
61	19.518	2838	2839	2842	rBV	414	421	0.11%	0.013%
62	19.583	2848	2850	2851	rVB	630	430	0.11%	0.013%
63	19.601	2851	2853	2854	rBV2	693	510	0.13%	0.016%
64	19.624	2856	2857	2860	rBV2	771	778	0.20%	0.024%
65	19.689	2865	2868	2870	rBV2	1079	1105	0.29%	0.034%
66	19.800	2881	2887	2893	rBV2	259498	383375	100.00%	11.740%
67	19.888	2901	2902	2905	rVB2	1148	626	0.16%	0.019%
68	19.912	2905	2906	2908	rBV	819	690	0.18%	0.021%
69	19.941	2908	2911	2912	rVV3	740	702	0.18%	0.021%
70	20.024	2924	2925	2927	rBV2	936	542	0.14%	0.017%
71	20.071	2931	2933	2937	rVB3	1088	1566	0.41%	0.048%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
 Data File : BG021457.D
 Acq On : 21 Mar 2016 23:42
 Operator : UM/SJ
 Sample : H1835-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	20.106	2937	2939	2940	rBV	1048	815	0.21%	0.025%
73	20.141	2944	2945	2947	rBV2	858	766	0.20%	0.023%
74	20.212	2955	2957	2959	rBV	1153	1267	0.33%	0.039%
75	20.282	2967	2969	2970	rBV	934	424	0.11%	0.013%
76	20.376	2981	2985	2986	rBV3	1153	1170	0.31%	0.036%
77	20.429	2992	2994	2995	rBV2	1354	716	0.19%	0.022%
78	20.476	3000	3002	3004	rBV4	1064	1138	0.30%	0.035%
79	20.529	3009	3011	3012	rBV2	1161	840	0.22%	0.026%
80	20.547	3012	3014	3015	rBV2	897	696	0.18%	0.021%
81	20.670	3033	3035	3038	rVB2	1259	1152	0.30%	0.035%
82	20.917	3075	3077	3078	rBV2	1578	1055	0.28%	0.032%
83	20.958	3082	3084	3086	rBV3	1879	1682	0.44%	0.052%
84	21.116	3109	3111	3112	rBV2	1597	968	0.25%	0.030%
85	21.675	3200	3206	3213	rBV	145085	240056	62.62%	7.351%
86	24.677	3708	3717	3731	rVB	137023	379661	99.03%	11.626%
87	24.894	3745	3754	3767	rVB2	81470	239489	62.47%	7.334%
88	25.288	3820	3821	3822	rBV	2541	1268	0.33%	0.039%
89	26.234	3978	3982	3985	rBV4	3430	5351	1.40%	0.164%
90	27.268	4156	4158	4159	rBV2	3211	2808	0.73%	0.086%


Sum of corrected areas: 3265549

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021457.D
Acq On : 21 Mar 2016 23:42
Operator : UM/SJ
Sample : H1835-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T23

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

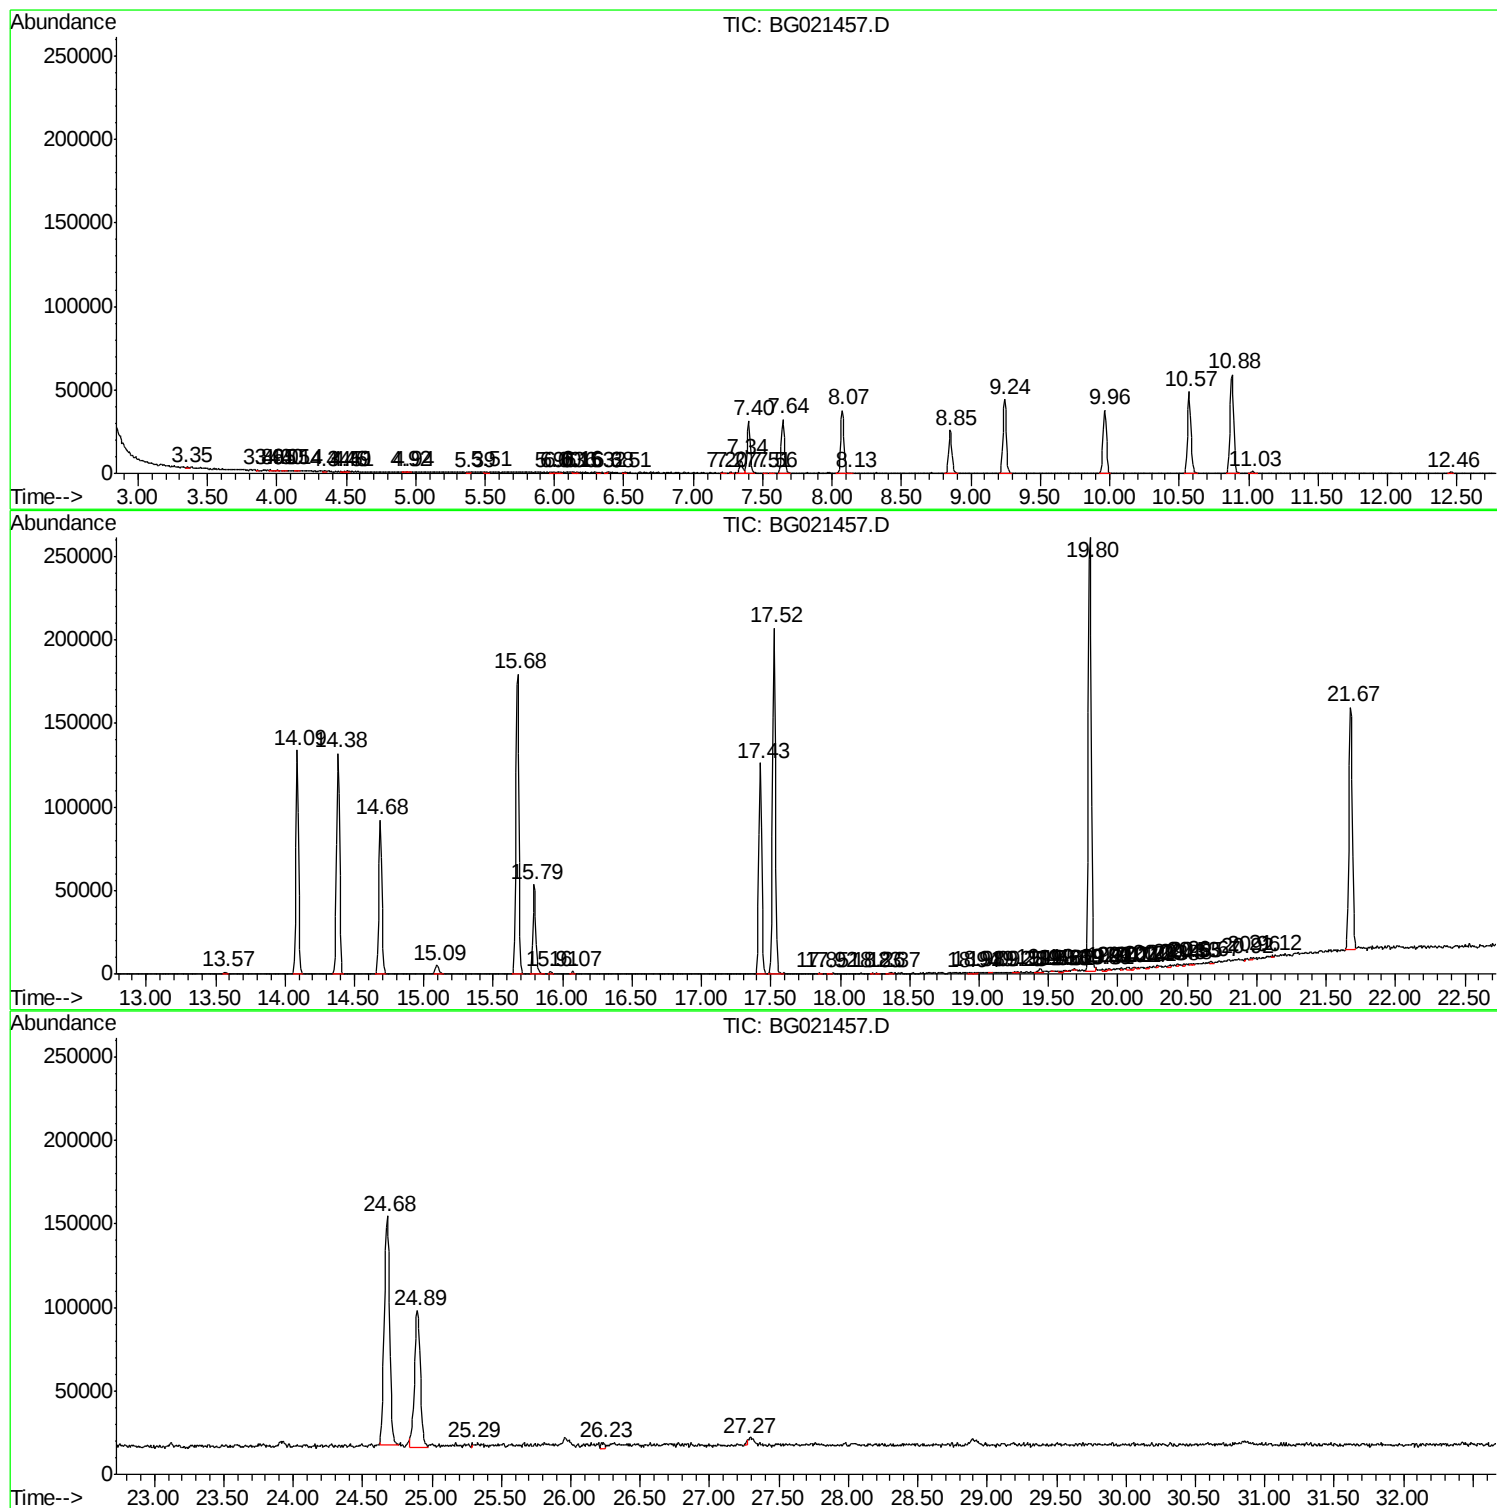

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021457.D
Acq On : 21 Mar 2016 23:42
Operator : UM/SJ
Sample : H1835-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T23

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032116\
Data File : BG021457.D
Acq On : 21 Mar 2016 23:42
Operator : UM/SJ
Sample : H1835-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T23

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc