
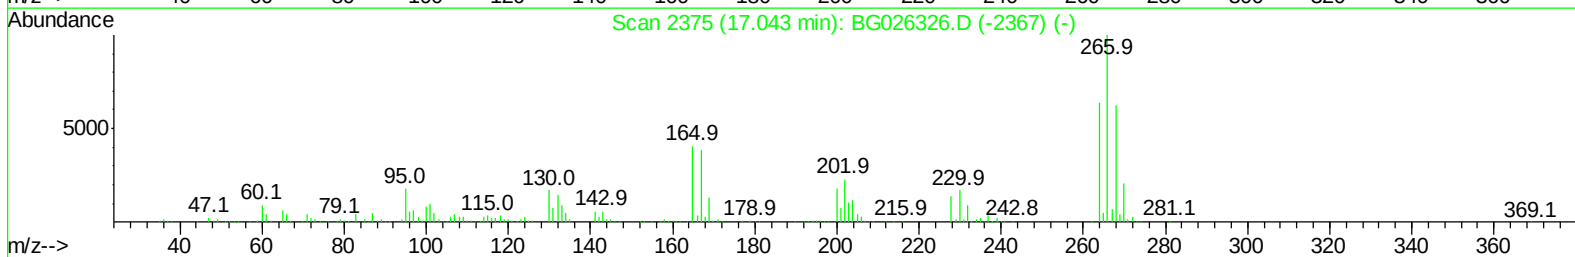
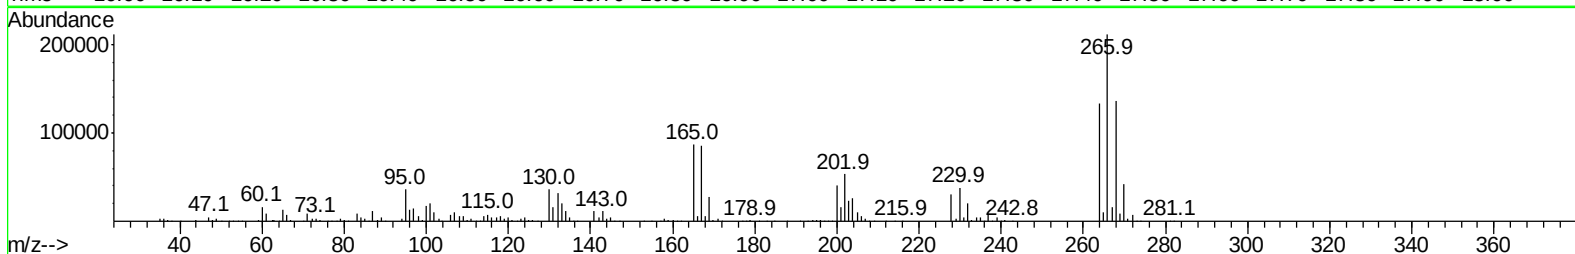


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032117\
Data File : BG026354.D
Acq On : 21 Mar 2017 10:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:41:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

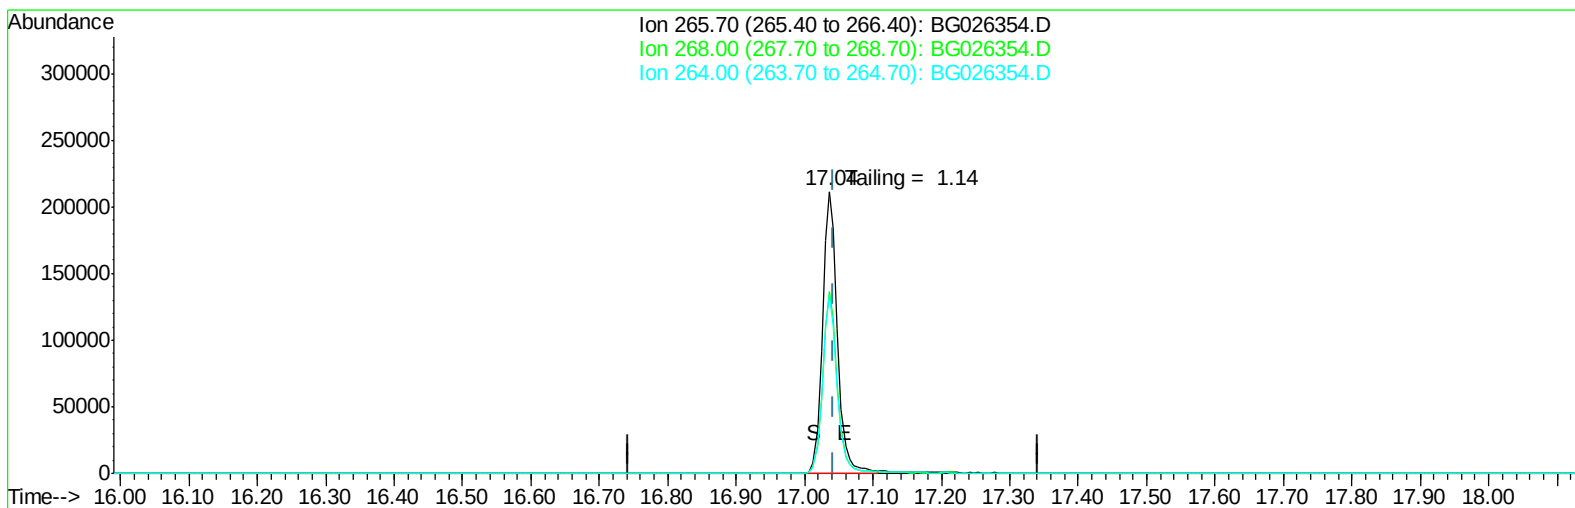

TIC: BG026354.D

(69) Pentachlorophenol (C)




17.036min (-0.007) 150726.18ng

response 324942

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	64.35
264.00	62.60	63.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032117\
Data File : BG026354.D
Acq On : 21 Mar 2017 10:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:41:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

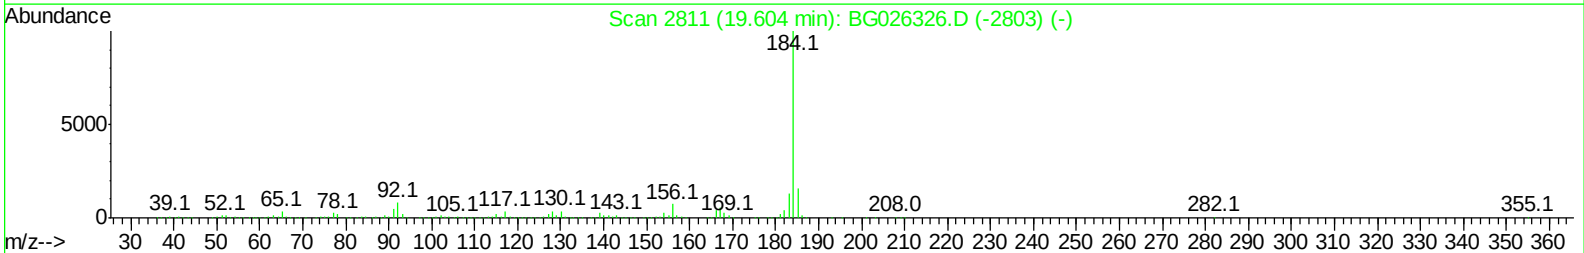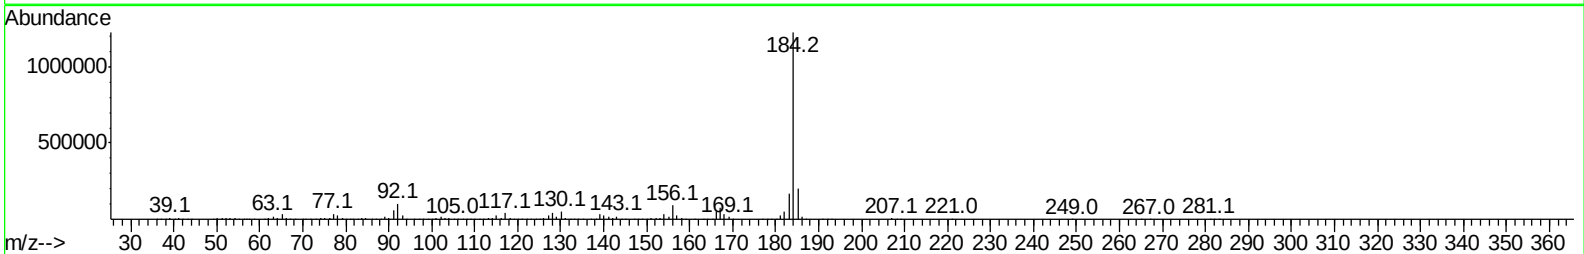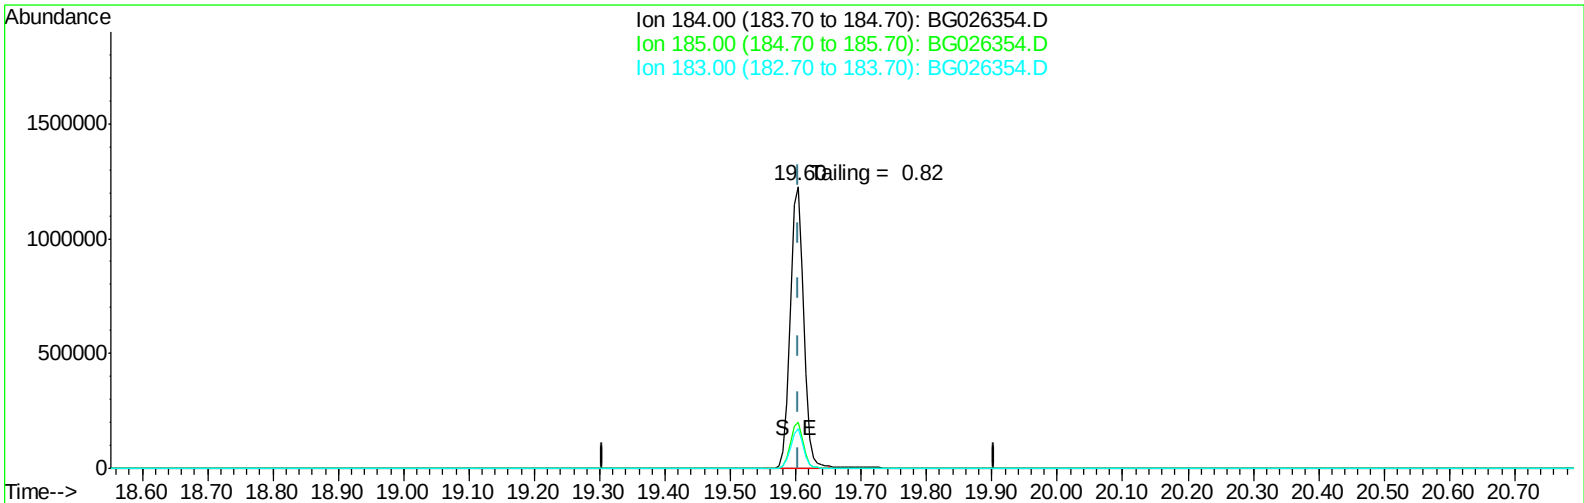

TIC: BG026354.D

(76) Benzidine

19.604min (-0.001) 19652.32ng

```
response 1781359
```

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.17
183.00	13.80	14.05
0.00	0.00	0.00