


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032117\
 Data File : BG026354.D
 Acq On : 21 Mar 2017 10:47
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 20 17:43:27 2017

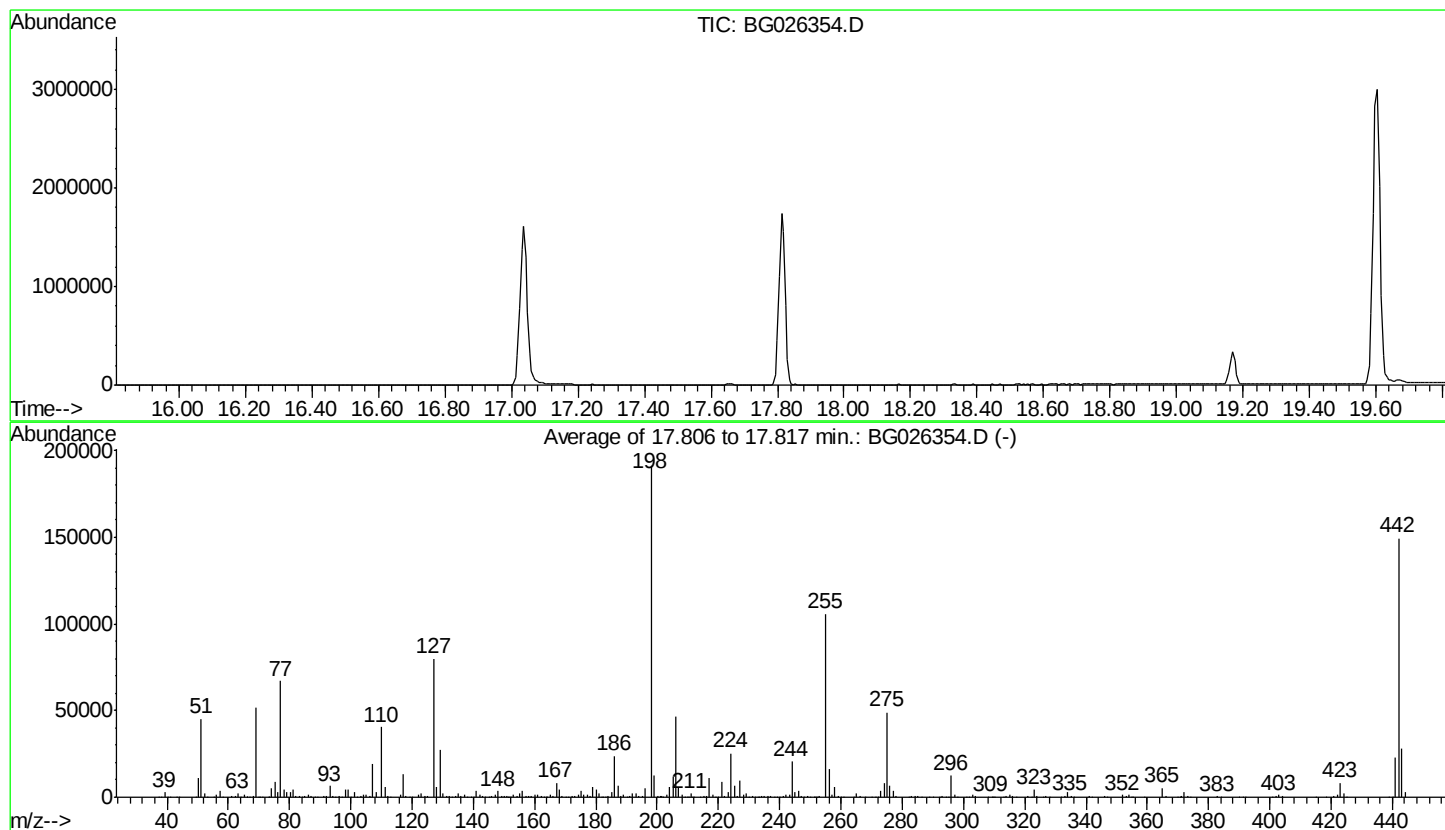

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.6	45122	PASS
68	69	0.00	2	0.9	467	PASS
69	198	0.00	100	26.9	51370	PASS
70	69	0.00	2	0.3	174	PASS
127	198	10	80	41.7	79834	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	191253	PASS
199	198	5	9	6.7	12839	PASS
275	198	10	60	25.6	49016	PASS
365	198	1	100	2.9	5541	PASS
441	442	0.01	24	15.6	23273	PASS
442	198	50	100	78.2	149485	PASS
443	442	15	24	18.9	28277	PASS