


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032119\
 Data File : BG040066.D
 Acq On : 21 Mar 2019 14:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

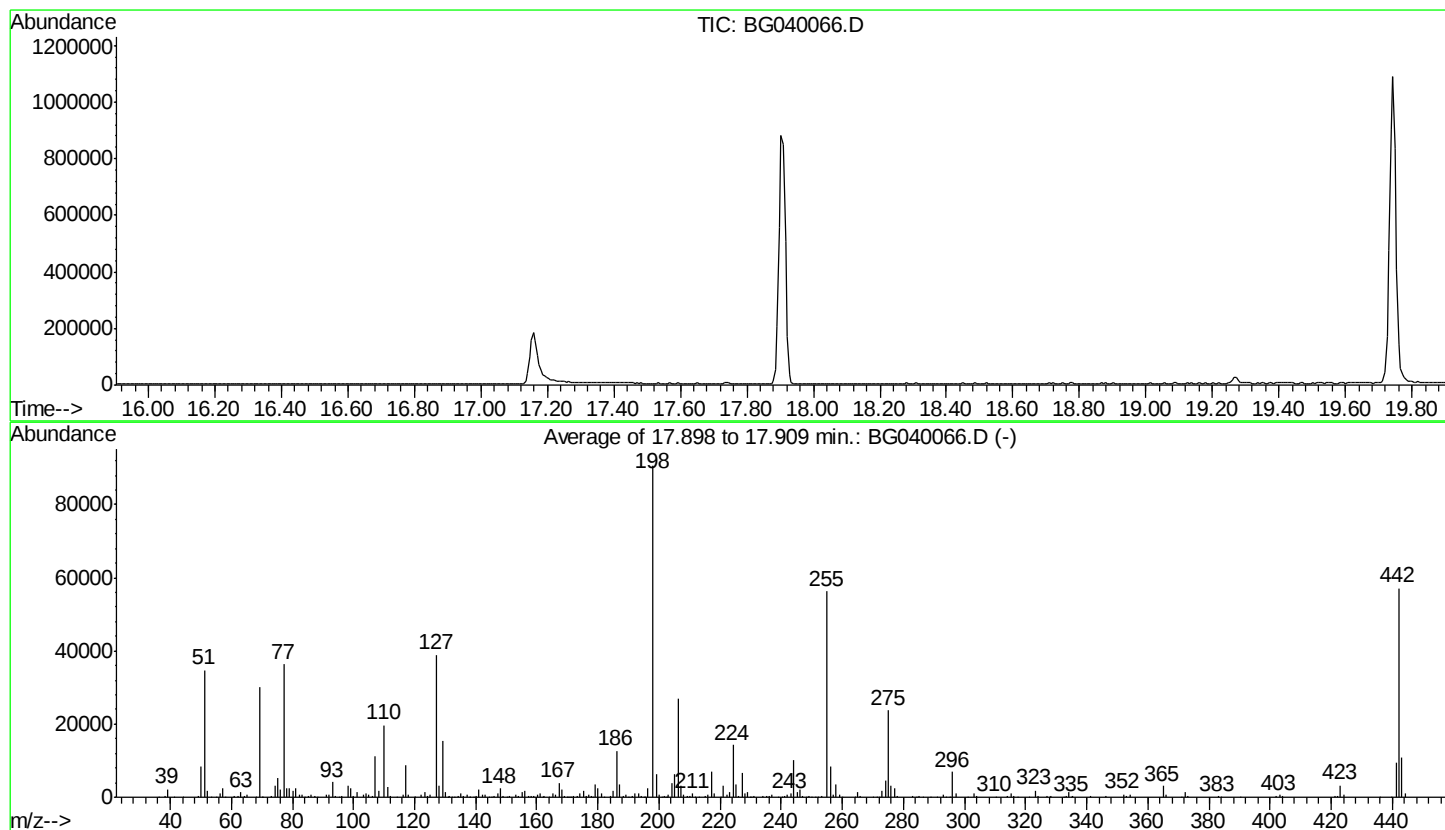

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	34669	PASS
68	69	0.00	2	0.6	187	PASS
69	198	0.00	100	33.1	29978	PASS
70	69	0.00	2	0.3	81	PASS
127	198	10	80	43.0	39029	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90674	PASS
199	198	5	9	6.8	6196	PASS
275	198	10	60	26.2	23741	PASS
365	198	1	100	3.3	3031	PASS
441	198	0.01	100	10.6	9593	PASS
442	198	50	100	63.0	57122	PASS
443	442	15	24	18.8	10716	PASS