

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021467.D
 Acq On : 22 Mar 2016 9:52
 Operator : UM/SJ
 Sample : H1829-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04Y5

Quant Time: Mar 23 01:32:15 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 01:30:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	11596	20.00	ng/ul	0.00
18) Naphthalene-d8	10.88	136	54908	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	33170	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.42	188	73391	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	87473	20.00	ng/ul	0.00
86) Perylene-d12	24.89	264	84853	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.34	99	6899	6.29	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.40	67	15658	24.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	18594	22.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	13519	14.40	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	11113	26.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.96	143	12244	26.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	23277	27.65	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	14.08	166	80163	29.02	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	98566	28.95	ng/ul	0.00
52) 4-Nitrophenol-d4	15.09	143	2260	5.12	ng/ul	0.02
58) Fluorene-d10	15.67	176	69961	28.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	12491	25.76	ng/ul	0.00
71) Anthracene-d10	17.52	188	100934	28.06	ng/ul	0.00
79) Pyrene-d10	19.80	212	119194	29.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.67	264	114204	29.16	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.13	163	8590	2.99	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021467.D
Acq On : 22 Mar 2016 9:52
Operator : UM/SJ
Sample : H1829-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04Y5

Quant Time: Mar 23 01:32:15 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 01:30:27 2016
Response via : Initial Calibration

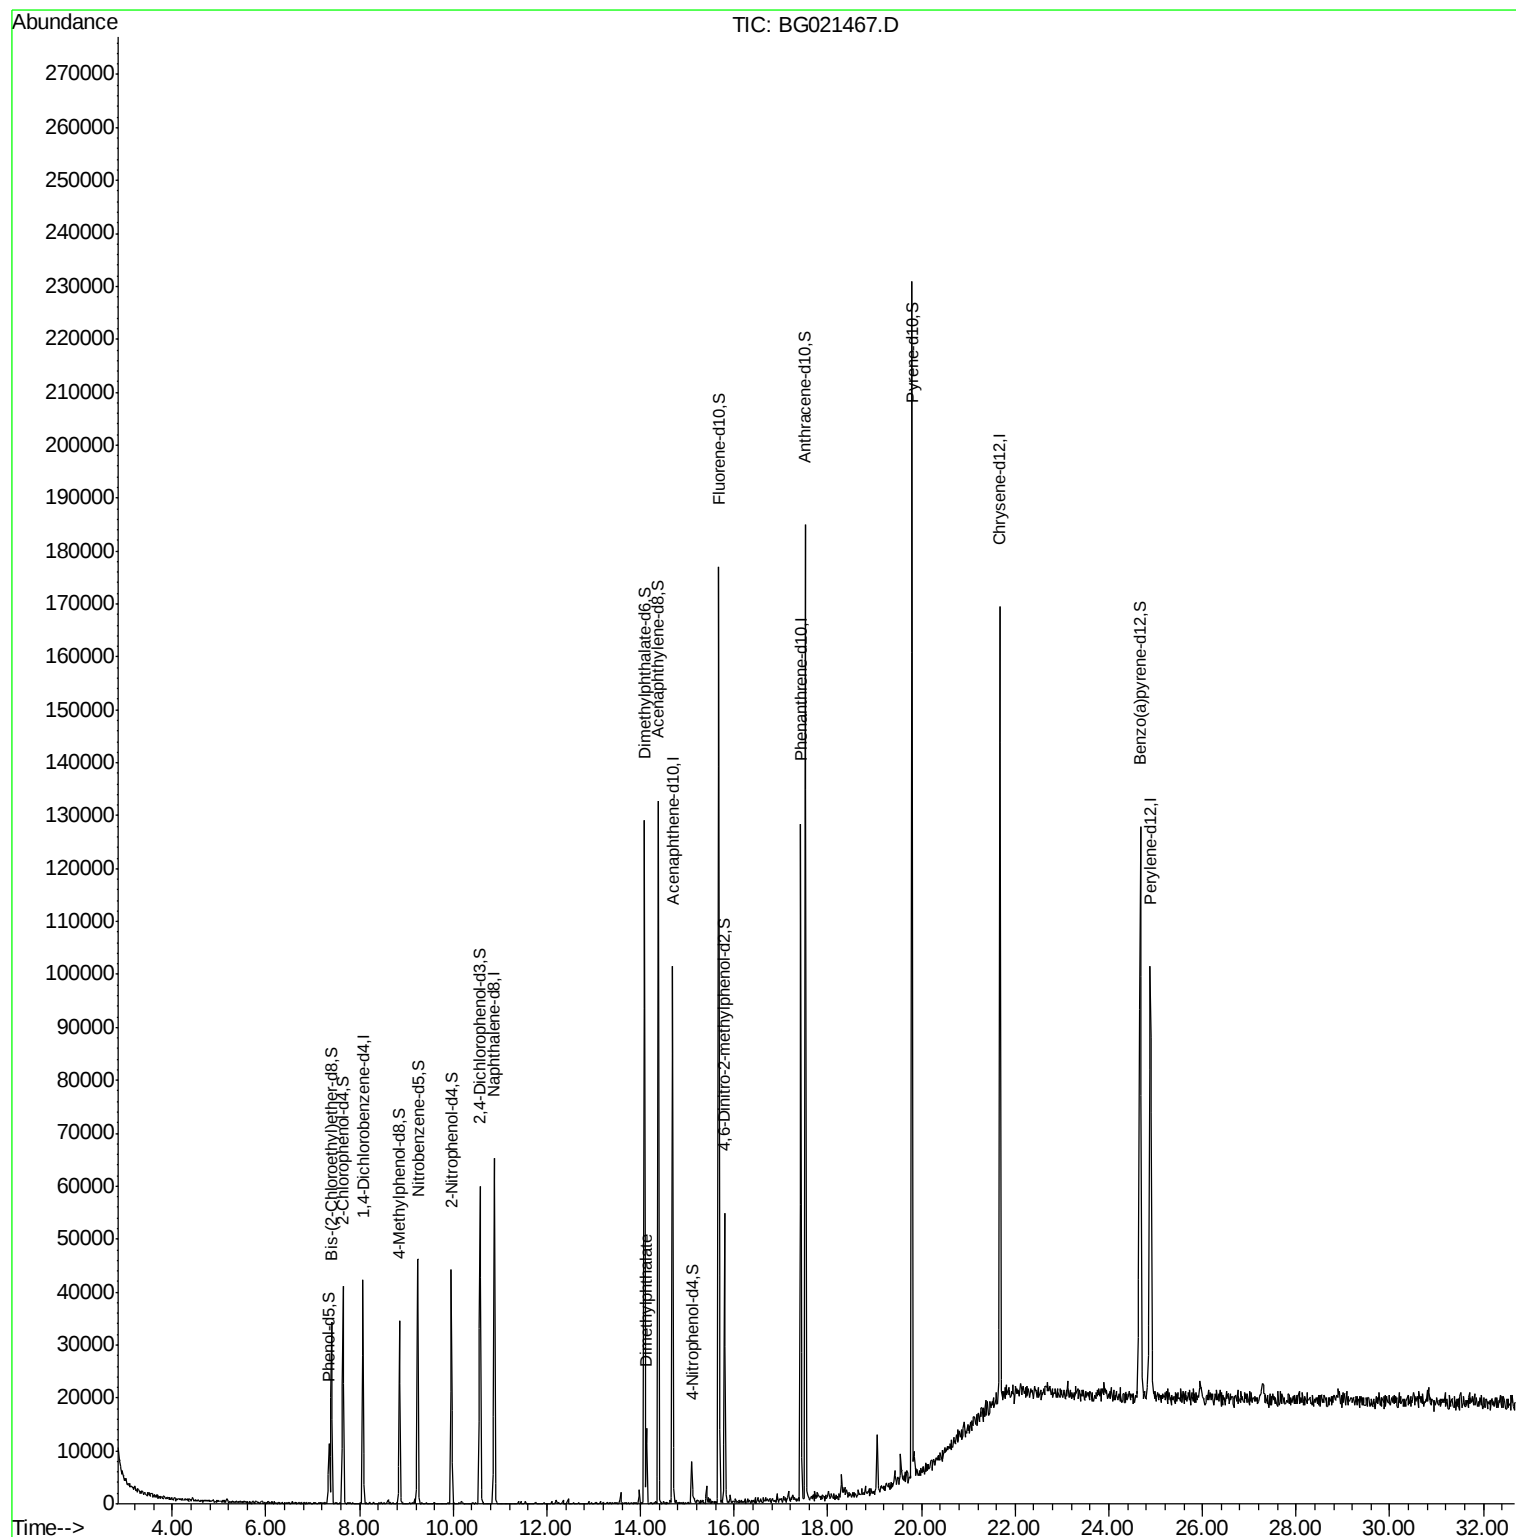

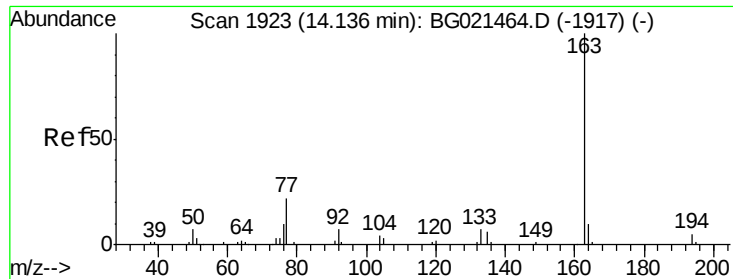

#45

Dimethylphthalate

Concen: 2.99 ng/ul

RT: 14.13 min Scan# 1922

Delta R.T. -0.01 min

Lab File: BG021467.D


Acq: 22 Mar 2016 9:52

Instrument :

BNA_G

ClientSampleId :

C04Y5

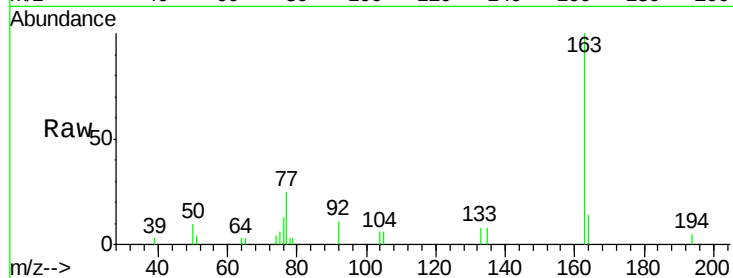

Tgt Ion:	163	Resp:	8590
Ion	Ratio	Lower	Upper
163	100		
194	4.9	3.9	5.9
164	13.9	8.7	13.1

