

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021474.D
 Acq On : 22 Mar 2016 14:59
 Operator : UM/SJ
 Sample : H1835-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.155	52	54	56	rVB2	765	560	0.16%	0.019%
2	3.754	154	156	157	rBV2	553	430	0.12%	0.014%
3	3.772	157	159	162	rVB3	498	508	0.14%	0.017%
4	4.060	206	208	211	rVB2	464	402	0.11%	0.014%
5	4.353	256	258	262	rBV2	308	476	0.13%	0.016%
6	4.395	262	265	269	rVB	457	511	0.14%	0.017%
7	4.688	314	315	320	rVB2	415	373	0.11%	0.013%
8	4.765	323	328	330	rVB3	376	623	0.18%	0.021%
9	4.794	330	333	336	rBV2	393	572	0.16%	0.019%
10	4.941	356	358	362	rVB	436	478	0.13%	0.016%
11	5.011	366	370	372	rBV	674	603	0.17%	0.020%
12	5.117	383	388	392	rBV3	359	681	0.19%	0.023%
13	5.223	404	406	408	rBV	512	582	0.16%	0.020%
14	5.317	420	422	427	rVB2	341	404	0.11%	0.014%
15	5.540	455	460	461	rBV	472	736	0.21%	0.025%
16	5.699	483	487	490	rBV3	374	387	0.11%	0.013%
17	5.728	490	492	493	rVB3	569	370	0.10%	0.012%
18	5.752	493	496	497	rBV	469	587	0.17%	0.020%
19	5.799	501	504	505	rBV	417	424	0.12%	0.014%
20	5.887	516	519	520	rBV2	454	375	0.11%	0.013%
21	6.004	534	539	542	rBV	399	700	0.20%	0.024%
22	6.057	545	548	551	rVV	319	451	0.13%	0.015%
23	6.098	553	555	560	rBV2	432	859	0.24%	0.029%
24	6.145	560	563	567	rVB	440	530	0.15%	0.018%
25	6.298	585	589	591	rVV2	521	446	0.13%	0.015%
26	6.316	591	592	595	rVB	417	386	0.11%	0.013%
27	6.386	603	604	606	rBV	417	411	0.12%	0.014%
28	6.510	623	625	627	rVB	582	457	0.13%	0.015%
29	6.627	644	645	648	rVB	389	382	0.11%	0.013%
30	6.657	648	650	653	rBV	413	473	0.13%	0.016%
31	7.015	707	711	713	rBB	401	494	0.14%	0.017%
32	7.350	762	768	771	rBV	6896	10501	2.96%	0.353%
33	7.397	771	776	784	rVB	28329	44567	12.57%	1.500%
34	7.644	813	818	825	rBV	28530	46118	13.01%	1.552%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021474.D
 Acq On : 22 Mar 2016 14:59
 Operator : UM/SJ
 Sample : H1835-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	8.073	885	891	898	rBB	32639	52606	14.84%	1.770%
36	8.854	1018	1024	1035	rBB	23669	41287	11.65%	1.389%
37	9.242	1083	1090	1097	rBB	37238	65552	18.50%	2.206%
38	9.959	1206	1212	1220	rBB2	34029	58935	16.63%	1.983%
39	10.576	1311	1317	1327	rBV	46253	80163	22.62%	2.698%
40	10.875	1362	1368	1376	rBB	51490	91151	25.72%	3.068%
41	11.034	1390	1395	1399	rBB2	879	1557	0.44%	0.052%
42	12.456	1634	1637	1640	rBB	475	522	0.15%	0.018%
43	13.572	1823	1827	1830	rBB	866	1172	0.33%	0.039%
44	14.089	1909	1915	1923	rBB	118820	172884	48.78%	5.818%
45	14.377	1958	1964	1973	rBV	118160	187814	52.99%	6.321%
46	14.682	2010	2016	2023	rBB2	86104	139887	39.47%	4.708%
47	15.100	2083	2087	2094	rBV2	3896	7168	2.02%	0.241%
48	15.670	2178	2184	2192	rBB	168279	252626	71.28%	8.502%
49	15.793	2200	2205	2215	rBB	52142	78975	22.28%	2.658%
50	15.910	2222	2225	2228	rBB2	1163	1155	0.33%	0.039%
51	17.420	2476	2482	2489	rBB	118907	172423	48.65%	5.803%
52	17.520	2493	2499	2506	rBV	203323	298070	84.10%	10.031%
53	18.208	2613	2616	2618	rBV	427	407	0.11%	0.014%
54	18.302	2631	2632	2636	rVB	451	385	0.11%	0.013%
55	18.713	2698	2702	2705	rBV2	475	558	0.16%	0.019%
56	18.930	2735	2739	2742	rBV2	312	487	0.14%	0.016%
57	19.001	2748	2751	2753	rBV	466	487	0.14%	0.016%
58	19.095	2765	2767	2769	rBV	424	418	0.12%	0.014%
59	19.259	2793	2795	2797	rBV	737	413	0.12%	0.014%
60	19.289	2797	2800	2803	rBV3	642	706	0.20%	0.024%
61	19.348	2809	2810	2813	rBV2	497	538	0.15%	0.018%
62	19.389	2813	2817	2818	rVB3	495	356	0.10%	0.012%
63	19.436	2822	2825	2830	rBV2	1961	2707	0.76%	0.091%
64	19.553	2843	2845	2847	rBV2	628	566	0.16%	0.019%
65	19.612	2850	2855	2856	rBV2	754	944	0.27%	0.032%
66	19.647	2859	2861	2865	rVB2	702	686	0.19%	0.023%
67	19.688	2865	2868	2871	rBV2	1904	2294	0.65%	0.077%
68	19.753	2875	2879	2880	rBV	481	513	0.14%	0.017%
69	19.794	2880	2886	2895	rVV	245781	354417	100.00%	11.928%
70	19.865	2897	2898	2899	rBV	731	366	0.10%	0.012%
71	19.912	2903	2906	2908	rVB3	541	574	0.16%	0.019%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021474.D
 Acq On : 22 Mar 2016 14:59
 Operator : UM/SJ
 Sample : H1835-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	19.947	2910	2912	2913	rBV	779	632	0.18%	0.021%
73	19.982	2916	2918	2922	rBV2	826	1101	0.31%	0.037%
74	20.012	2922	2923	2926	rBV2	800	700	0.20%	0.024%
75	20.053	2928	2930	2931	rVB2	1265	683	0.19%	0.023%
76	20.070	2931	2933	2934	rBV2	617	525	0.15%	0.018%
77	20.111	2938	2940	2942	rVV	840	612	0.17%	0.021%
78	20.158	2946	2948	2949	rVB	940	477	0.13%	0.016%
79	20.247	2961	2963	2966	rBV3	877	1040	0.29%	0.035%
80	20.276	2966	2968	2969	rVB2	741	436	0.12%	0.015%
81	20.423	2991	2993	2995	rBV2	770	530	0.15%	0.018%
82	20.464	2997	3000	3001	rBV2	1599	1545	0.44%	0.052%
83	20.805	3056	3058	3059	rBV2	1517	936	0.26%	0.032%
84	20.893	3072	3073	3077	rBV3	1534	1644	0.46%	0.055%
85	21.392	3157	3158	3159	rBV	2022	767	0.22%	0.026%
86	21.674	3200	3206	3214	rBV	134296	219634	61.97%	7.392%
87	24.671	3706	3716	3726	rBV	128072	346018	97.63%	11.645%
88	24.888	3744	3753	3765	rVB2	71780	202954	57.26%	6.830%
89	25.934	3929	3931	3932	rBV2	3073	2565	0.72%	0.086%


Sum of corrected areas: 2971425

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021474.D
Acq On : 22 Mar 2016 14:59
Operator : UM/SJ
Sample : H1835-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T32

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

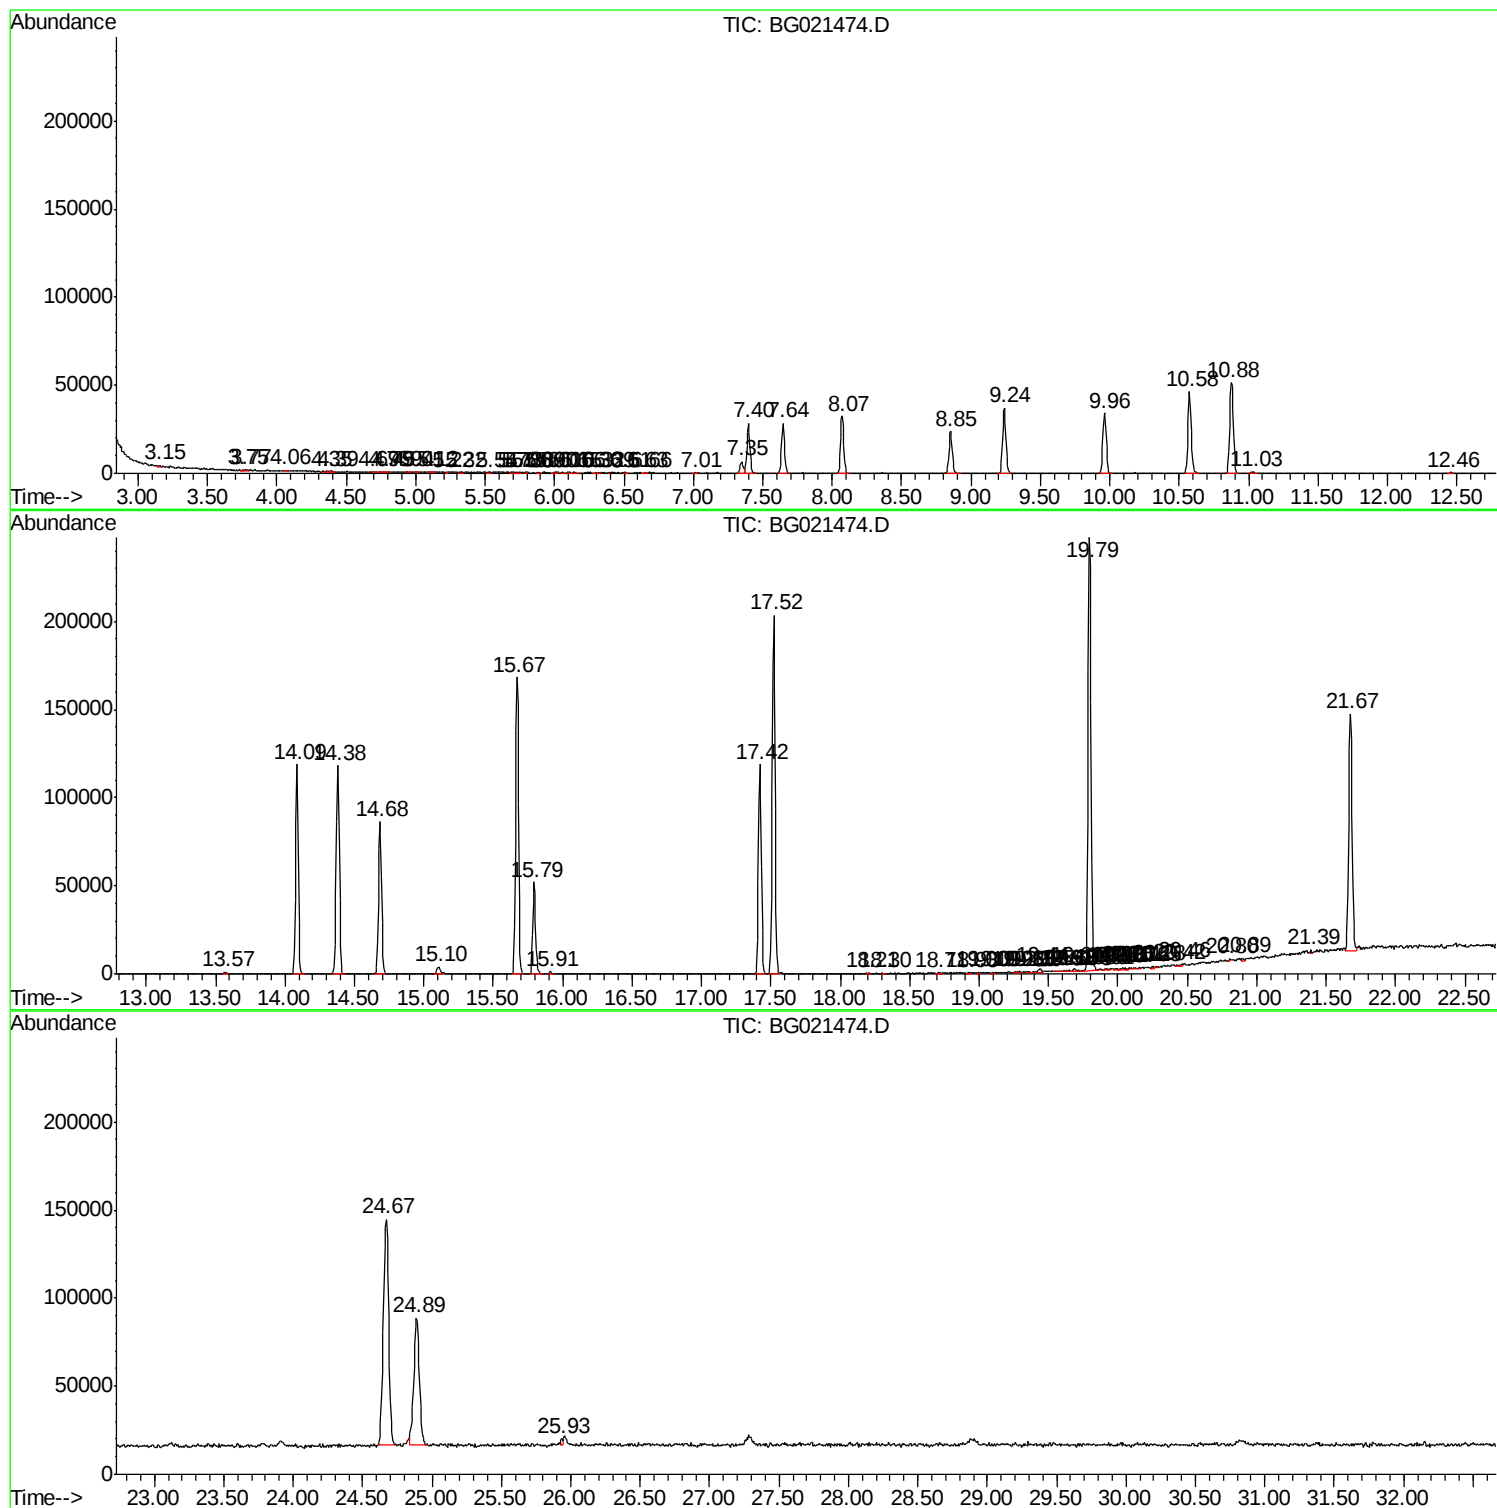

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021474.D
Acq On : 22 Mar 2016 14:59
Operator : UM/SJ
Sample : H1835-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T32

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021474.D
Acq On : 22 Mar 2016 14:59
Operator : UM/SJ
Sample : H1835-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T32

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc