

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021475.D
 Acq On : 22 Mar 2016 15:38
 Operator : UM/SJ
 Sample : H1835-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.447	101	103	104	rVB2	740	454	0.13%	0.015%
2	3.470	104	107	110	rVB5	863	1225	0.34%	0.040%
3	3.499	110	112	113	rBV2	747	546	0.15%	0.018%
4	3.552	120	121	124	rVB3	510	414	0.12%	0.013%
5	3.905	179	181	183	rBV2	496	536	0.15%	0.017%
6	3.928	183	185	189	rVB3	469	511	0.14%	0.016%
7	4.052	204	206	209	rVB	593	505	0.14%	0.016%
8	4.081	209	211	215	rBV3	285	360	0.10%	0.012%
9	4.205	229	232	235	rVB2	573	660	0.19%	0.021%
10	4.228	235	236	238	rBV	521	428	0.12%	0.014%
11	4.252	238	240	245	rVB3	572	598	0.17%	0.019%
12	4.334	252	254	256	rBV2	456	419	0.12%	0.014%
13	4.445	269	273	277	rVV2	331	549	0.15%	0.018%
14	4.604	298	300	302	rVB	468	363	0.10%	0.012%
15	4.733	320	322	324	rBV	372	388	0.11%	0.013%
16	5.015	368	370	373	rBV2	419	368	0.10%	0.012%
17	5.503	450	453	456	rVB	618	853	0.24%	0.028%
18	5.532	456	458	459	rBV	453	442	0.12%	0.014%
19	5.562	462	463	469	rVB2	336	496	0.14%	0.016%
20	5.773	496	499	501	rVB2	356	399	0.11%	0.013%
21	6.132	559	560	562	rBV2	428	406	0.11%	0.013%
22	6.331	590	594	596	rBB2	420	526	0.15%	0.017%
23	6.402	603	606	609	rVB2	489	563	0.16%	0.018%
24	6.449	612	614	616	rBV2	368	482	0.14%	0.016%
25	6.596	636	639	642	rBV2	452	551	0.15%	0.018%
26	6.637	645	646	650	rVB	400	391	0.11%	0.013%
27	7.230	746	747	751	rBB	482	363	0.10%	0.012%
28	7.348	761	767	771	rBV2	8305	14187	3.98%	0.458%
29	7.395	771	775	782	rVB	30836	48002	13.47%	1.550%
30	7.648	810	818	826	rBB	32404	51705	14.51%	1.669%
31	8.071	884	890	897	rBB	38874	63787	17.90%	2.059%
32	8.852	1017	1023	1034	rBB	26412	45349	12.73%	1.464%
33	9.240	1083	1089	1097	rBB	42724	70528	19.80%	2.277%
34	9.957	1206	1211	1219	rBB	35078	61820	17.35%	1.996%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021475.D
 Acq On : 22 Mar 2016 15:38
 Operator : UM/SJ
 Sample : H1835-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	10.574	1310	1316	1324	rBV	47828	84906	23.83%	2.741%
36	10.626	1324	1325	1327	rVB	551	370	0.10%	0.012%
37	10.879	1361	1368	1376	rBB	59020	105890	29.72%	3.418%
38	11.026	1389	1393	1399	rBB	1089	1878	0.53%	0.061%
39	12.454	1634	1636	1639	rBB2	432	487	0.14%	0.016%
40	14.087	1908	1914	1921	rBB	123386	168197	47.21%	5.429%
41	14.381	1957	1964	1970	rBV	121536	181740	51.01%	5.867%
42	14.686	2009	2016	2023	rBB2	96188	154738	43.43%	4.995%
43	15.104	2083	2087	2096	rBB3	4612	8300	2.33%	0.268%
44	15.673	2177	2184	2191	rBB	157945	241258	67.71%	7.788%
45	15.797	2199	2205	2214	rBV	52128	79103	22.20%	2.553%
46	15.903	2222	2223	2227	rBB	936	991	0.28%	0.032%
47	17.424	2475	2482	2488	rBV	129405	196021	55.02%	6.328%
48	17.518	2491	2498	2508	rBV2	193511	291212	81.73%	9.400%
49	18.030	2583	2585	2588	rBV	352	441	0.12%	0.014%
50	18.206	2611	2615	2616	rVV	438	447	0.13%	0.014%
51	18.306	2629	2632	2636	rVV2	329	488	0.14%	0.016%
52	18.370	2640	2643	2646	rVB	653	888	0.25%	0.029%
53	18.635	2686	2688	2691	rBV	366	479	0.13%	0.015%
54	18.893	2729	2732	2735	rBV	334	389	0.11%	0.013%
55	18.981	2746	2747	2750	rBV	773	623	0.17%	0.020%
56	19.005	2750	2751	2754	rVV	605	484	0.14%	0.016%
57	19.093	2765	2766	2769	rBV2	524	375	0.11%	0.012%
58	19.216	2784	2787	2789	rBV	358	465	0.13%	0.015%
59	19.304	2800	2802	2804	rVB	687	535	0.15%	0.017%
60	19.369	2811	2813	2816	rBV2	573	528	0.15%	0.017%
61	19.434	2818	2824	2830	rBV2	2162	3439	0.97%	0.111%
62	19.540	2840	2842	2844	rBV2	595	483	0.14%	0.016%
63	19.581	2846	2849	2850	rVV	712	686	0.19%	0.022%
64	19.622	2853	2856	2858	rVB2	527	503	0.14%	0.016%
65	19.639	2858	2859	2860	rBV	794	362	0.10%	0.012%
66	19.681	2863	2866	2869	rVV2	1213	1522	0.43%	0.049%
67	19.710	2869	2871	2874	rVB2	524	476	0.13%	0.015%
68	19.798	2879	2886	2893	rVV	253615	356291	100.00%	11.501%
69	19.874	2897	2899	2902	rBV2	844	933	0.26%	0.030%
70	19.904	2902	2904	2906	rVB	424	383	0.11%	0.012%
71	19.945	2909	2911	2913	rBV3	561	555	0.16%	0.018%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021475.D
 Acq On : 22 Mar 2016 15:38
 Operator : UM/SJ
 Sample : H1835-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	19.974	2915	2916	2920	rVB2	991	888	0.25%	0.029%
73	20.015	2920	2923	2924	rBV3	874	879	0.25%	0.028%
74	20.039	2924	2927	2929	rVB3	768	876	0.25%	0.028%
75	20.121	2939	2941	2944	rBV3	589	495	0.14%	0.016%
76	20.151	2944	2946	2947	rBV2	561	440	0.12%	0.014%
77	20.180	2950	2951	2954	rBV	867	864	0.24%	0.028%
78	20.297	2970	2971	2974	rBV3	1095	695	0.20%	0.022%
79	20.527	3008	3010	3012	rBV3	890	860	0.24%	0.028%
80	20.697	3036	3039	3040	rBV3	1212	1282	0.36%	0.041%
81	20.826	3059	3061	3062	rBV2	1464	735	0.21%	0.024%
82	20.955	3081	3083	3084	rBV	1442	1007	0.28%	0.033%
83	21.672	3199	3205	3213	rVB	154968	247279	69.40%	7.982%
84	21.937	3248	3250	3252	rBV3	2395	2363	0.66%	0.076%
85	24.322	3654	3656	3659	rBV3	2674	2734	0.77%	0.088%
86	24.669	3705	3715	3725	rBV	131550	347402	97.51%	11.214%
87	24.892	3744	3753	3763	rVB	86092	230380	64.66%	7.437%
88	26.431	4013	4015	4018	rBV4	2792	2635	0.74%	0.085%


Sum of corrected areas: 3097854

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021475.D
Acq On : 22 Mar 2016 15:38
Operator : UM/SJ
Sample : H1835-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T33

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

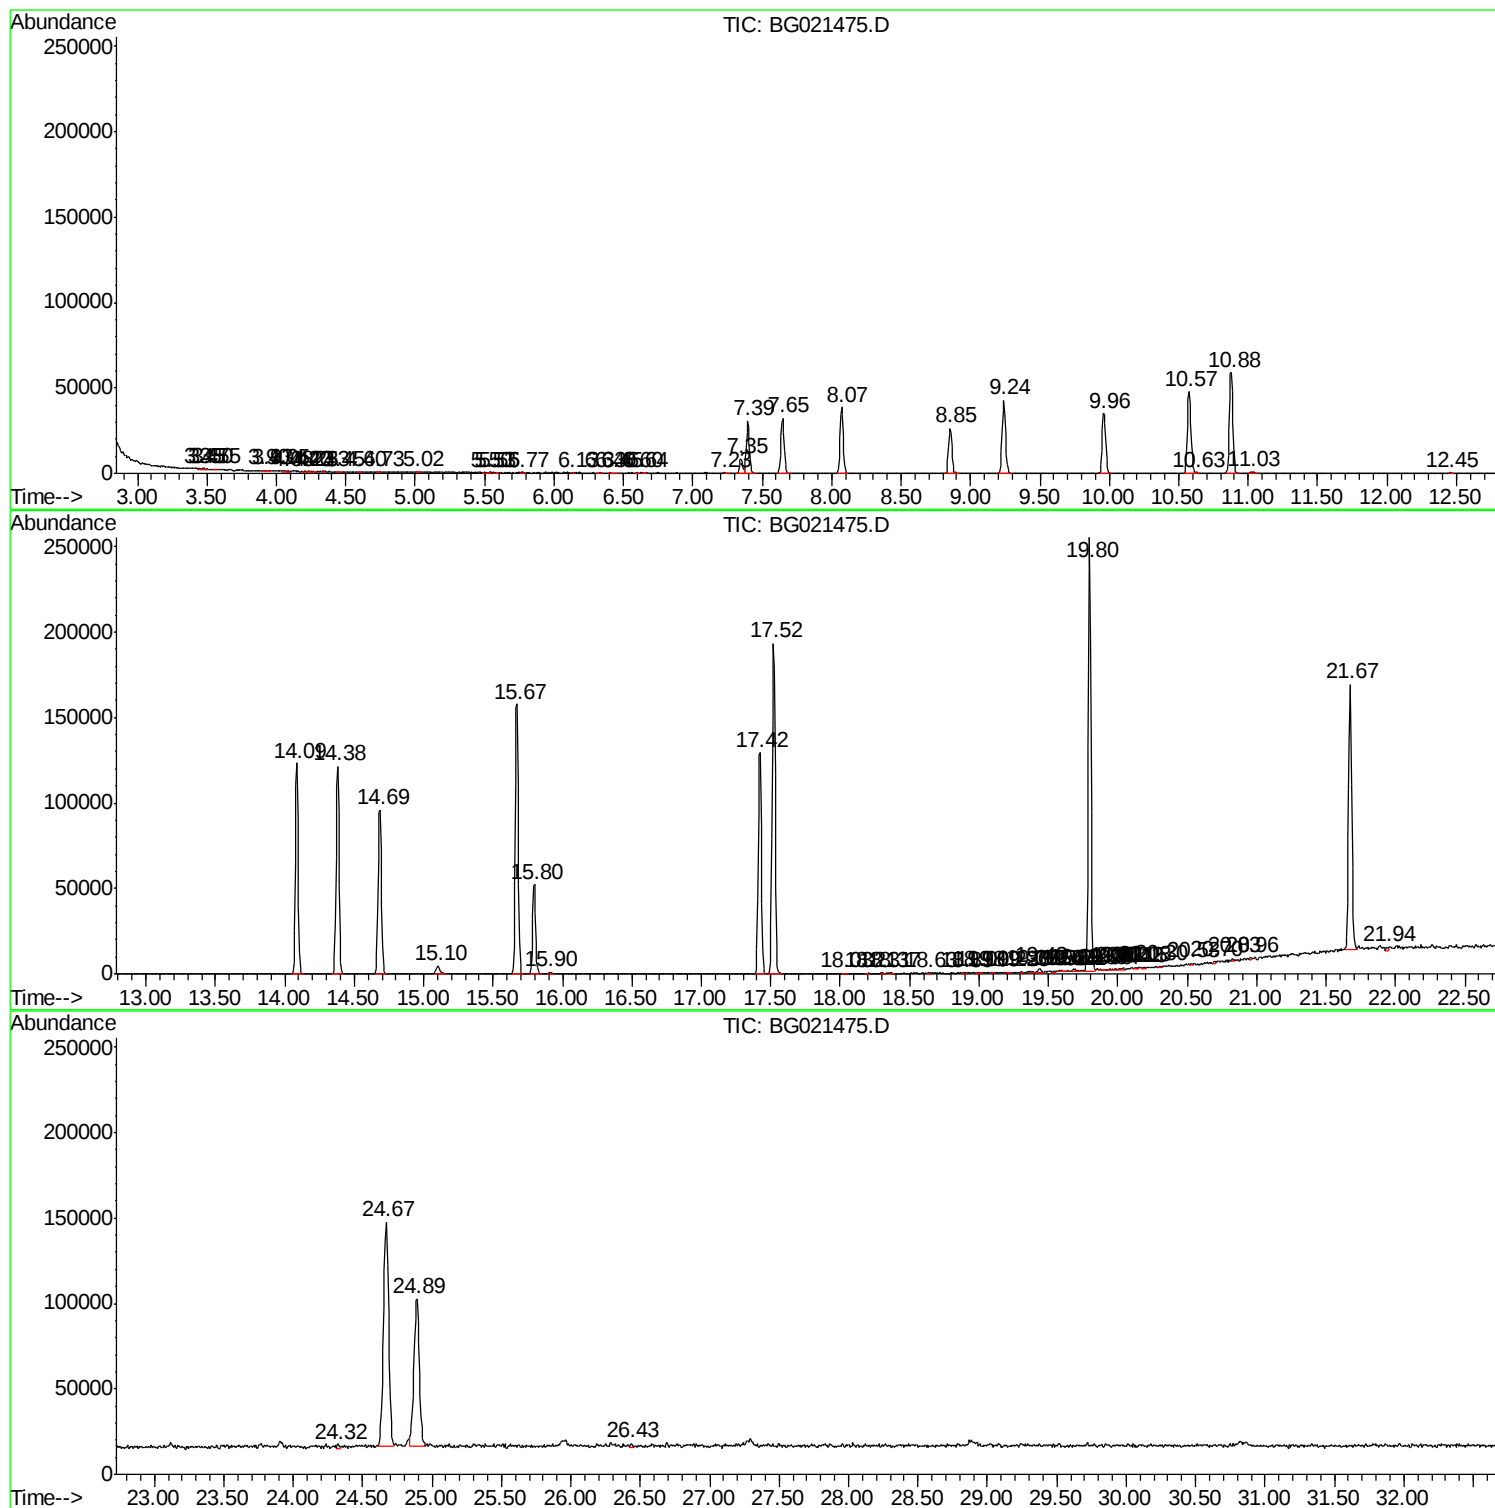

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021475.D
Acq On : 22 Mar 2016 15:38
Operator : UM/SJ
Sample : H1835-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T33

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021475.D
Acq On : 22 Mar 2016 15:38
Operator : UM/SJ
Sample : H1835-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T33

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc