

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021476.D
 Acq On : 22 Mar 2016 16:18
 Operator : UM/SJ
 Sample : H1835-23
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.655	137	139	143	rVB3	566	505	0.15%	0.017%
2	3.714	148	149	151	rBV	695	518	0.15%	0.017%
3	3.814	164	166	169	rVB3	503	399	0.11%	0.013%
4	3.843	169	171	173	rBV2	426	390	0.11%	0.013%
5	3.879	176	177	182	rBV3	528	512	0.15%	0.017%
6	3.990	194	196	200	rBV2	604	755	0.22%	0.025%
7	4.037	201	204	205	rVV2	433	367	0.11%	0.012%
8	4.055	205	207	209	rVV	486	459	0.13%	0.015%
9	4.084	209	212	215	rVB2	393	429	0.12%	0.014%
10	4.184	225	229	230	rBV3	623	508	0.15%	0.017%
11	4.231	235	237	238	rBV2	375	377	0.11%	0.012%
12	4.372	258	261	263	rBV2	274	370	0.11%	0.012%
13	4.431	270	271	274	rBV3	409	436	0.13%	0.014%
14	4.560	291	293	296	rVB2	378	384	0.11%	0.013%
15	4.719	318	320	324	rVB2	454	629	0.18%	0.021%
16	4.777	328	330	333	rVB2	337	381	0.11%	0.012%
17	5.400	434	436	440	rVB	385	364	0.10%	0.012%
18	5.665	478	481	482	rVB	594	427	0.12%	0.014%
19	5.894	518	520	521	rBV	466	448	0.13%	0.015%
20	6.193	568	571	573	rVB	394	370	0.11%	0.012%
21	6.323	590	593	595	rBV	410	406	0.12%	0.013%
22	6.411	605	608	609	rBV	361	435	0.13%	0.014%
23	6.428	609	611	614	rVB	552	627	0.18%	0.021%
24	6.523	623	627	628	rBB	423	457	0.13%	0.015%
25	6.669	651	652	654	rBV	564	399	0.11%	0.013%
26	6.758	664	667	670	rBB	354	426	0.12%	0.014%
27	7.345	762	767	771	rBV2	8215	13769	3.96%	0.451%
28	7.398	771	776	783	rVB	29610	47847	13.76%	1.566%
29	7.645	811	818	825	rBB	31063	50556	14.53%	1.655%
30	7.839	848	851	854	rBB	329	394	0.11%	0.013%
31	8.074	884	891	898	rBV	37301	60888	17.50%	1.993%
32	8.849	1018	1023	1030	rBV	27563	47651	13.70%	1.560%
33	9.237	1083	1089	1097	rBV	39934	69310	19.93%	2.269%
34	9.960	1206	1212	1219	rBB	37234	61549	17.69%	2.015%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021476.D
 Acq On : 22 Mar 2016 16:18
 Operator : UM/SJ
 Sample : H1835-23
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	10.571	1310	1316	1329	rBB	49205	89399	25.70%	2.926%
36	10.876	1361	1368	1376	rBB	57838	102003	29.33%	3.339%
37	12.451	1634	1636	1639	rBB	436	424	0.12%	0.014%
38	13.573	1823	1827	1830	rBB	1192	1461	0.42%	0.048%
39	14.084	1908	1914	1921	rBB	122319	172427	49.57%	5.644%
40	14.378	1958	1964	1973	rBV	123134	188912	54.31%	6.184%
41	14.684	2010	2016	2023	rBV2	94718	147706	42.46%	4.835%
42	15.101	2083	2087	2094	rBV2	4943	8818	2.54%	0.289%
43	15.671	2178	2184	2193	rBB	173588	251409	72.28%	8.230%
44	15.794	2200	2205	2213	rBB	54039	78400	22.54%	2.566%
45	15.906	2222	2224	2228	rBB2	850	1020	0.29%	0.033%
46	17.210	2443	2446	2449	rBB	261	363	0.10%	0.012%
47	17.422	2476	2482	2491	rBB	130805	186447	53.60%	6.103%
48	17.521	2491	2499	2512	rBB	187840	281610	80.96%	9.218%
49	18.021	2581	2584	2585	rBV	435	408	0.12%	0.013%
50	18.132	2600	2603	2604	rVB	439	352	0.10%	0.012%
51	18.156	2604	2607	2608	rBB	416	392	0.11%	0.013%
52	18.185	2608	2612	2613	rBV	365	448	0.13%	0.015%
53	18.315	2633	2634	2638	rVB	414	523	0.15%	0.017%
54	18.362	2638	2642	2644	rBV	689	852	0.24%	0.028%
55	18.438	2653	2655	2658	rBV	324	373	0.11%	0.012%
56	18.479	2658	2662	2666	rBV2	755	1227	0.35%	0.040%
57	18.608	2683	2684	2687	rVB	365	357	0.10%	0.012%
58	18.761	2707	2710	2714	rVB	606	569	0.16%	0.019%
59	18.802	2714	2717	2719	rBV	478	530	0.15%	0.017%
60	18.931	2737	2739	2741	rBV	299	372	0.11%	0.012%
61	19.108	2768	2769	2772	rVB2	411	377	0.11%	0.012%
62	19.131	2772	2773	2776	rBV	318	370	0.11%	0.012%
63	19.243	2788	2792	2793	rVV2	448	531	0.15%	0.017%
64	19.272	2796	2797	2800	rBV	765	515	0.15%	0.017%
65	19.343	2806	2809	2813	rBV2	705	1053	0.30%	0.034%
66	19.390	2816	2817	2819	rBV2	410	385	0.11%	0.013%
67	19.437	2821	2825	2829	rVV2	3078	3507	1.01%	0.115%
68	19.466	2829	2830	2833	rVB	500	352	0.10%	0.012%
69	19.501	2833	2836	2839	rVB2	662	925	0.27%	0.030%
70	19.525	2839	2840	2842	rBV	430	415	0.12%	0.014%
71	19.637	2857	2859	2861	rVB2	597	360	0.10%	0.012%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021476.D
 Acq On : 22 Mar 2016 16:18
 Operator : UM/SJ
 Sample : H1835-23
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T34

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	19.666	2861	2864	2865	rBV2	719	642	0.18%	0.021%
73	19.684	2865	2867	2872	rBV4	1807	2083	0.60%	0.068%
74	19.731	2872	2875	2876	rBV	586	511	0.15%	0.017%
75	19.795	2880	2886	2896	rBV	248104	347833	100.00%	11.386%
76	19.872	2896	2899	2901	rBV2	590	610	0.18%	0.020%
77	19.895	2901	2903	2905	rVB2	1063	864	0.25%	0.028%
78	19.913	2905	2906	2909	rBV2	661	645	0.19%	0.021%
79	19.942	2909	2911	2913	rBV3	522	593	0.17%	0.019%
80	20.001	2919	2921	2923	rBV2	790	532	0.15%	0.017%
81	20.024	2923	2925	2926	rBV2	539	411	0.12%	0.013%
82	20.101	2936	2938	2941	rBV4	918	1175	0.34%	0.038%
83	20.130	2941	2943	2945	rBV3	792	659	0.19%	0.022%
84	20.154	2945	2947	2949	rBV2	803	879	0.25%	0.029%
85	20.201	2954	2955	2958	rBV2	901	617	0.18%	0.020%
86	20.465	2998	3000	3001	rVB2	1039	526	0.15%	0.017%
87	20.524	3008	3010	3011	rBV	991	570	0.16%	0.019%
88	20.624	3025	3027	3029	rBV3	960	830	0.24%	0.027%
89	20.735	3042	3046	3047	rBV3	1624	1446	0.42%	0.047%
90	20.870	3068	3069	3071	rBV2	1727	1472	0.42%	0.048%
91	21.675	3199	3206	3214	rBV	145465	241116	69.32%	7.893%
92	24.507	3686	3688	3691	rBV3	2668	3220	0.93%	0.105%
93	24.672	3707	3716	3726	rVB	119374	325985	93.72%	10.671%
94	24.760	3729	3731	3735	rBV3	3067	3491	1.00%	0.114%
95	24.889	3745	3753	3767	rVB2	79435	227164	65.31%	7.436%
96	26.082	3954	3956	3958	rVB2	3195	1740	0.50%	0.057%


Sum of corrected areas: 3054948

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021476.D
Acq On : 22 Mar 2016 16:18
Operator : UM/SJ
Sample : H1835-23
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T34

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

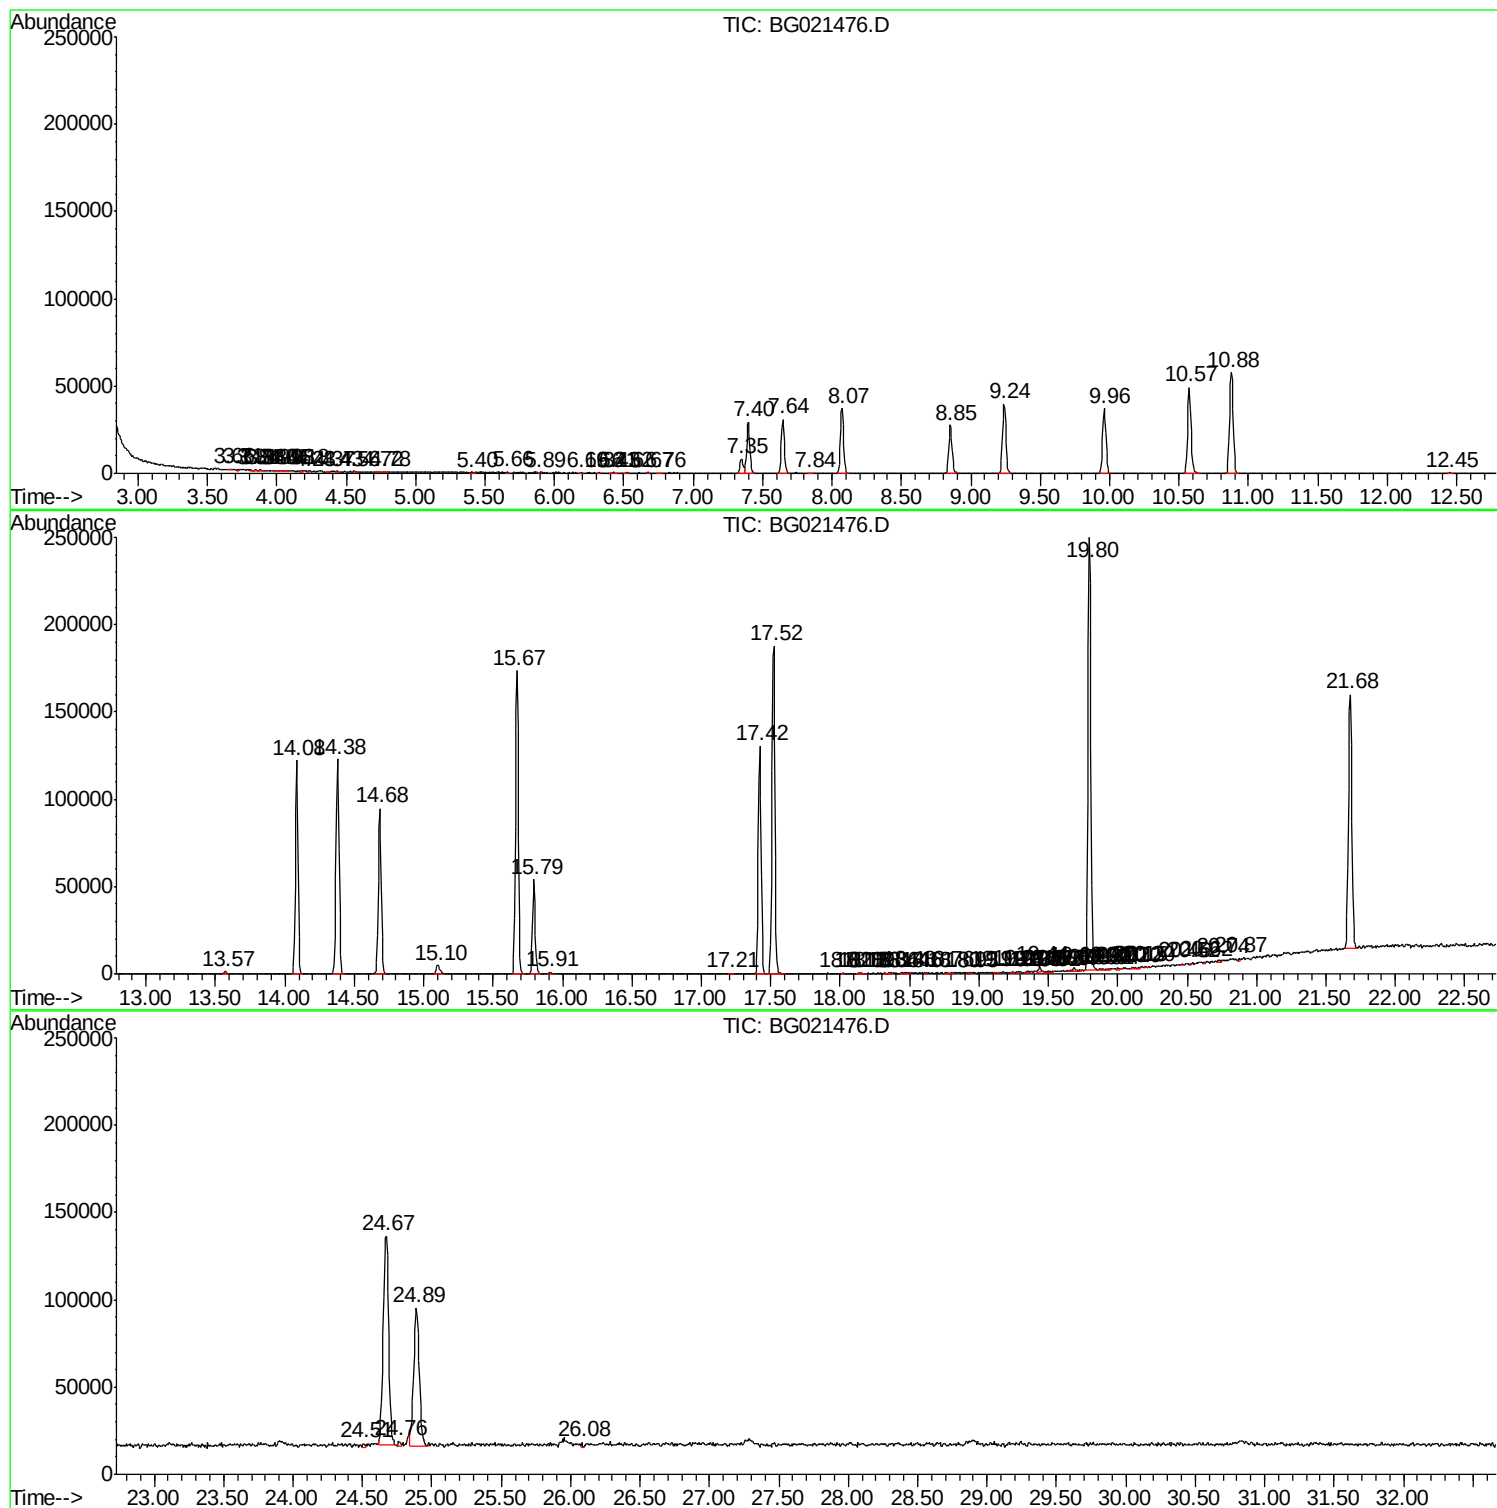

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021476.D
Acq On : 22 Mar 2016 16:18
Operator : UM/SJ
Sample : H1835-23
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T34

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021476.D
Acq On : 22 Mar 2016 16:18
Operator : UM/SJ
Sample : H1835-23
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T34

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc