

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021477.D
 Acq On : 22 Mar 2016 16:57
 Operator : UM/SJ
 Sample : H1835-24
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.195	58	61	65	rVB2	615	978	0.29%	0.032%
2	3.624	132	134	137	rVB3	472	357	0.11%	0.012%
3	3.660	138	140	142	rVB2	450	379	0.11%	0.012%
4	3.754	155	156	157	rBV	788	383	0.11%	0.012%
5	3.801	160	164	166	rBV3	554	841	0.25%	0.027%
6	4.130	217	220	223	rBV2	318	481	0.14%	0.016%
7	4.159	223	225	228	rVB	411	343	0.10%	0.011%
8	4.406	264	267	270	rBV2	330	421	0.12%	0.014%
9	4.523	284	287	291	rBV2	341	444	0.13%	0.014%
10	4.617	302	303	307	rVB2	282	344	0.10%	0.011%
11	4.658	307	310	311	rBV	406	362	0.11%	0.012%
12	4.811	334	336	340	rBV2	353	472	0.14%	0.015%
13	4.964	359	362	365	rVB	462	493	0.15%	0.016%
14	4.999	365	368	370	rBV2	417	450	0.13%	0.015%
15	5.093	380	384	387	rVB2	449	614	0.18%	0.020%
16	5.181	396	399	401	rBV2	445	625	0.18%	0.020%
17	5.228	406	407	408	rBV2	683	407	0.12%	0.013%
18	5.487	447	451	453	rBV2	290	348	0.10%	0.011%
19	5.534	458	459	462	rBV2	481	510	0.15%	0.016%
20	5.598	468	470	472	rVB2	572	522	0.15%	0.017%
21	5.622	472	474	476	rBV2	491	461	0.14%	0.015%
22	5.692	482	486	487	rVB2	594	536	0.16%	0.017%
23	5.704	487	488	491	rBV2	423	476	0.14%	0.015%
24	5.834	507	510	514	rVB	491	635	0.19%	0.021%
25	5.939	526	528	531	rVB	394	391	0.12%	0.013%
26	5.986	534	536	539	rBV	255	354	0.10%	0.011%
27	6.039	541	545	546	rVB	431	437	0.13%	0.014%
28	6.092	552	554	556	rVB	407	363	0.11%	0.012%
29	6.151	562	564	566	rBB	350	340	0.10%	0.011%
30	6.210	570	574	575	rBB	408	375	0.11%	0.012%
31	6.233	575	578	581	rBB	398	377	0.11%	0.012%
32	6.274	582	585	587	rBB	415	359	0.11%	0.012%
33	6.386	601	604	607	rBB	345	406	0.12%	0.013%
34	7.349	762	768	771	rBV2	8440	13197	3.89%	0.426%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021477.D
 Acq On : 22 Mar 2016 16:57
 Operator : UM/SJ
 Sample : H1835-24
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	7.396	771	776	784	rVB	32920	54432	16.06%	1.758%
36	7.643	813	818	827	rBB	34371	57766	17.04%	1.865%
37	8.072	885	891	899	rBB	39391	64614	19.06%	2.086%
38	8.854	1018	1024	1032	rBV2	26949	47491	14.01%	1.533%
39	9.241	1083	1090	1099	rBB	46991	80999	23.89%	2.615%
40	9.958	1207	1212	1220	rBB2	40157	70070	20.67%	2.262%
41	10.575	1310	1317	1326	rBV	51065	91248	26.92%	2.946%
42	10.875	1361	1368	1376	rBV	65129	110217	32.51%	3.559%
43	12.455	1634	1637	1640	rBB	795	709	0.21%	0.023%
44	13.566	1824	1826	1829	rBB	686	657	0.19%	0.021%
45	14.083	1908	1914	1922	rBB	129881	182525	53.84%	5.893%
46	14.376	1958	1964	1974	rBB	131395	203280	59.96%	6.564%
47	14.682	2010	2016	2023	rBB2	104808	160832	47.44%	5.193%
48	15.105	2083	2088	2097	rBB3	4236	6975	2.06%	0.225%
49	15.669	2178	2184	2193	rBB	179990	267964	79.04%	8.652%
50	15.792	2200	2205	2215	rBB	52963	77928	22.99%	2.516%
51	15.916	2221	2226	2229	rBB	828	1090	0.32%	0.035%
52	17.203	2444	2445	2449	rBB	395	461	0.14%	0.015%
53	17.420	2476	2482	2489	rBV	125725	178009	52.51%	5.748%
54	17.520	2492	2499	2507	rBV	204532	294864	86.98%	9.521%
55	18.037	2585	2587	2590	rVB	435	351	0.10%	0.011%
56	18.154	2604	2607	2608	rBV	387	356	0.11%	0.011%
57	18.237	2618	2621	2624	rVB	384	486	0.14%	0.016%
58	18.307	2630	2633	2635	rVV	425	340	0.10%	0.011%
59	18.366	2640	2643	2646	rVV	441	597	0.18%	0.019%
60	18.425	2649	2653	2656	rVV	304	351	0.10%	0.011%
61	18.654	2689	2692	2694	rBV	339	351	0.10%	0.011%
62	18.777	2709	2713	2714	rVB	404	484	0.14%	0.016%
63	19.006	2749	2752	2753	rBV	496	491	0.14%	0.016%
64	19.053	2757	2760	2762	rBV	462	427	0.13%	0.014%
65	19.094	2764	2767	2769	rBV	542	603	0.18%	0.019%
66	19.230	2787	2790	2791	rBV2	749	495	0.15%	0.016%
67	19.253	2791	2794	2795	rBV2	507	488	0.14%	0.016%
68	19.265	2795	2796	2800	rVV3	432	475	0.14%	0.015%
69	19.306	2800	2803	2804	rVV	428	518	0.15%	0.017%
70	19.353	2806	2811	2813	rBV	613	809	0.24%	0.026%
71	19.382	2813	2816	2817	rBV	488	414	0.12%	0.013%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021477.D
 Acq On : 22 Mar 2016 16:57
 Operator : UM/SJ
 Sample : H1835-24
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T35

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	19.400	2817	2819	2822	rVV2	315	359	0.11%	0.012%
73	19.435	2822	2825	2830	rVB	1760	2126	0.63%	0.069%
74	19.488	2830	2834	2835	rVB2	606	476	0.14%	0.015%
75	19.529	2839	2841	2842	rVV2	694	447	0.13%	0.014%
76	19.635	2857	2859	2861	rBV2	786	608	0.18%	0.020%
77	19.682	2864	2867	2872	rVV2	1040	1461	0.43%	0.047%
78	19.729	2872	2875	2876	rVB2	760	630	0.19%	0.020%
79	19.794	2880	2886	2896	rBV	231568	339012	100.00%	10.946%
80	19.923	2906	2908	2909	rBV2	685	482	0.14%	0.016%
81	19.935	2909	2910	2912	rBV2	680	572	0.17%	0.018%
82	19.982	2917	2918	2920	rBV2	839	624	0.18%	0.020%
83	20.035	2925	2927	2931	rBV4	1058	1406	0.41%	0.045%
84	20.087	2934	2936	2938	rBV2	1018	930	0.27%	0.030%
85	20.111	2938	2940	2941	rBV	717	462	0.14%	0.015%
86	20.176	2948	2951	2952	rBV3	658	757	0.22%	0.024%
87	20.270	2965	2967	2968	rVB2	882	489	0.14%	0.016%
88	20.358	2980	2982	2983	rBV	735	499	0.15%	0.016%
89	20.387	2985	2987	2989	rBV4	930	635	0.19%	0.021%
90	21.674	3200	3206	3213	rBV	136920	223410	65.90%	7.214%
91	24.664	3706	3715	3727	rVB	124675	328609	96.93%	10.610%
92	24.888	3746	3753	3766	rVB	73433	204420	60.30%	6.600%


Sum of corrected areas: 3097062

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021477.D
Acq On : 22 Mar 2016 16:57
Operator : UM/SJ
Sample : H1835-24
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T35

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

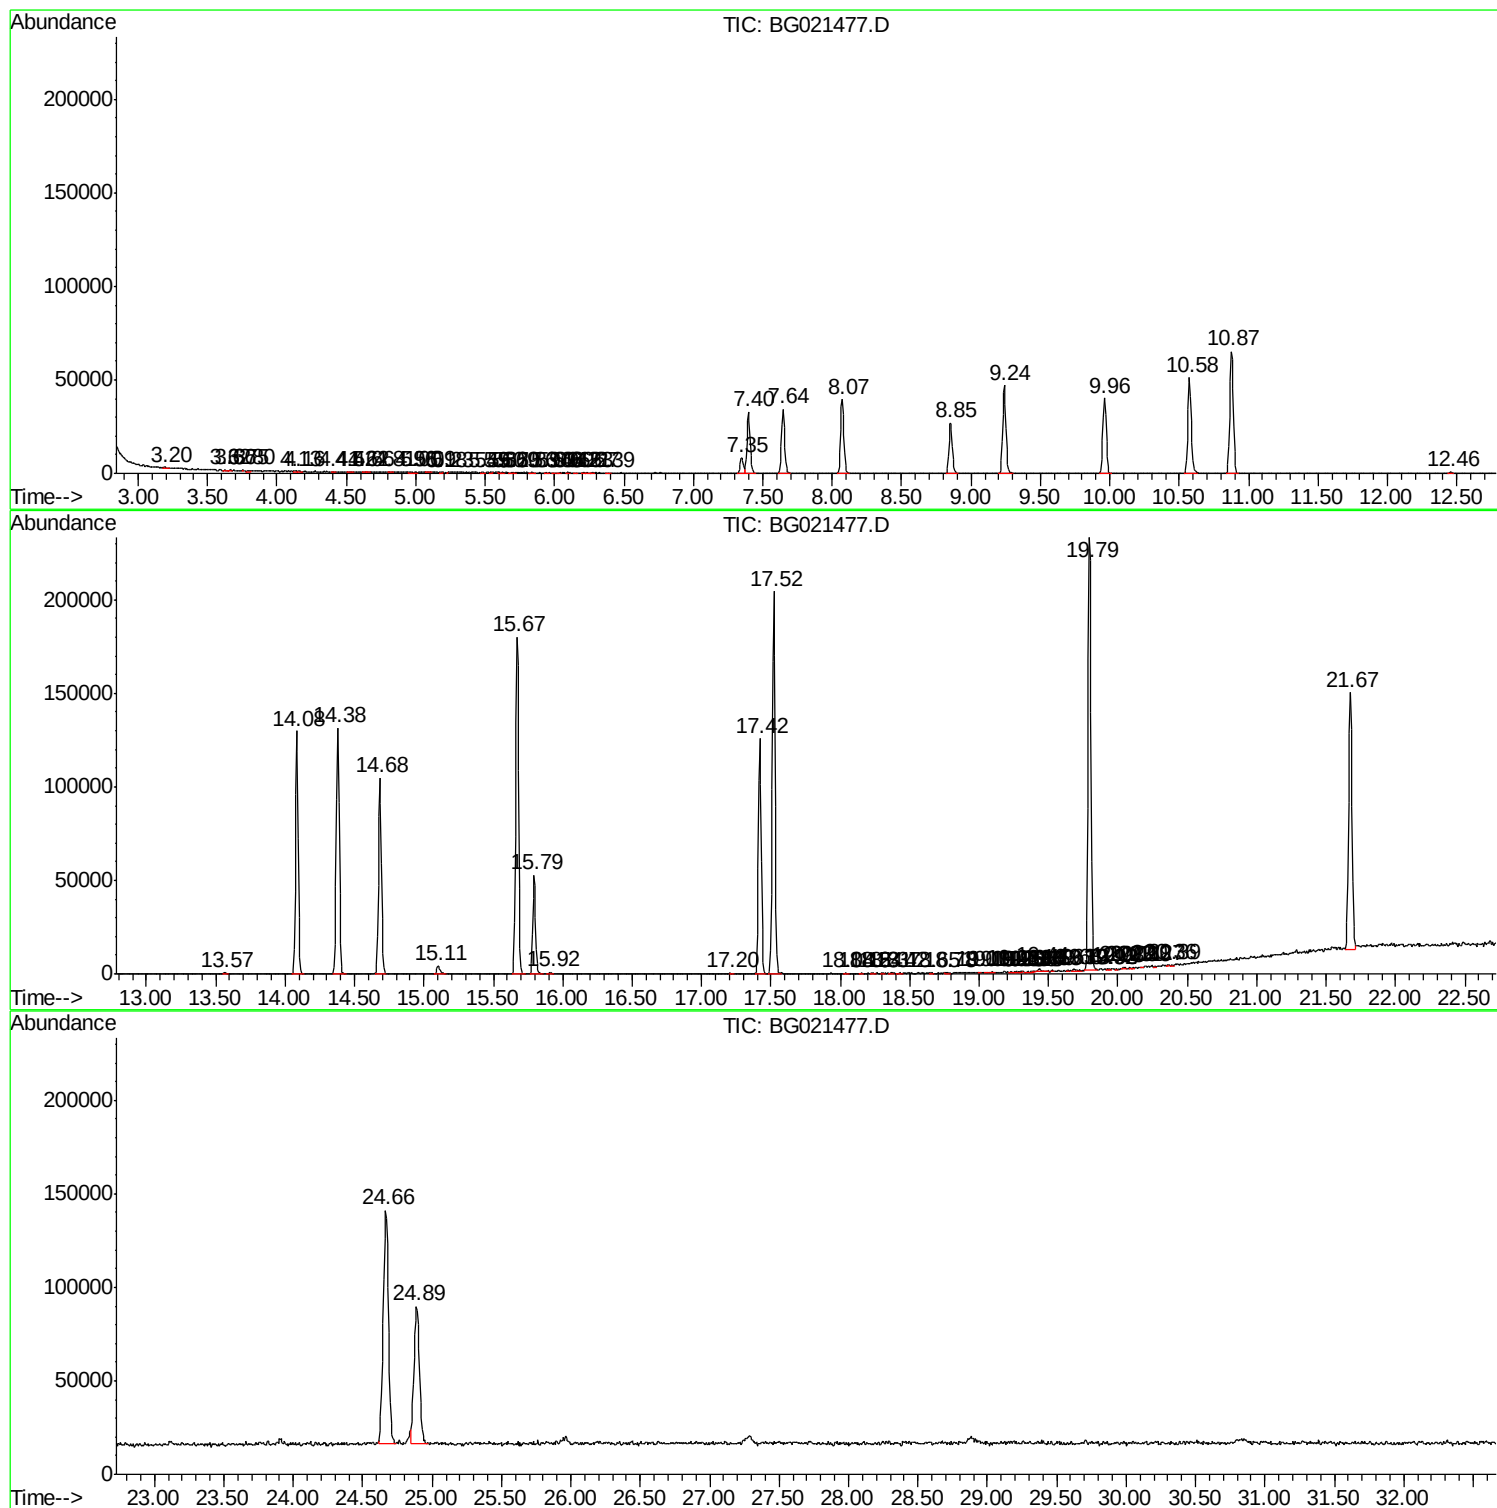

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021477.D
Acq On : 22 Mar 2016 16:57
Operator : UM/SJ
Sample : H1835-24
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T35

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021477.D
Acq On : 22 Mar 2016 16:57
Operator : UM/SJ
Sample : H1835-24
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T35

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc