

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021478.D
 Acq On : 22 Mar 2016 17:37
 Operator : UM/SJ
 Sample : H1835-25
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.056	35	37	39	rBV2	806	650	0.17%	0.021%
2	3.150	50	53	54	rBV3	712	630	0.17%	0.020%
3	3.273	73	74	76	rVB2	630	440	0.12%	0.014%
4	3.502	112	113	118	rBV2	662	902	0.24%	0.029%
5	3.561	121	123	124	rBV	713	531	0.14%	0.017%
6	3.743	150	154	156	rBV3	387	529	0.14%	0.017%
7	3.784	160	161	162	rBV	629	402	0.11%	0.013%
8	3.978	193	194	198	rBV3	383	458	0.12%	0.015%
9	4.360	256	259	260	rBV2	406	539	0.14%	0.017%
10	4.436	269	272	274	rBV2	434	479	0.13%	0.015%
11	4.619	300	303	304	rBV2	337	376	0.10%	0.012%
12	4.777	327	330	333	rVB2	477	691	0.19%	0.022%
13	4.936	351	357	362	rBV3	400	1014	0.27%	0.032%
14	4.983	362	365	367	rBV2	331	404	0.11%	0.013%
15	5.635	471	476	478	rVB3	304	472	0.13%	0.015%
16	5.747	493	495	498	rVB	465	483	0.13%	0.015%
17	5.782	498	501	503	rBV2	426	537	0.14%	0.017%
18	5.946	526	529	530	rBV	424	407	0.11%	0.013%
19	6.005	535	539	542	rVB	359	499	0.13%	0.016%
20	6.040	542	545	548	rBV2	382	587	0.16%	0.019%
21	6.140	558	562	564	rBV	362	450	0.12%	0.014%
22	6.340	594	596	600	rVB2	322	505	0.14%	0.016%
23	6.446	613	614	616	rBV2	408	377	0.10%	0.012%
24	6.516	623	626	628	rBV2	301	422	0.11%	0.013%
25	6.804	673	675	678	rBB2	485	392	0.10%	0.012%
26	7.345	763	767	771	rVV2	9027	14848	3.98%	0.471%
27	7.398	771	776	785	rVV	32600	53447	14.32%	1.694%
28	7.644	811	818	826	rBB	36648	60535	16.21%	1.919%
29	7.803	841	845	847	rBB	357	440	0.12%	0.014%
30	8.073	884	891	899	rBB	33227	56768	15.21%	1.800%
31	8.355	936	939	942	rBB	375	423	0.11%	0.013%
32	8.855	1018	1024	1032	rBB	32204	54863	14.70%	1.739%
33	9.243	1083	1090	1097	rBV	45842	80839	21.65%	2.563%
34	9.959	1206	1212	1220	rBB	40455	72108	19.31%	2.286%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021478.D
 Acq On : 22 Mar 2016 17:37
 Operator : UM/SJ
 Sample : H1835-25
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	10.570	1309	1316	1328	rBB	58775	106989	28.66%	3.392%
36	10.876	1361	1368	1378	rBB	53589	94147	25.22%	2.985%
37	12.456	1634	1637	1640	rBB	428	498	0.13%	0.016%
38	14.084	1908	1914	1922	rBB	132337	188339	50.45%	5.971%
39	14.378	1958	1964	1973	rBB	137991	213872	57.29%	6.780%
40	14.683	2010	2016	2023	rBB2	88277	136133	36.46%	4.316%
41	15.095	2083	2086	2095	rBB2	4879	9261	2.48%	0.294%
42	15.670	2178	2184	2192	rBB	195008	274034	73.40%	8.688%
43	15.794	2200	2205	2215	rBB	59827	85968	23.03%	2.725%
44	15.905	2221	2224	2228	rBB	985	1168	0.31%	0.037%
45	17.421	2476	2482	2489	rBV	116463	162376	43.49%	5.148%
46	17.521	2492	2499	2509	rBV	203715	299209	80.14%	9.486%
47	17.915	2565	2566	2569	rBV	380	406	0.11%	0.013%
48	18.361	2639	2642	2647	rVB2	741	930	0.25%	0.029%
49	18.444	2655	2656	2658	rBV	502	413	0.11%	0.013%
50	18.661	2690	2693	2694	rBV	461	411	0.11%	0.013%
51	18.837	2719	2723	2724	rVB	500	435	0.12%	0.014%
52	19.037	2753	2757	2760	rBV2	595	865	0.23%	0.027%
53	19.066	2760	2762	2764	rVV	510	393	0.11%	0.012%
54	19.096	2764	2767	2768	rVV	505	487	0.13%	0.015%
55	19.125	2770	2772	2774	rVV	641	534	0.14%	0.017%
56	19.190	2780	2783	2784	rBV2	494	401	0.11%	0.013%
57	19.231	2787	2790	2792	rBV	854	561	0.15%	0.018%
58	19.272	2792	2797	2798	rVV3	616	675	0.18%	0.021%
59	19.290	2798	2800	2803	rVB2	526	543	0.15%	0.017%
60	19.384	2814	2816	2820	rBV	625	878	0.24%	0.028%
61	19.437	2820	2825	2831	rVB4	1969	3463	0.93%	0.110%
62	19.542	2841	2843	2844	rBV	978	552	0.15%	0.017%
63	19.560	2844	2846	2850	rBV	1197	867	0.23%	0.027%
64	19.607	2850	2854	2856	rVB2	591	583	0.16%	0.018%
65	19.625	2856	2857	2859	rBV2	546	479	0.13%	0.015%
66	19.683	2861	2867	2871	rBV3	1445	2352	0.63%	0.075%
67	19.795	2880	2886	2894	rBV	266319	373341	100.00%	11.836%
68	19.854	2894	2896	2898	rVV2	1099	658	0.18%	0.021%
69	19.889	2901	2902	2904	rVV	851	538	0.14%	0.017%
70	19.907	2904	2905	2906	rVV	978	445	0.12%	0.014%
71	19.924	2906	2908	2910	rVB2	831	647	0.17%	0.021%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
 Data File : BG021478.D
 Acq On : 22 Mar 2016 17:37
 Operator : UM/SJ
 Sample : H1835-25
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	19.942	2910	2911	2913	rBV	520	474	0.13%	0.015%
73	19.977	2915	2917	2918	rBV2	958	549	0.15%	0.017%
74	19.989	2918	2919	2922	rBV3	825	851	0.23%	0.027%
75	20.065	2929	2932	2933	rBV2	891	862	0.23%	0.027%
76	20.159	2946	2948	2950	rBV2	757	465	0.12%	0.015%
77	20.183	2950	2952	2955	rVB3	662	455	0.12%	0.014%
78	20.212	2955	2957	2960	rBV3	965	1036	0.28%	0.033%
79	20.271	2964	2967	2970	rBV4	1008	1352	0.36%	0.043%
80	20.371	2982	2984	2987	rBV3	1077	1409	0.38%	0.045%
81	20.459	2998	2999	3001	rBV2	1055	500	0.13%	0.016%
82	20.482	3001	3003	3005	rBV2	1248	814	0.22%	0.026%
83	20.547	3012	3014	3015	rBV2	1127	840	0.22%	0.027%
84	20.994	3088	3090	3091	rBV2	1381	649	0.17%	0.021%
85	21.675	3200	3206	3212	rVB	130064	211128	56.55%	6.693%
86	22.327	3315	3317	3318	rBV2	2833	2154	0.58%	0.068%
87	23.050	3438	3440	3442	rBV3	3196	3689	0.99%	0.117%
88	24.672	3707	3716	3730	rVB	138138	359079	96.18%	11.384%
89	24.895	3745	3754	3764	rVB2	67729	194567	52.12%	6.168%
90	29.918	4607	4609	4613	rBV5	2658	2152	0.58%	0.068%


Sum of corrected areas: 3154323

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021478.D
Acq On : 22 Mar 2016 17:37
Operator : UM/SJ
Sample : H1835-25
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T36

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

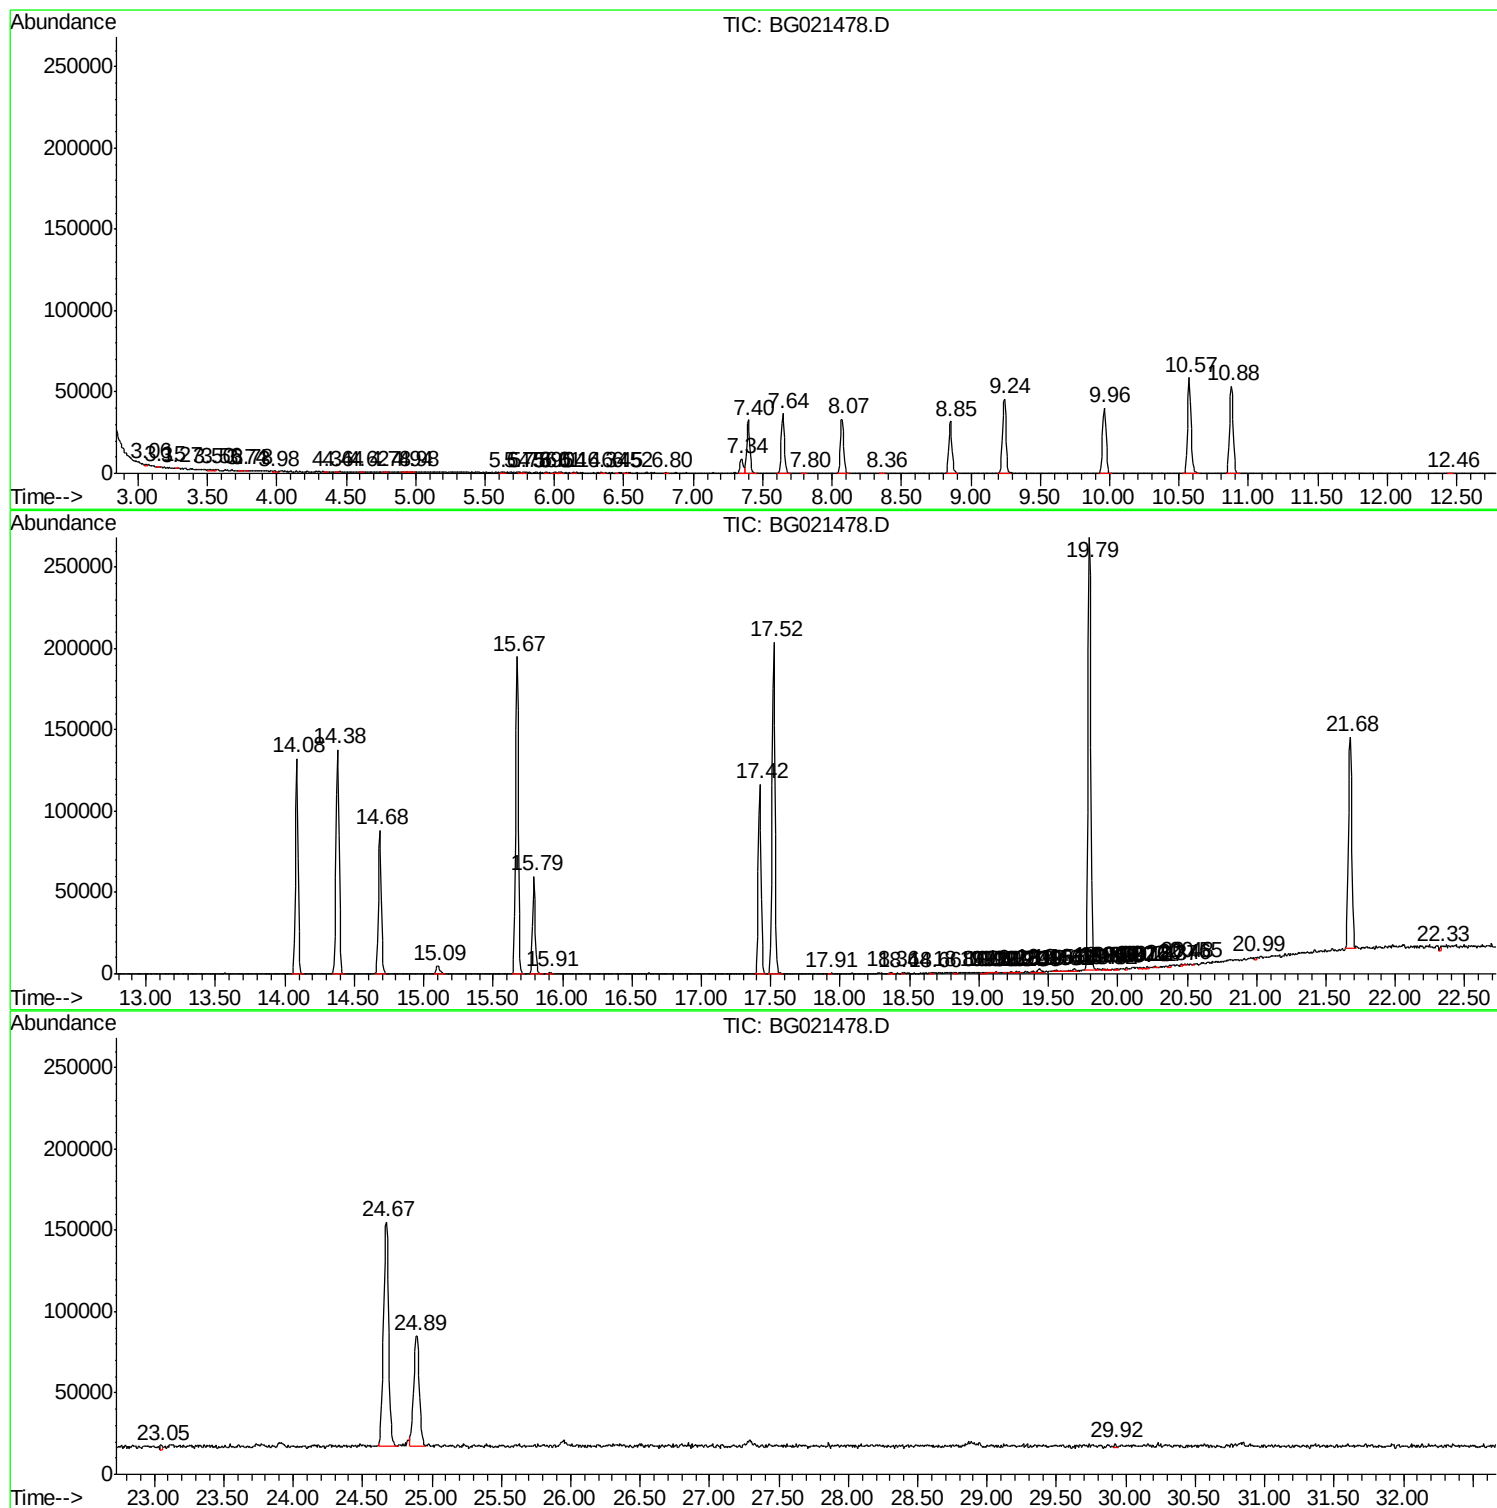

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021478.D
Acq On : 22 Mar 2016 17:37
Operator : UM/SJ
Sample : H1835-25
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T36

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032216\
Data File : BG021478.D
Acq On : 22 Mar 2016 17:37
Operator : UM/SJ
Sample : H1835-25
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T36

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc