
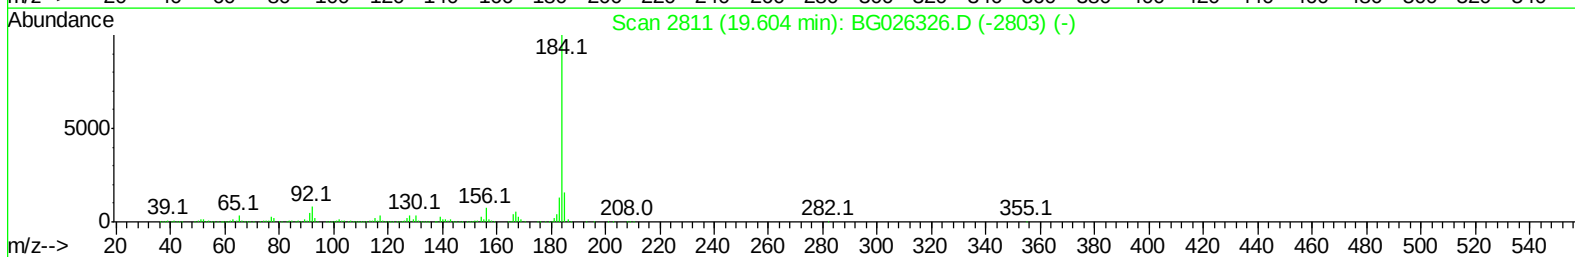
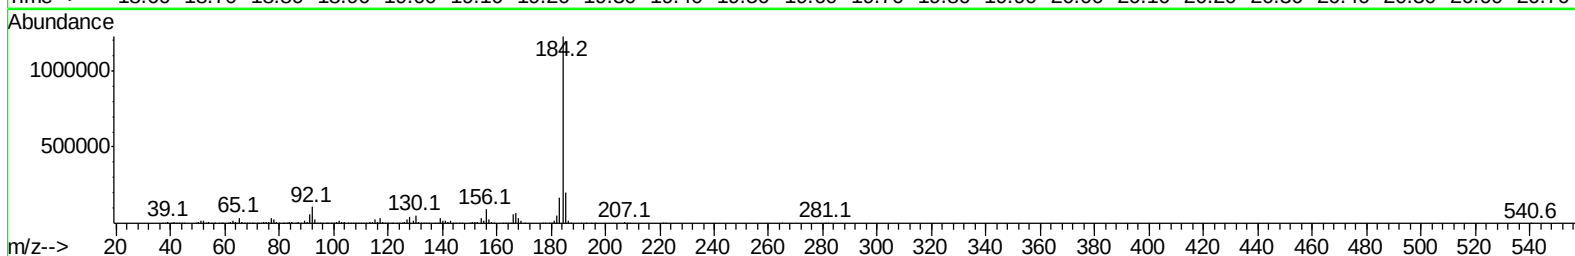


Data Path : Z:\HPCHEM1\BNA G\Data\BG032217\
Data File : BG026369.D
Acq On : 22 Mar 2017 8:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:24:22 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

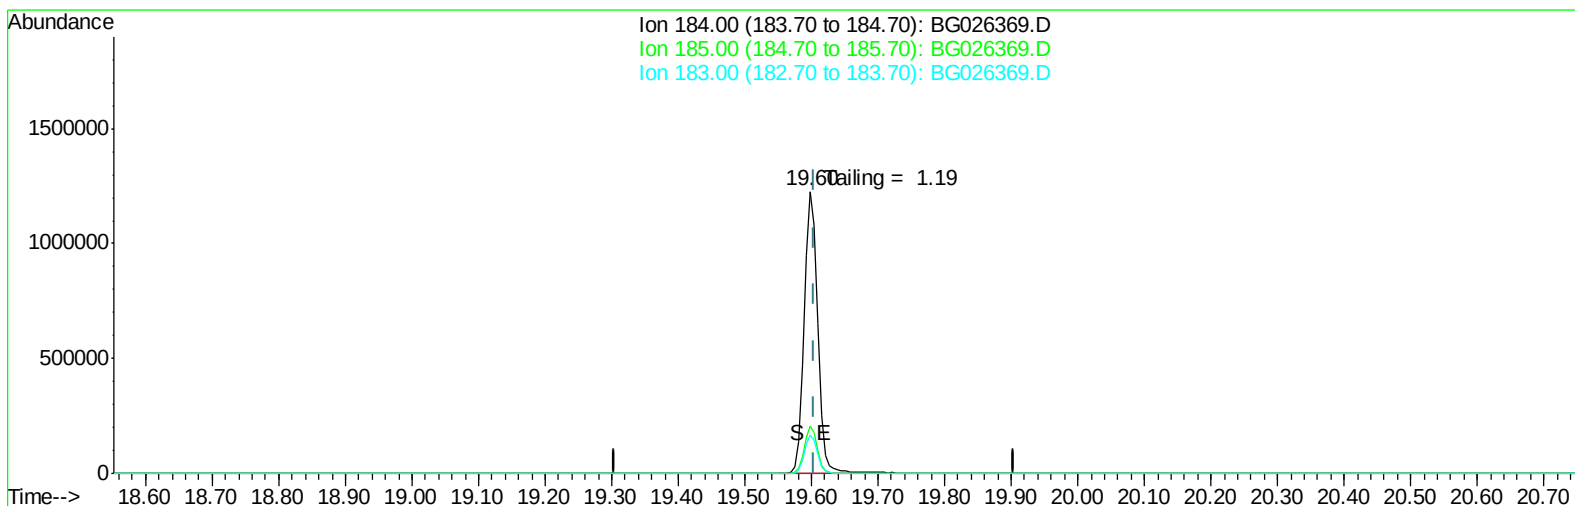

TIC: BG026369.D

(76) Benzidine




19.598min (-0.006) 4420.26ng

response 1774889

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.74
183.00	13.80	13.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG032217\
Data File : BG026369.D
Acq On : 22 Mar 2017 8:44
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:24:22 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

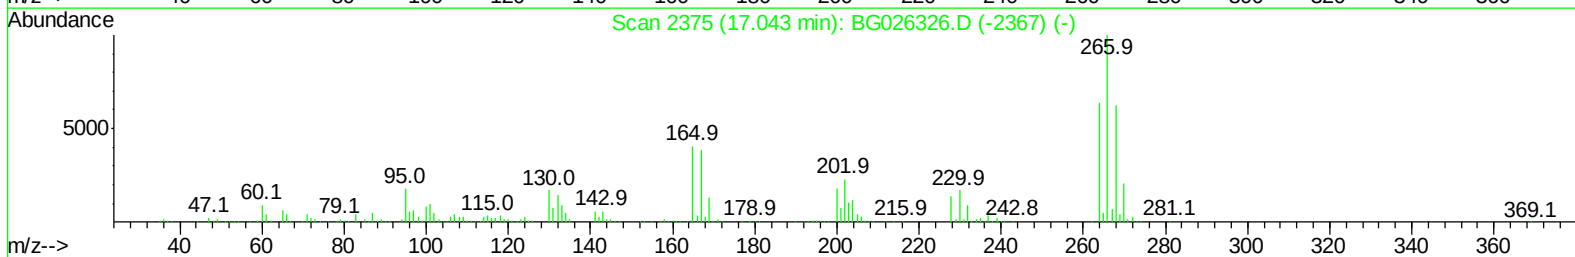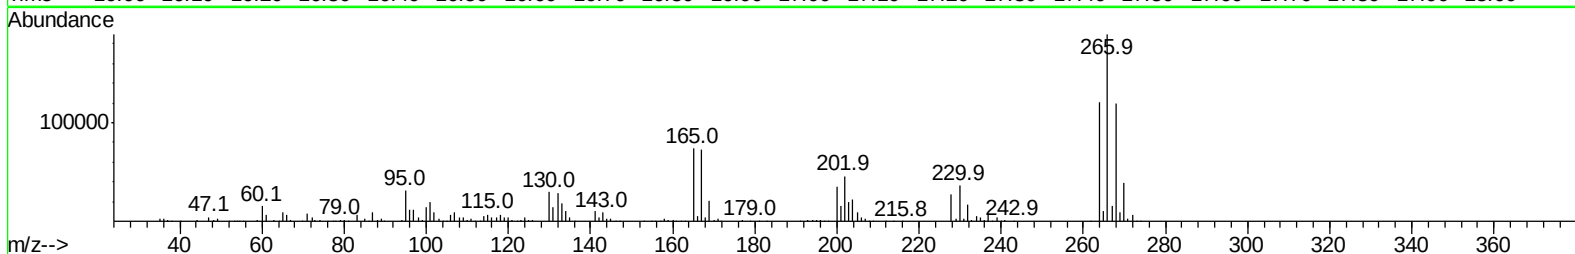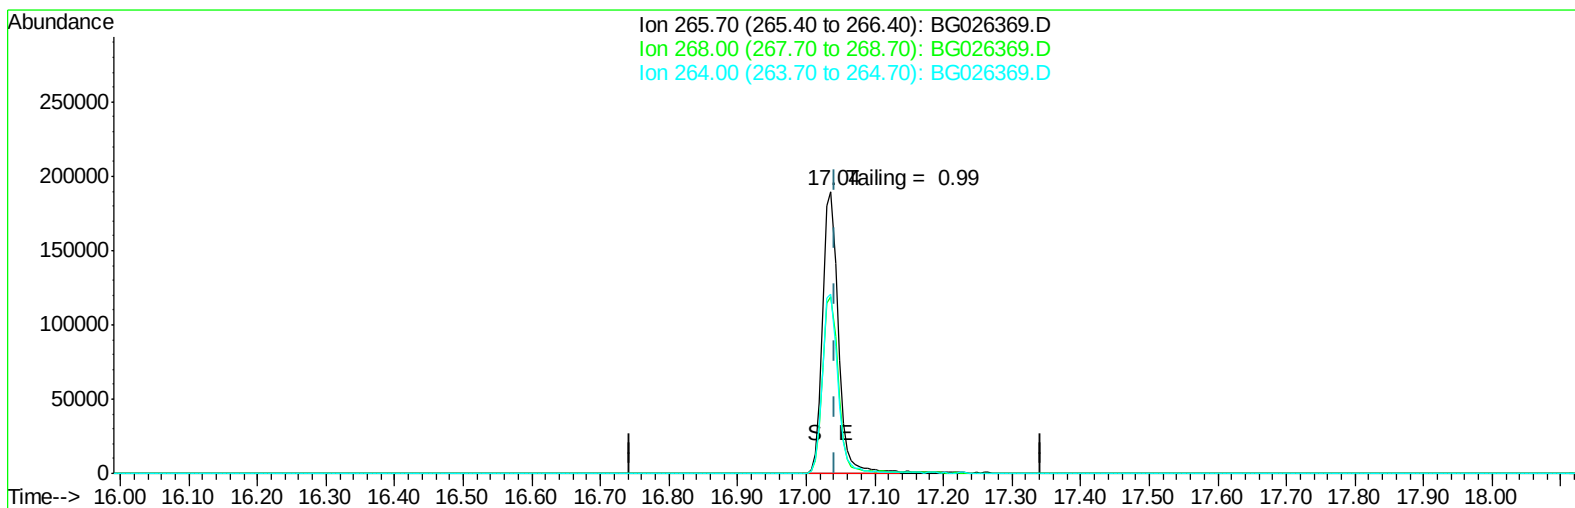

TIC: BG026369.D

(69) Pentachlorophenol (C)

17.036min (-0.006) 20022.12ng

response 299722

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.91
264.00	62.60	63.85
0.00	0.00	0.00