
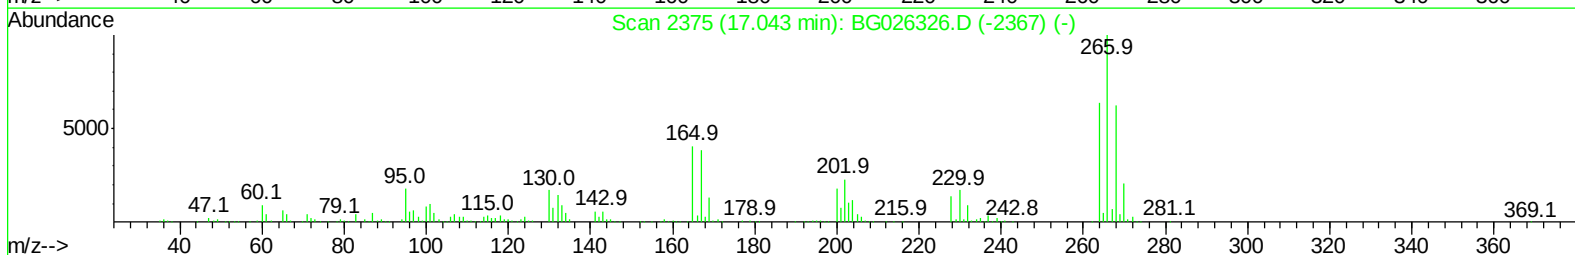
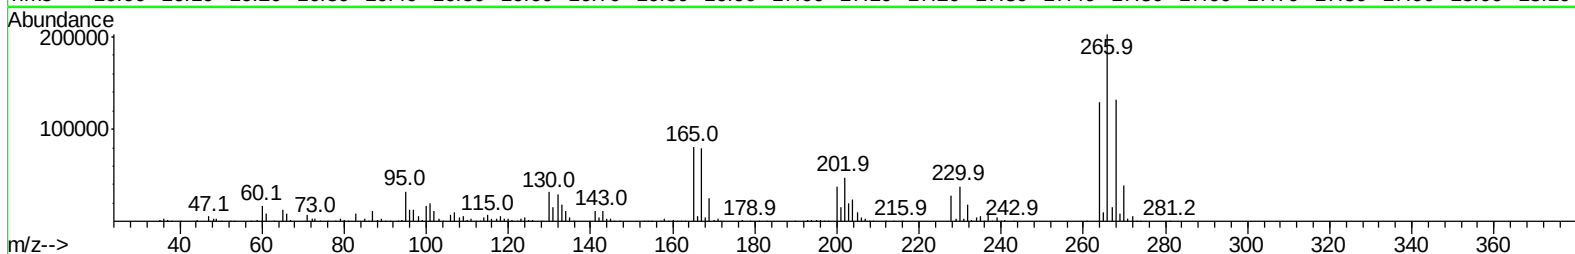


Data Path : Z:\HPCHEM1\BNA G\Data\BG032217\
Data File : BG026376.D
Acq On : 22 Mar 2017 15:18
Operator : SJ/MA
Sample : DFTPP
Misc : L00 20 PPB
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:25:01 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

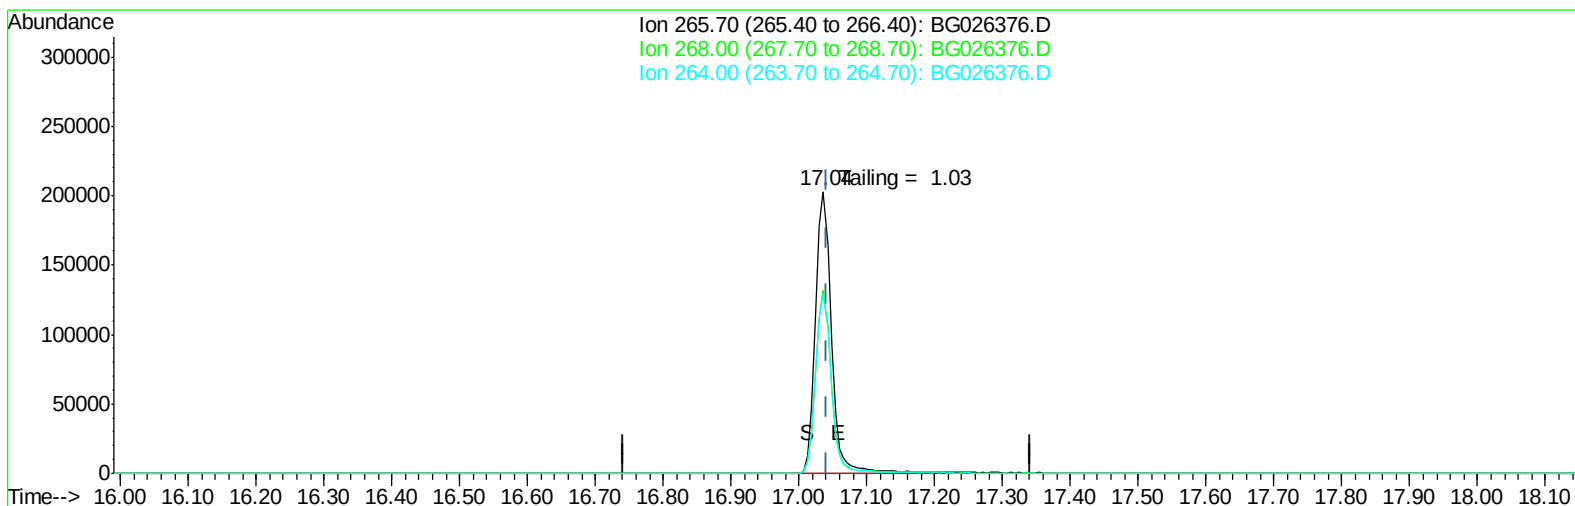

TIC: BG026376.D

(69) Pentachlorophenol (C)




17.036min (-0.006) 733845.70ng

response 324793

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	64.97
264.00	62.60	63.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG032217\
 Data File : BG026376.D
 Acq On : 22 Mar 2017 15:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc : L00 20 PPB
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:25:01 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 20 17:43:27 2017
 Response via : Initial Calibration

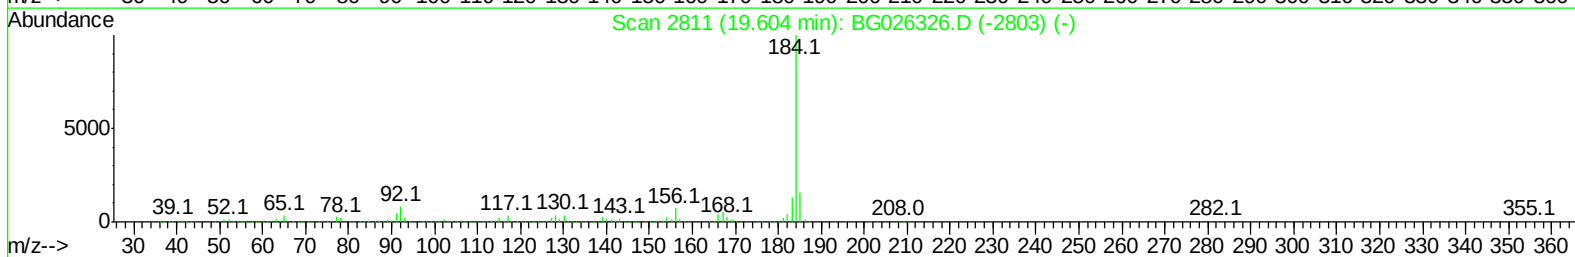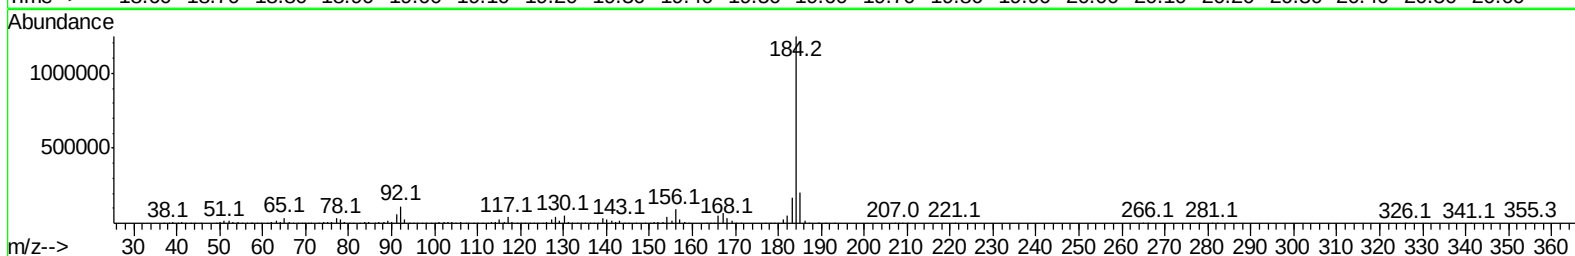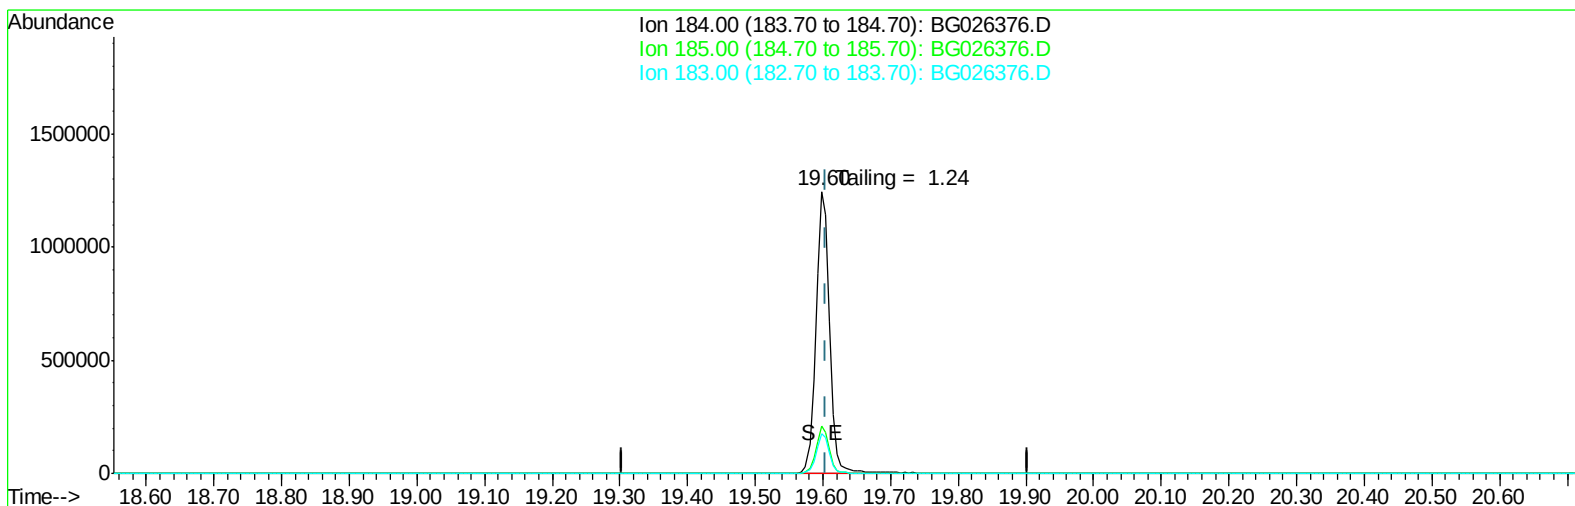

TIC: BG026376.D

(76) Benzidine

19.598min (-0.006) 32114.76ng

response 1770517

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.76
183.00	13.80	13.97
0.00	0.00	0.00