

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032217\
 Data File : BG026374.D
 Acq On : 22 Mar 2017 12:40
 Operator : SJ/MA
 Sample : I2332-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FK-SF-01-002-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.145	344	350	363	rBV	87883	140439	3.16%	0.475%
2	5.620	424	431	447	rBV	980908	1613597	36.34%	5.460%
3	7.207	694	701	718	rBV	1004932	1768170	39.82%	5.983%
4	7.583	758	765	775	rBV	1061914	1832462	41.27%	6.201%
5	8.047	837	844	854	rBV	433443	750115	16.89%	2.538%
6	8.370	892	899	910	rBV	797301	1412125	31.80%	4.779%
7	9.204	1033	1041	1056	rBV	594379	1088360	24.51%	3.683%
8	10.850	1313	1321	1328	rBV	705228	1263335	28.45%	4.275%
9	13.282	1728	1735	1747	rBV	2182403	3360512	75.68%	11.372%
10	14.099	1868	1874	1880	rBV	82870	125293	2.82%	0.424%
11	14.657	1959	1969	1977	rBV2	1180122	1890394	42.57%	6.397%
12	16.132	2212	2220	2234	rBV	1479729	2329233	52.45%	7.882%
13	16.343	2252	2256	2260	rBV2	33204	49373	1.11%	0.167%
14	17.383	2427	2433	2439	rBV2	1413944	2216470	49.91%	7.501%
15	19.428	2777	2781	2786	rVB	117938	163257	3.68%	0.552%
16	19.786	2839	2842	2847	rVB	102296	138821	3.13%	0.470%
17	19.980	2870	2875	2881	rBV	3455497	4440651	100.00%	15.027%
18	21.631	3150	3156	3162	rBV	1497693	2495076	56.19%	8.443%
19	24.816	3689	3698	3709	rVB2	875941	2473181	55.69%	8.369%


Sum of corrected areas: 29550864

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032217\
Data File : BG026374.D
Acq On : 22 Mar 2017 12:40
Operator : SJ/MA
Sample : I2332-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-01-002-B

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

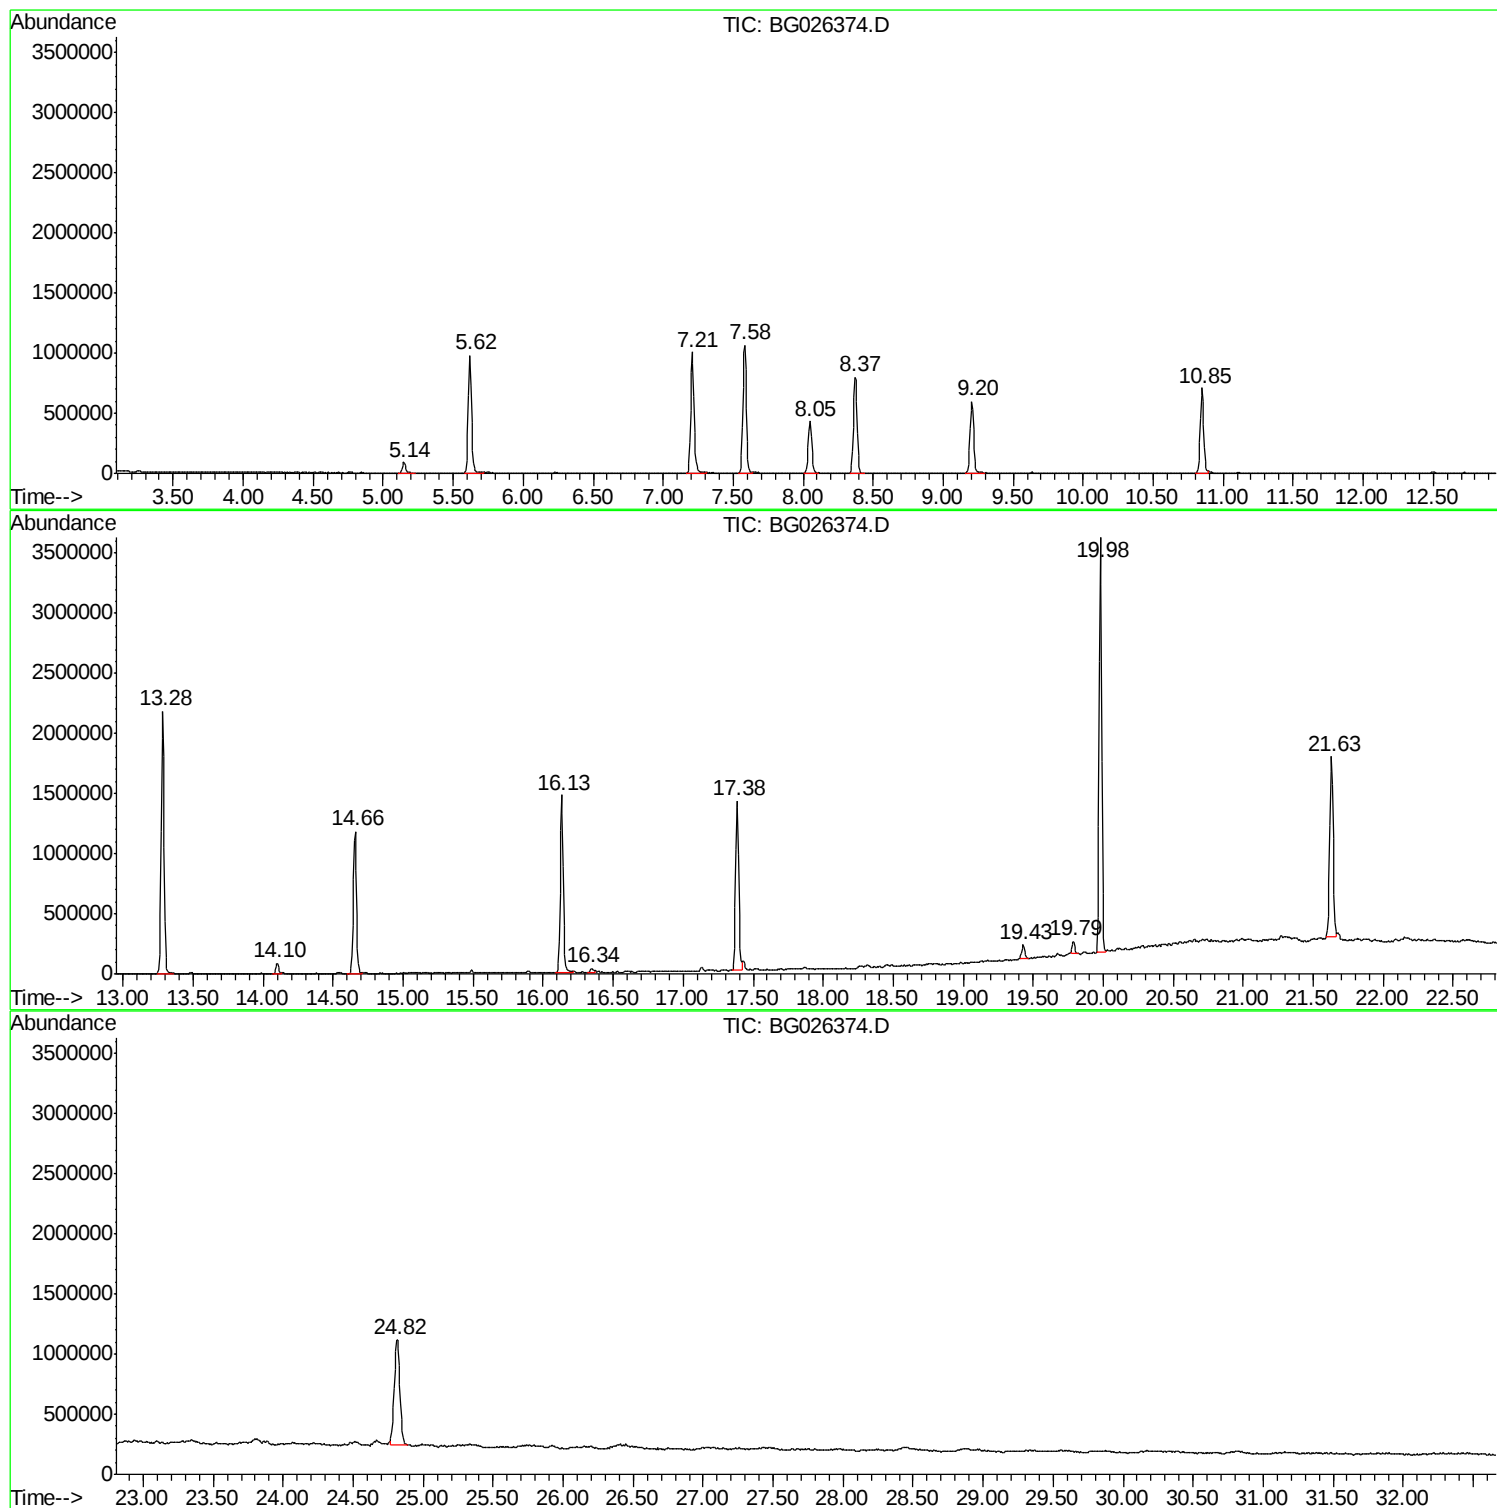

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032217\
Data File : BG026374.D
Acq On : 22 Mar 2017 12:40
Operator : SJ/MA
Sample : I2332-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-01-002-B










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.14	3.74 ng	140439	1,4-Dichlorobenzene-d4	8.05

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Guanidine	59	CH5N3	000113-00-8	50
3			4-Ethyl-3-octanol	158	C10H22O	019781-26-1	42
4			3-Hexanol	102	C6H14O	000623-37-0	36
5			Succinic acid, heptyl 2-methoxye...	274	C14H26O5	1000325-80-7	36

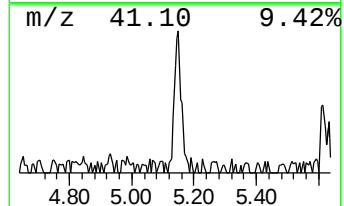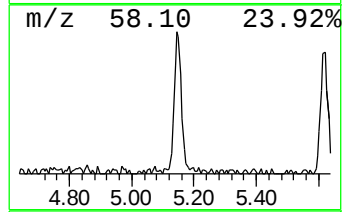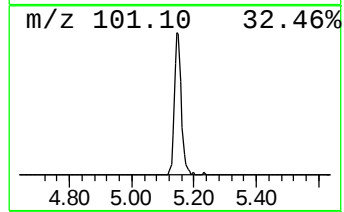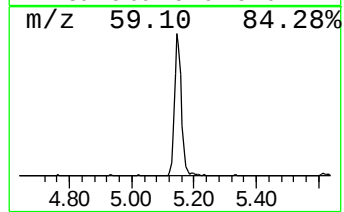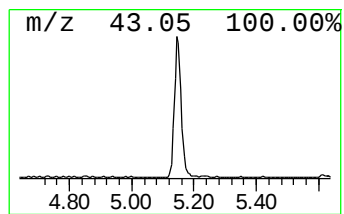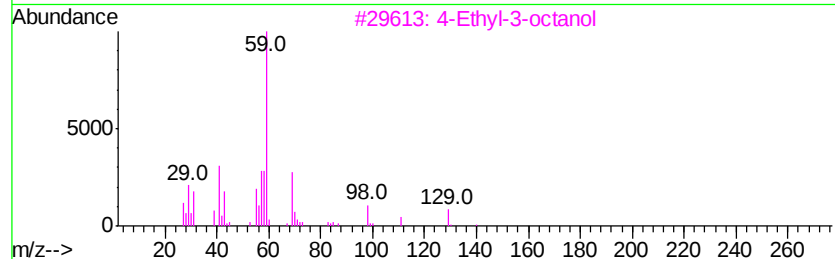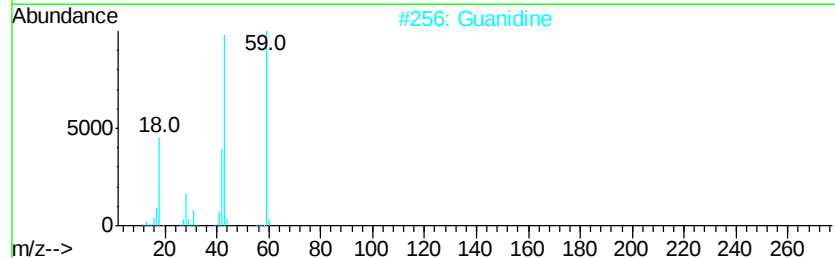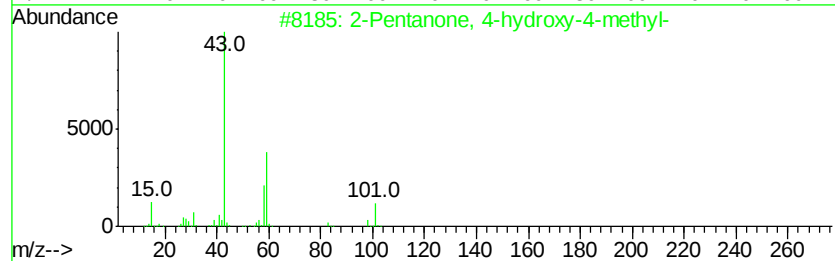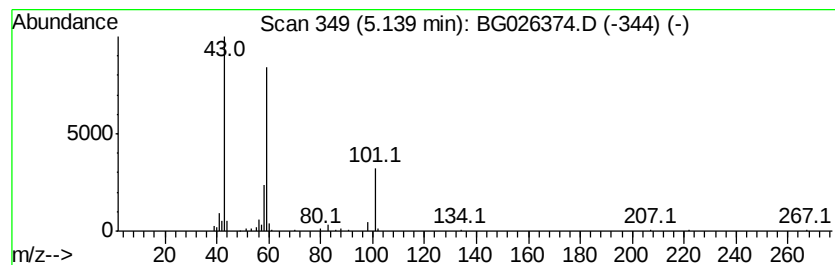

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032217\
Data File : BG026374.D
Acq On : 22 Mar 2017 12:40
Operator : SJ/MA
Sample : I2332-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-01-002-B










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	48.86 ng	1832460	1,4-Dichlorobenzene-d4	8.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

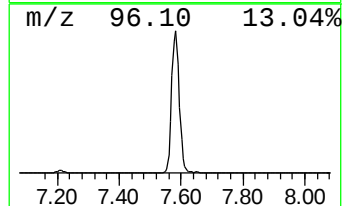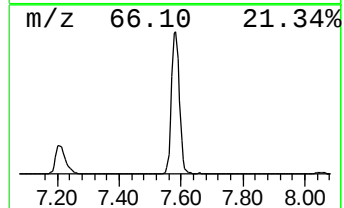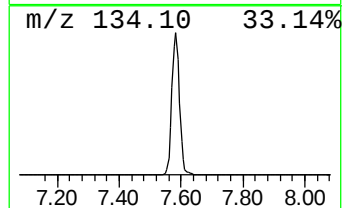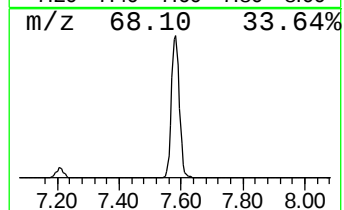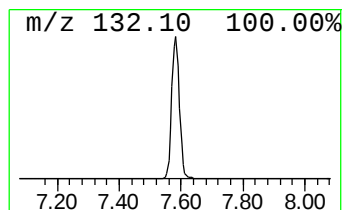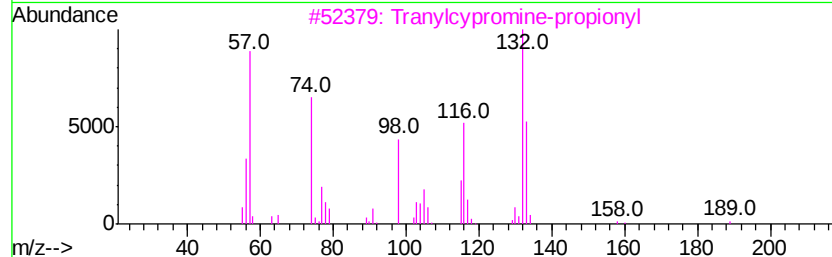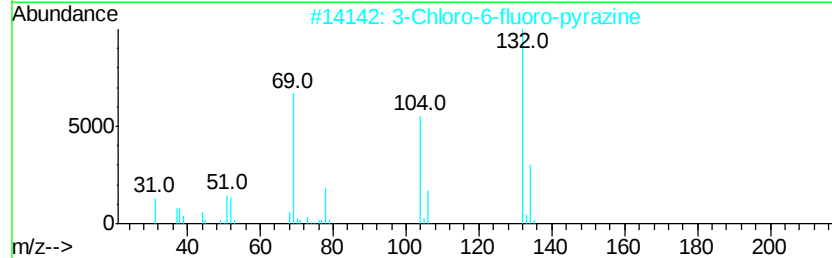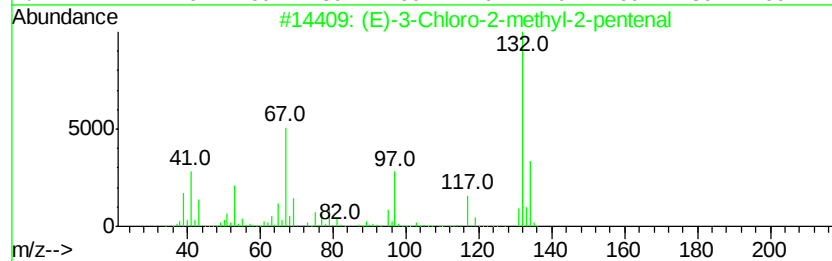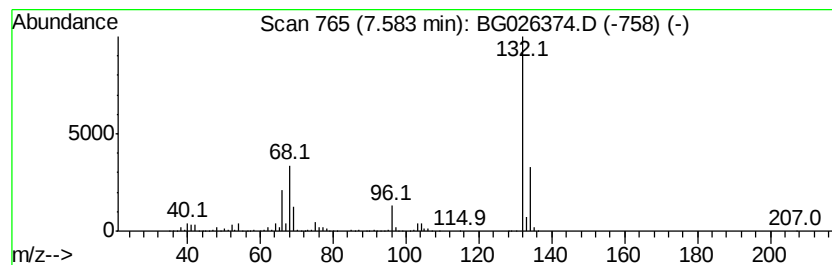

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032217\
Data File : BG026374.D
Acq On : 22 Mar 2017 12:40
Operator : SJ/MA
Sample : I2332-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-SF-01-002-B

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.14	3.7	ng	140439	1	8.05	750115	20.0
unknown7.58	7.58	48.9	ng	1832460	1	8.05	750115	20.0