
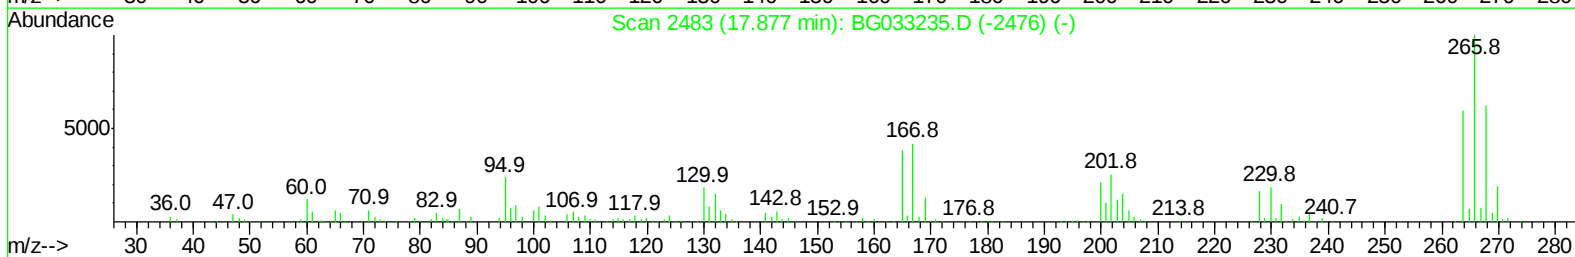
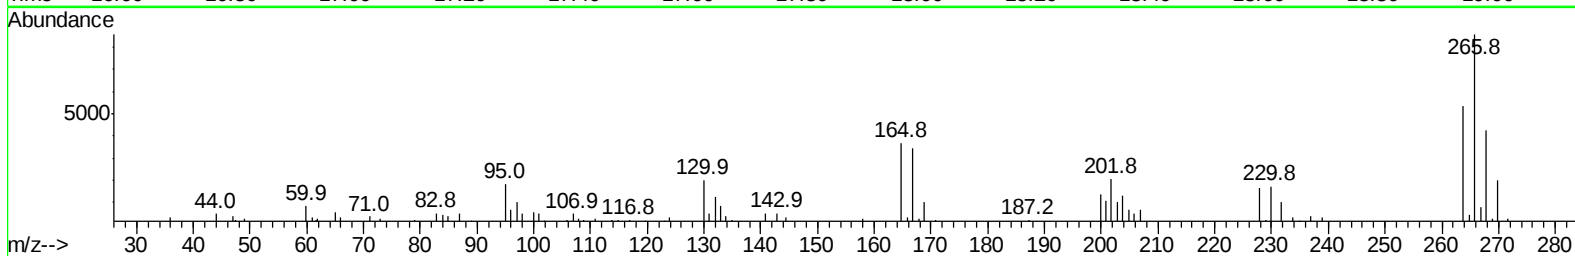


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG032218\
Data File : BG033290.D
Acq On : 22 Mar 2018 12:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 05:51:27 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 22 17:32:09 2018
Response via : Initial Calibration

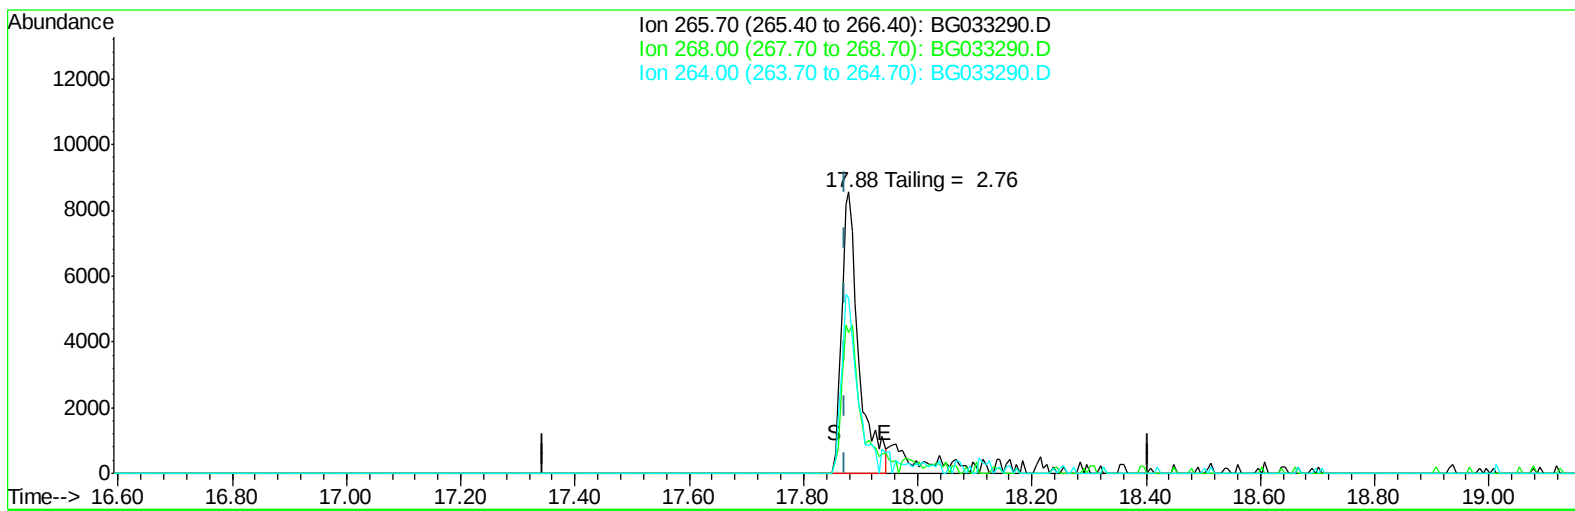

TIC: BG033290.D

(69) Pentachlorophenol (C)




17.879min (+0.005) 40322.61ng

response 18180

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	49.88#
264.00	62.00	62.19
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG032218\
Data File : BG033290.D
Acq On : 22 Mar 2018 12:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 05:51:27 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 22 17:32:09 2018
Response via : Initial Calibration

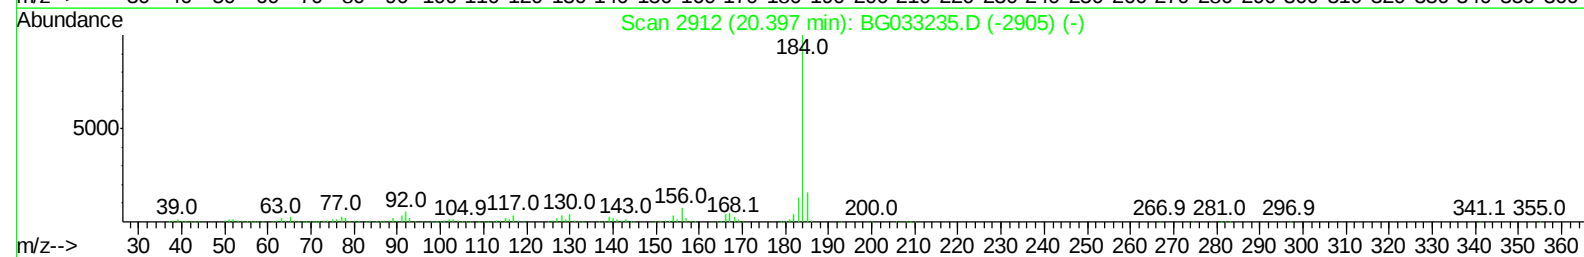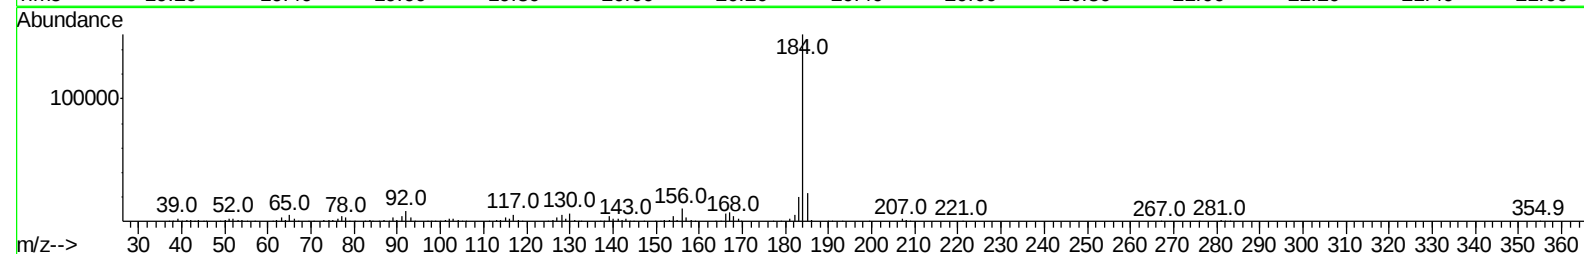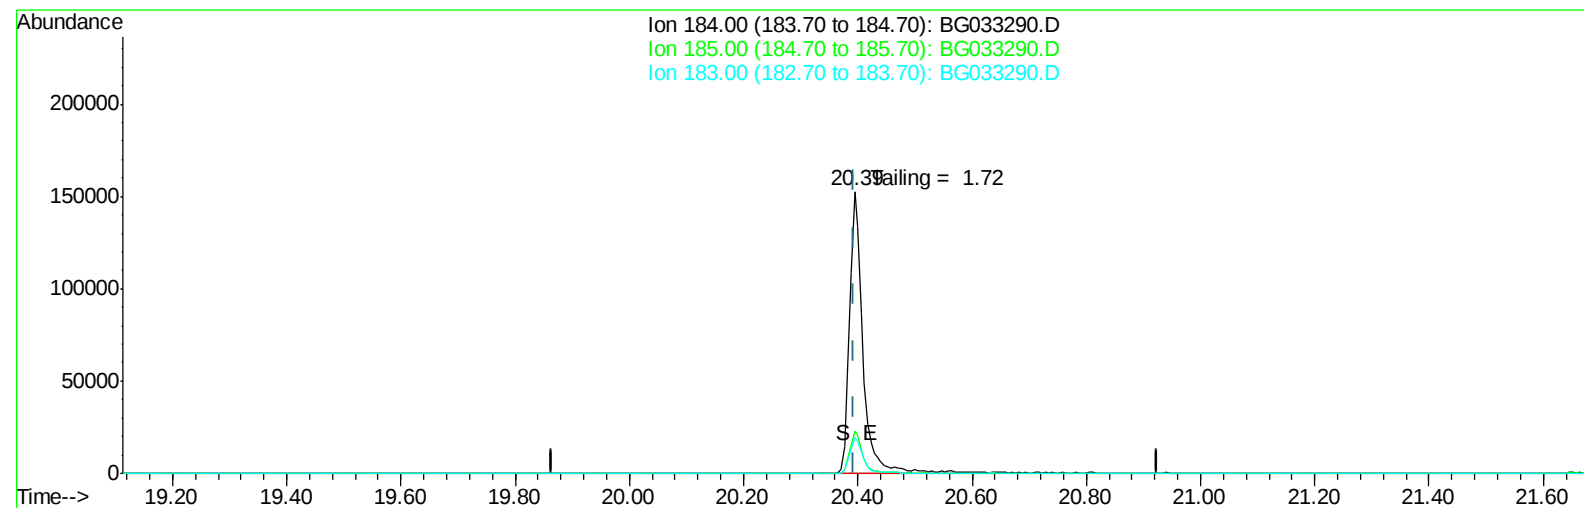

TIC: BG033290.D

(76) Benzidine

20.394min (-0.001) 0.00ng

response 246138

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.14
183.00	13.30	12.84
0.00	0.00	0.00