
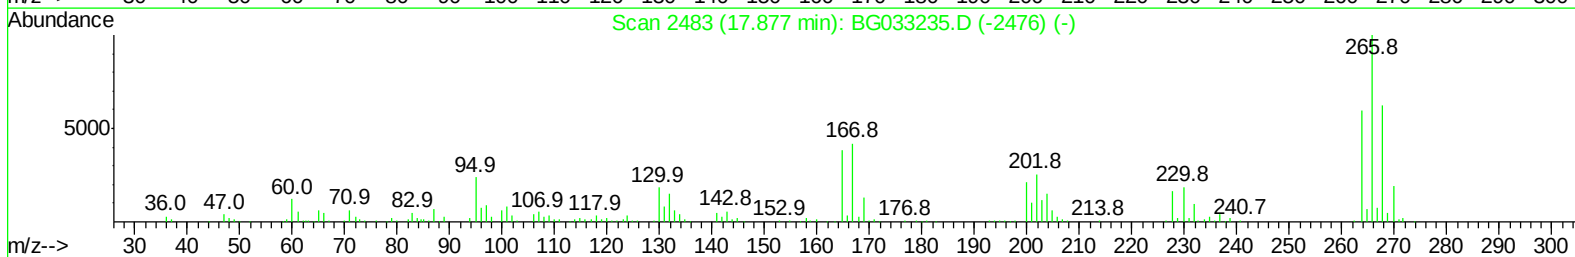
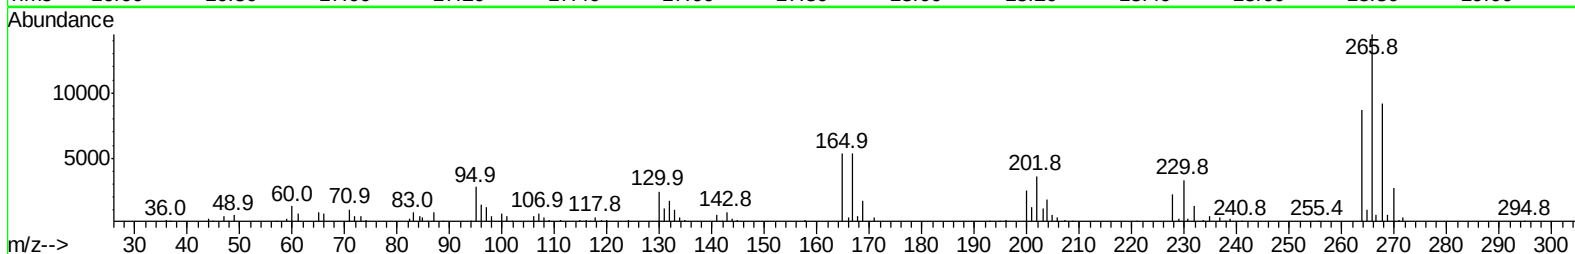


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG032218\
Data File : BG033309.D
Acq On : 23 Mar 2018 00:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 04:19:15 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 22 17:32:09 2018
Response via : Initial Calibration

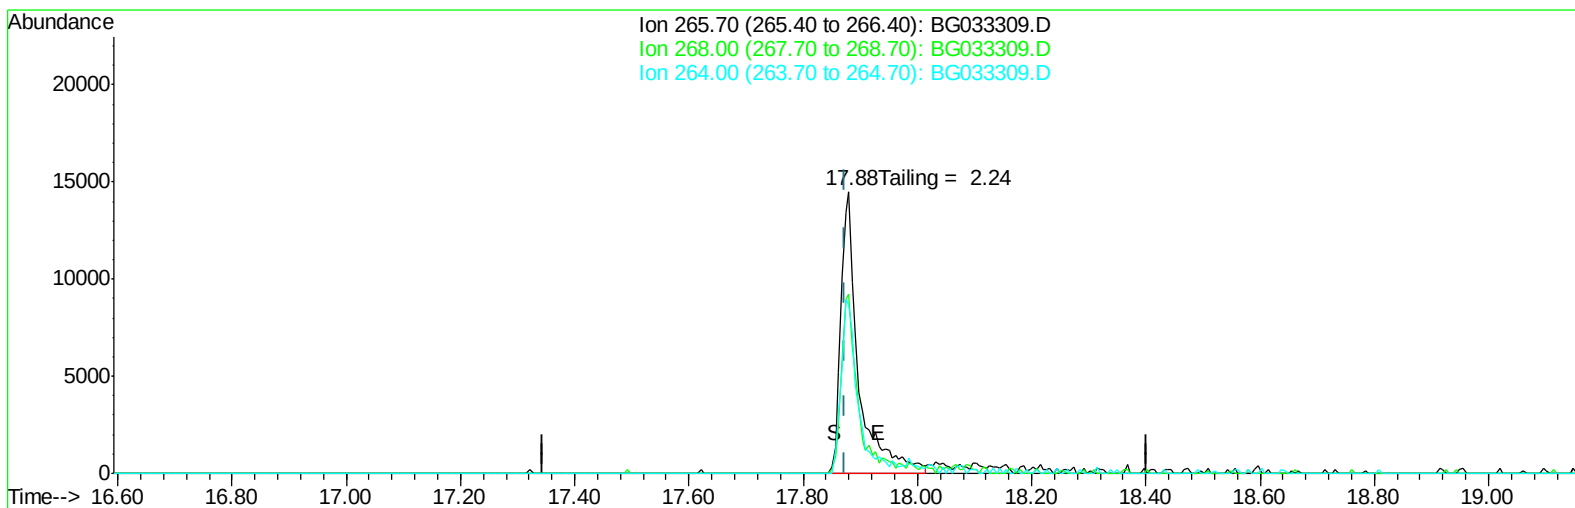

TIC: BG033309.D

(69) Pentachlorophenol (C)




17.880min (+0.006) 67848.96ng

response 31745

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.70
264.00	62.00	60.04
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG032218\
Data File : BG033309.D
Acq On : 23 Mar 2018 00:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 04:19:15 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 22 17:32:09 2018
Response via : Initial Calibration

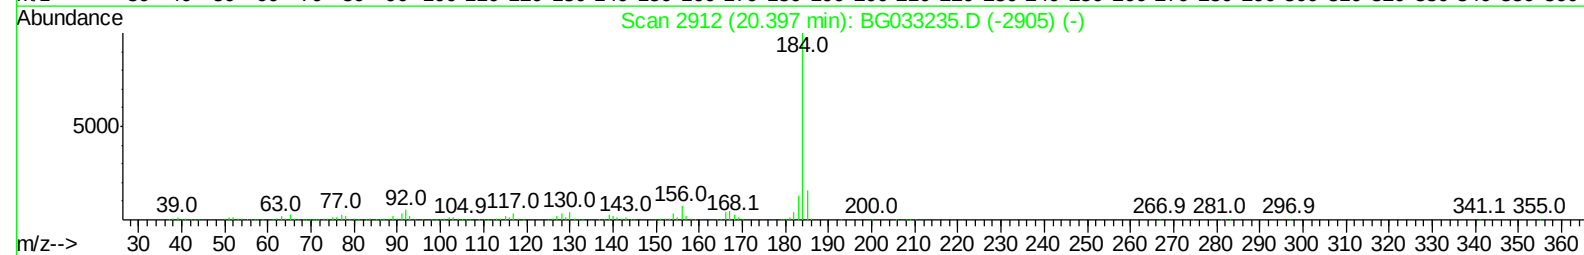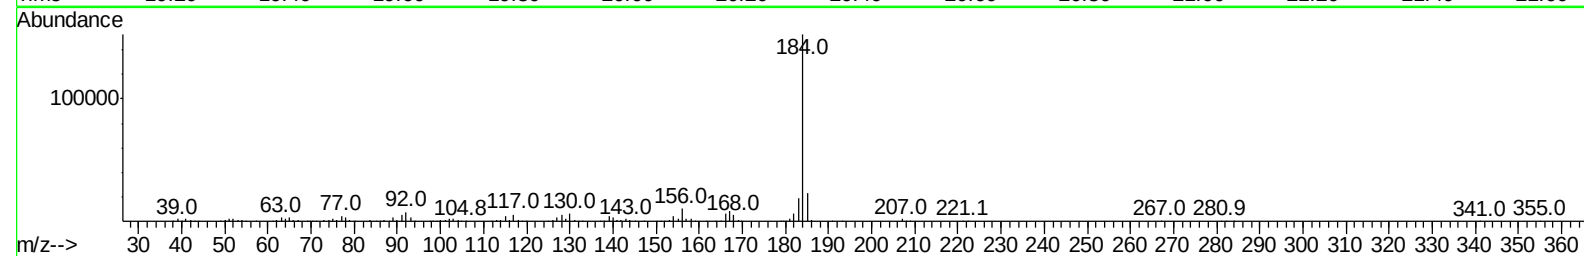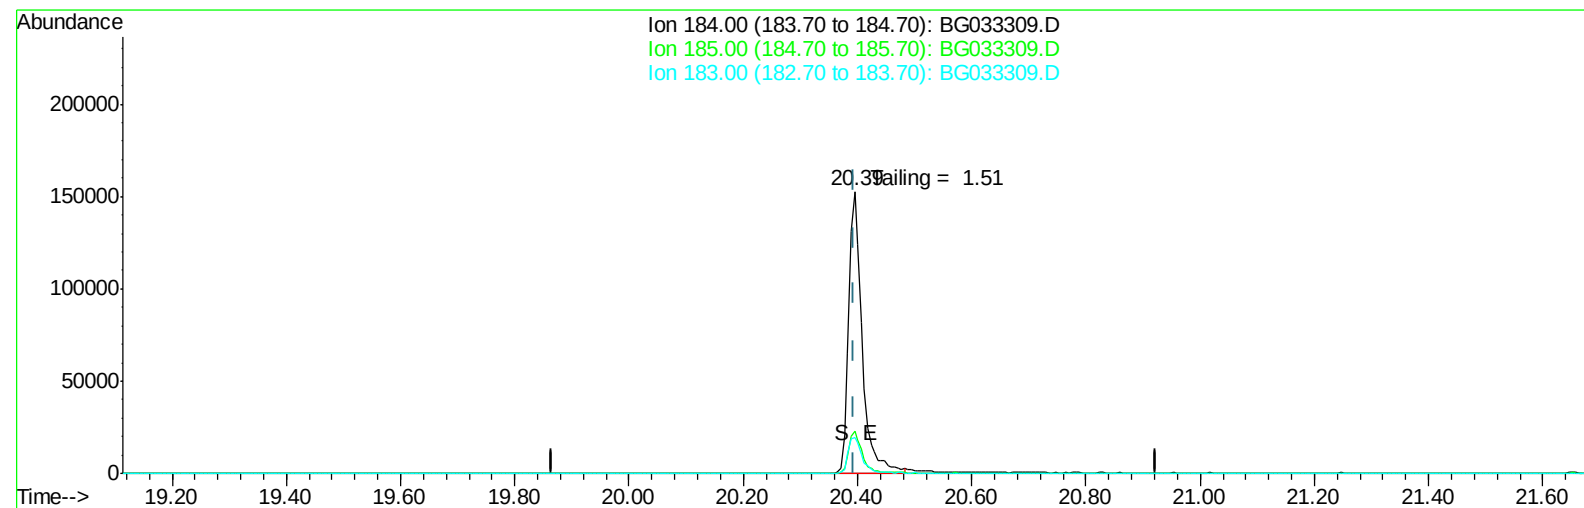

TIC: BG033309.D

(76) Benzidine

20.395min (-0.000) 0.00ng

response 257187

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.16
183.00	13.30	12.55
0.00	0.00	0.00