


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG032218\
 Data File : BG033290.D
 Acq On : 22 Mar 2018 12:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 22 17:32:09 2018

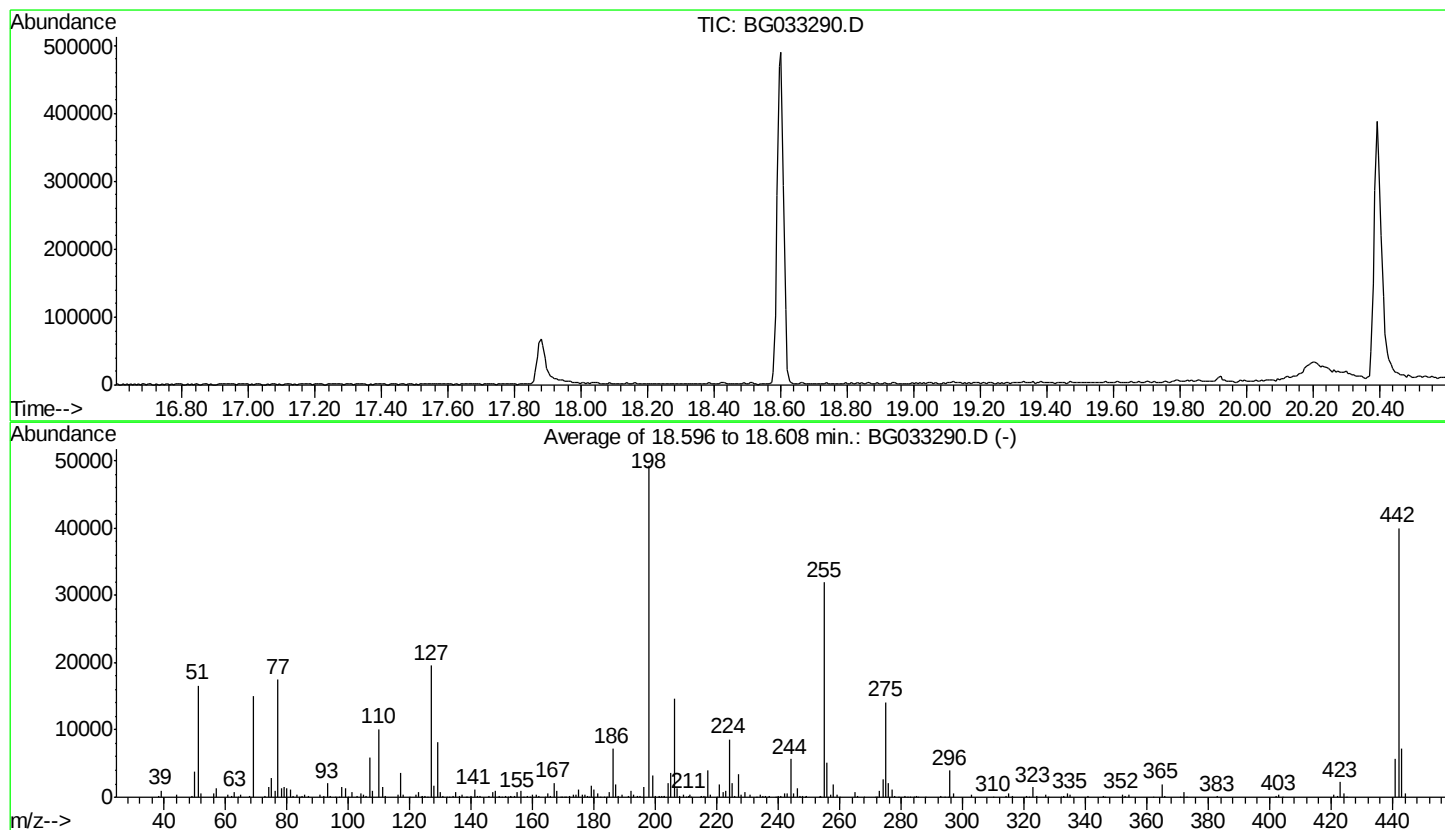

AutoFind: Scans 2605, 2606, 2607; Background Corrected with Scan 2598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	16576	PASS
68	69	0.00	2	1.2	185	PASS
69	198	0.00	100	30.5	15005	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.7	19530	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49250	PASS
199	198	5	9	6.7	3284	PASS
275	198	10	60	28.6	14079	PASS
365	198	1	100	4.0	1964	PASS
441	443	0.01	100	79.7	5739	PASS
442	198	50	100	81.2	39984	PASS
443	442	15	24	18.0	7205	PASS