


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG032218\
 Data File : BG033309.D
 Acq On : 23 Mar 2018 00:51
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 22 17:32:09 2018

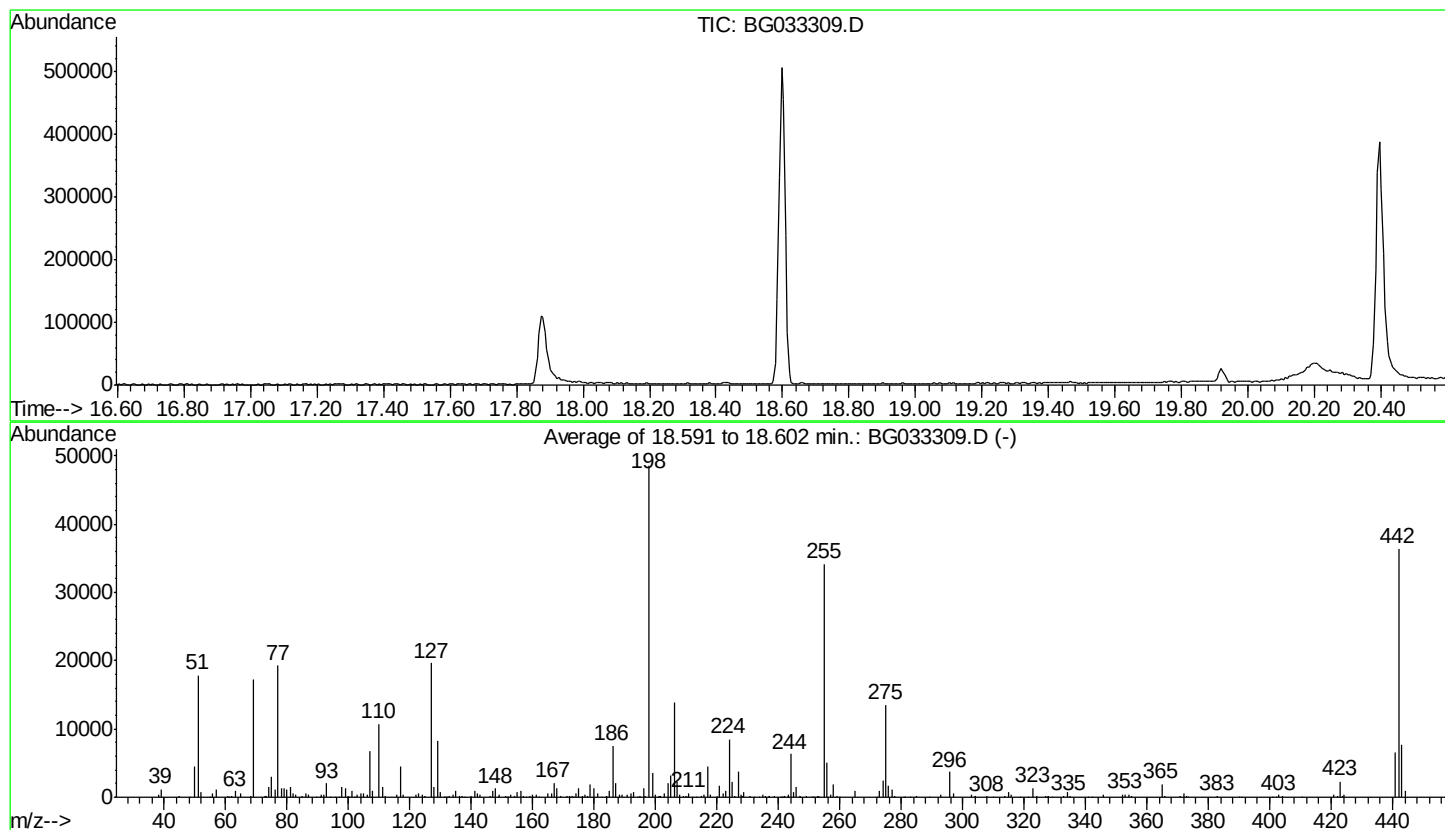

AutoFind: Scans 2604, 2605, 2606; Background Corrected with Scan 2598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	17864	PASS
68	69	0.00	2	1.2	202	PASS
69	198	0.00	100	35.4	17197	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.5	19639	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48544	PASS
199	198	5	9	7.5	3620	PASS
275	198	10	60	27.9	13568	PASS
365	198	1	100	3.9	1896	PASS
441	443	0.01	100	84.6	6480	PASS
442	198	50	100	75.0	36405	PASS
443	442	15	24	21.0	7659	PASS