
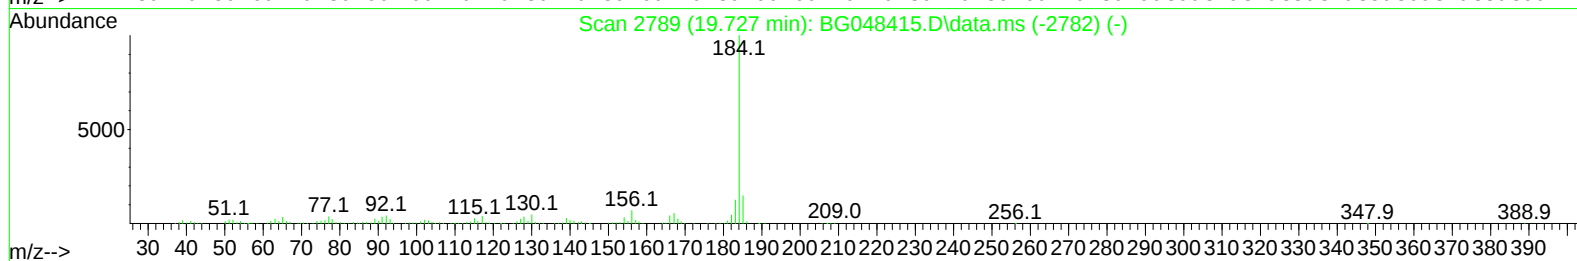
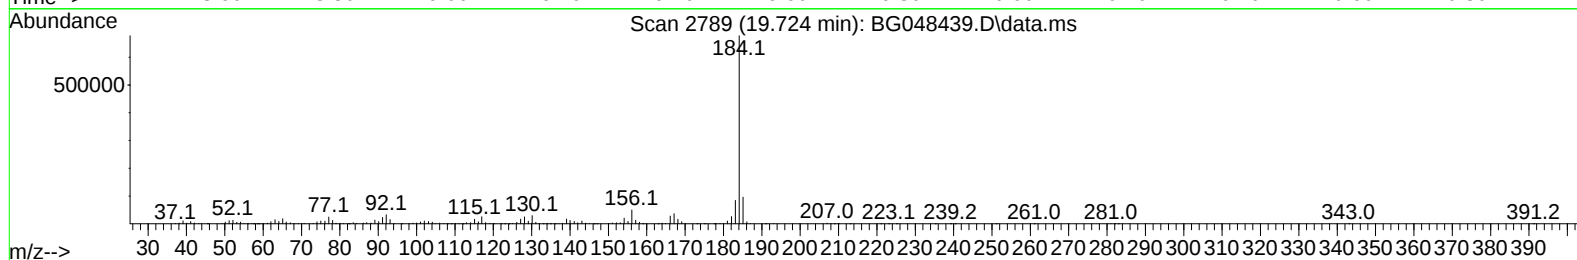


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
 Data File : BG048439.D
 Acq On : 22 Mar 2021 9:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 10:58:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 18 16:38:55 2021
 Response via : Initial Calibration

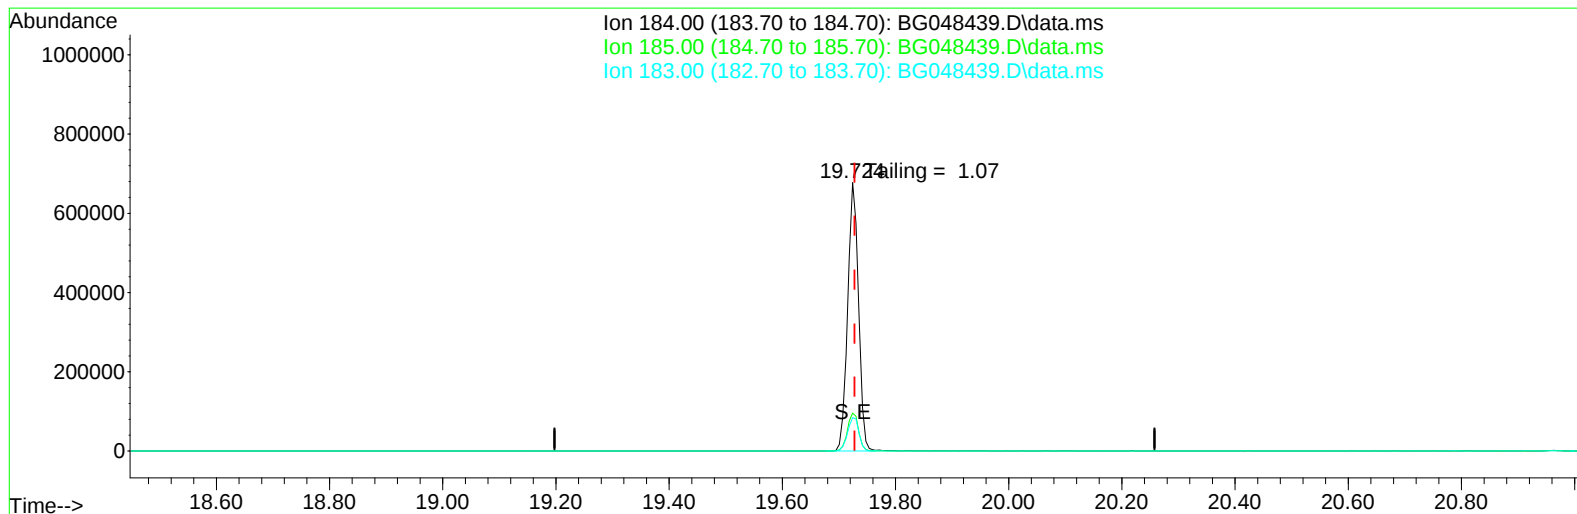




TIC: BG048439.D\data.ms

(77) Benzidine**19.724min (-0.003) 449969.80 ng****response 903077**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.16
183.00	13.20	12.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048439.D
Acq On : 22 Mar 2021 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 10:58:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration

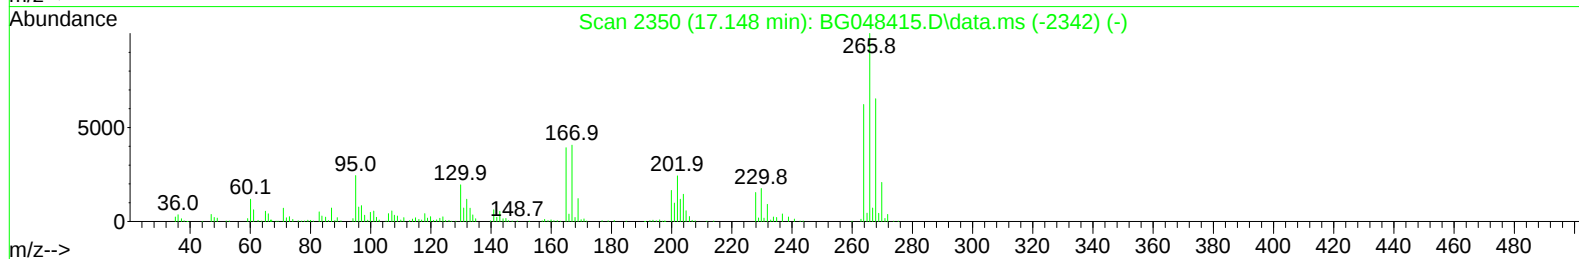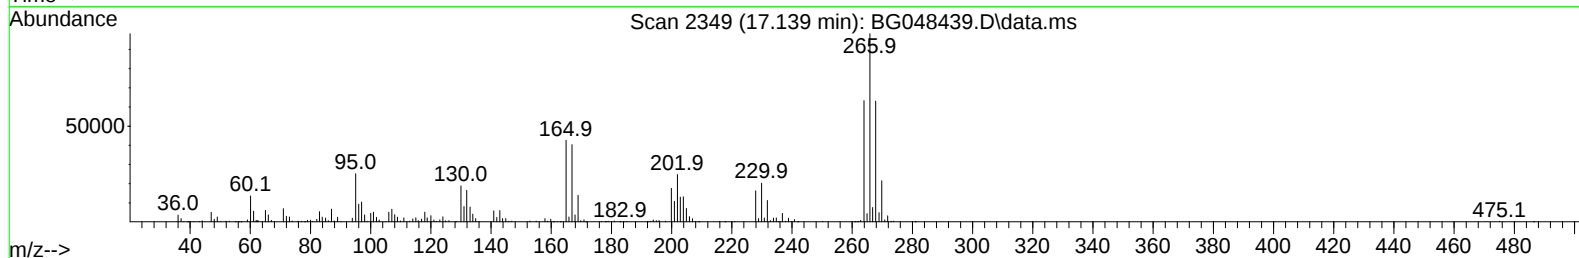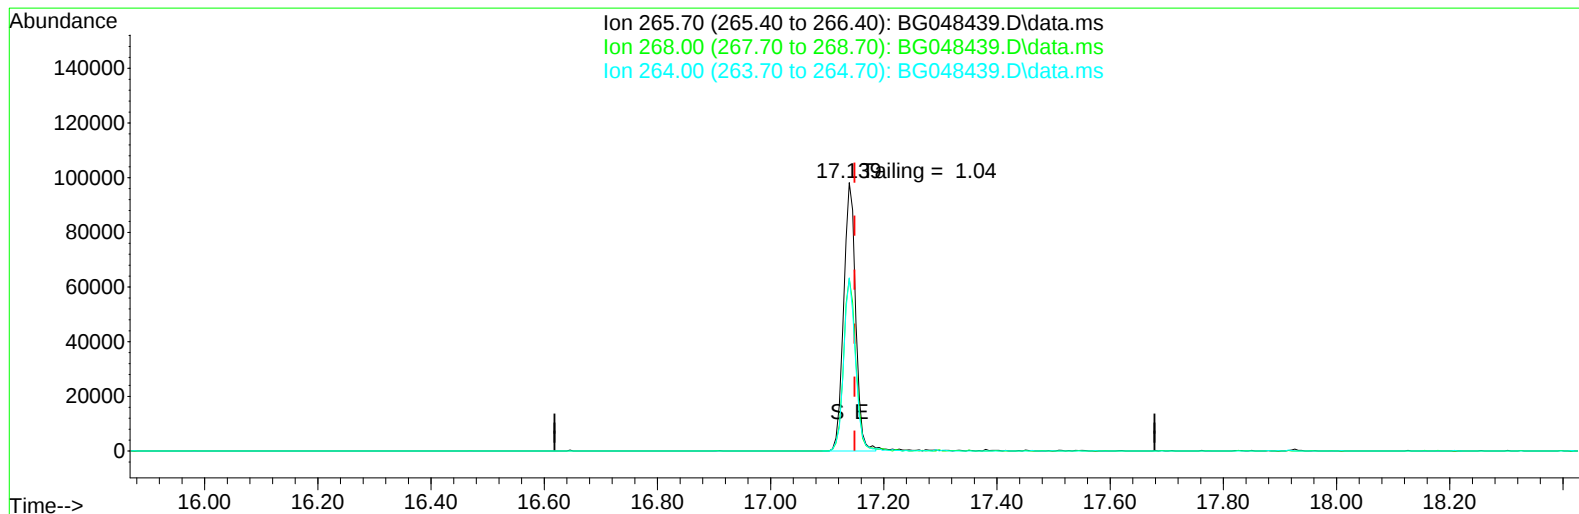

TIC: BG048439.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.009) 210849.83 ng

response 145653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.25
264.00	61.60	64.52
0.00	0.00	0.00