
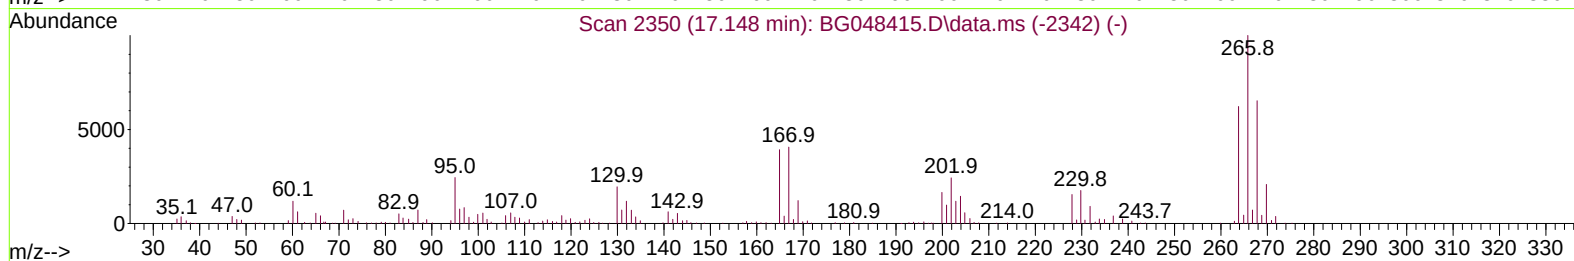
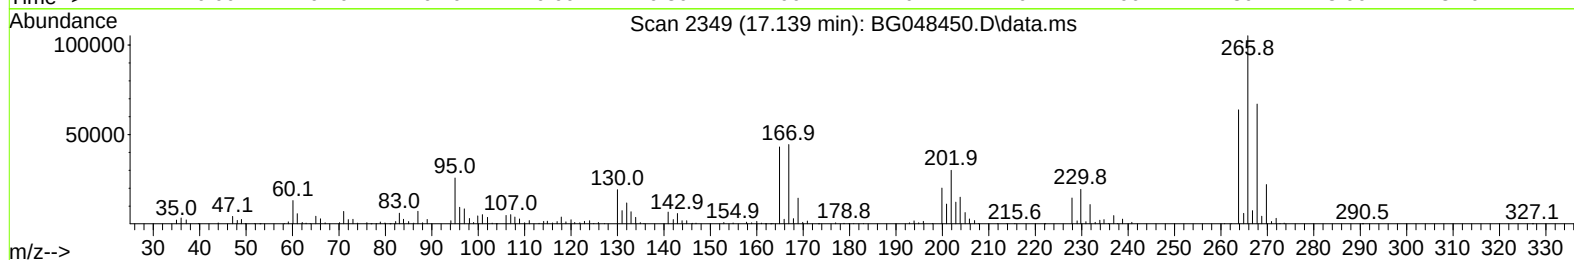


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032221\  
Data File : BG048450.D  
Acq On : 22 Mar 2021 19:13  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 09:03:34 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 22 11:22:24 2021  
Response via : Initial Calibration

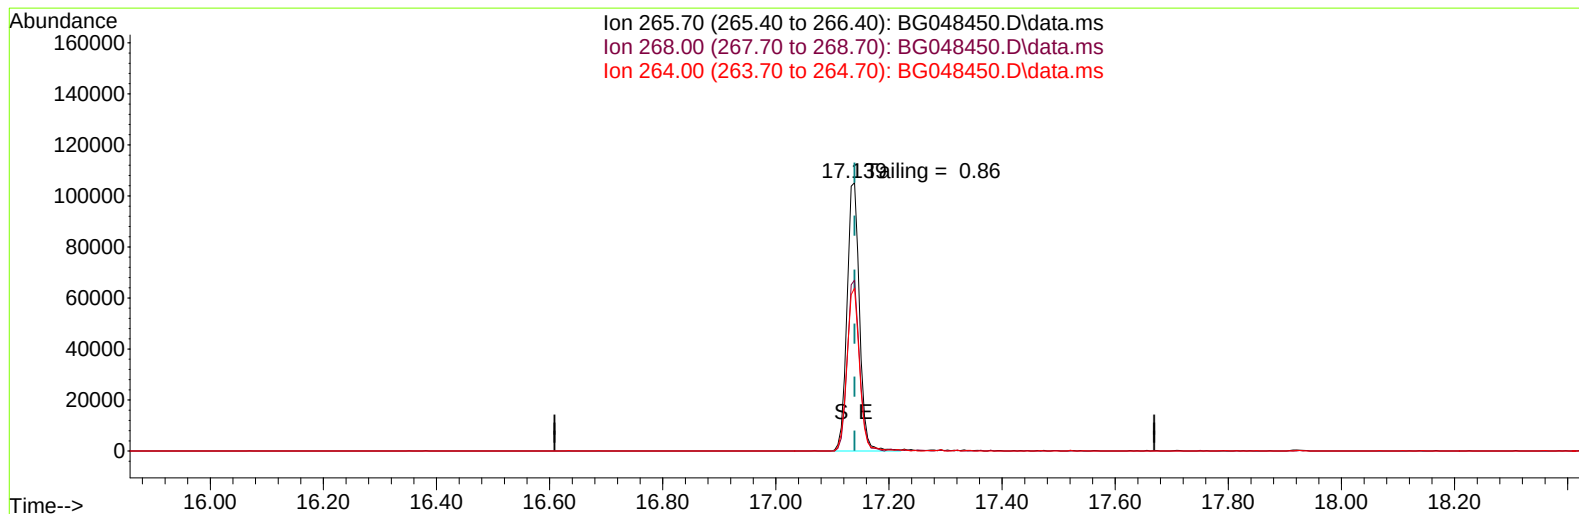

TIC: BG048450.D\data.ms

**(70) Pentachlorophenol (C)**




17.139min (-0.000) 260802.64 ng

response 161442

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.68  |
| 264.00 | 61.60  | 60.68  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032221\  
 Data File : BG048450.D  
 Acq On : 22 Mar 2021 19:13  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 09:03:34 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031821.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Mar 22 11:22:24 2021  
 Response via : Initial Calibration

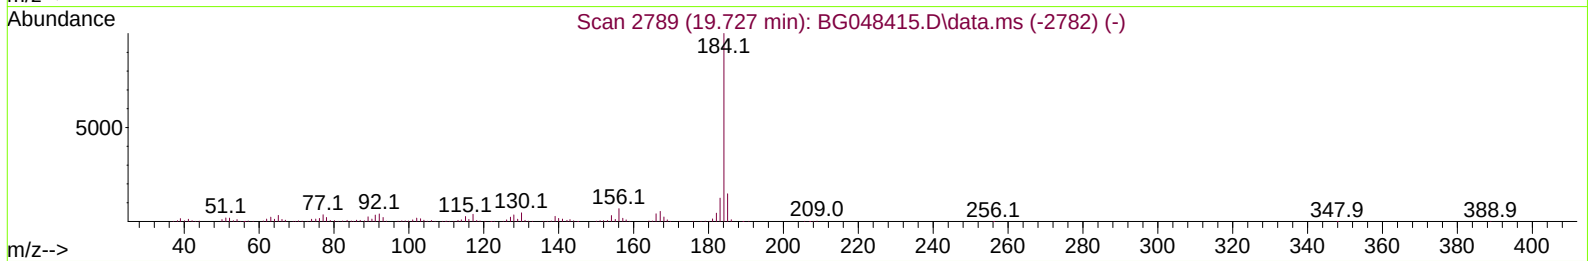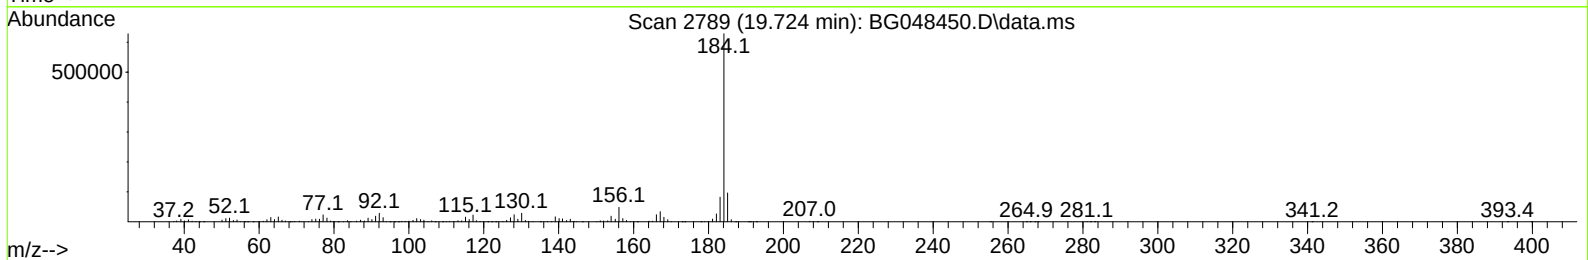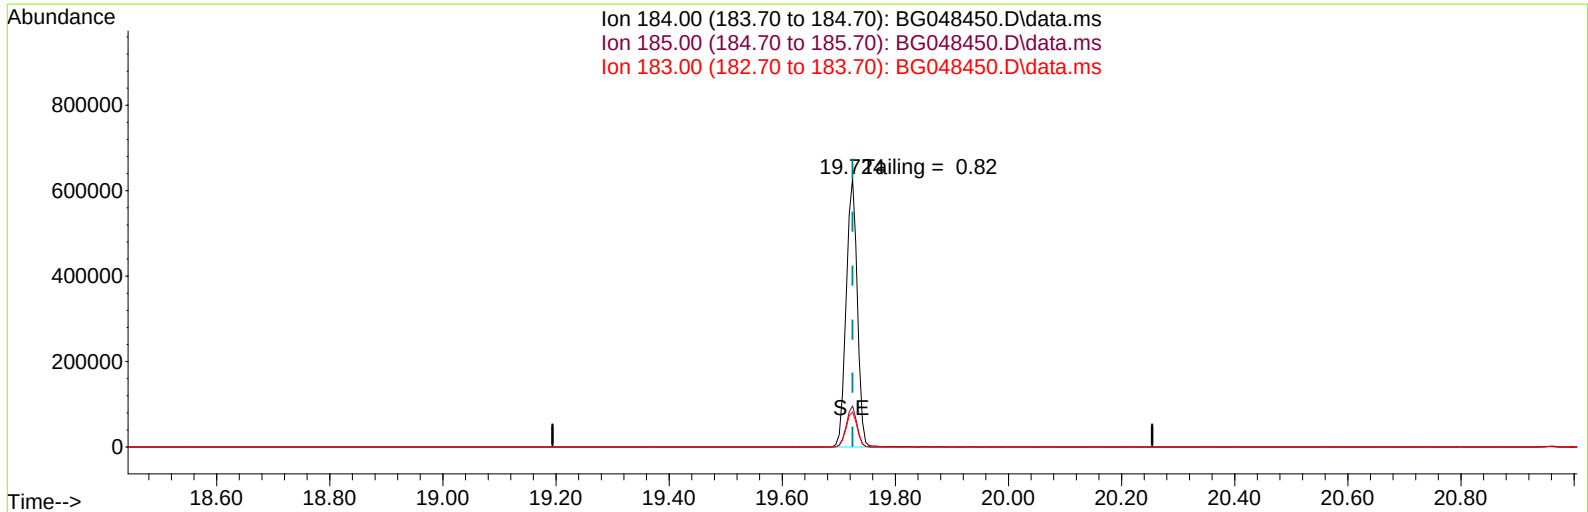

TIC: BG048450.D\data.ms

**(77) Benzidine****19.724min (-0.000) 55160.16 ng****response 857550**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 15.32  |
| 183.00 | 13.20  | 13.10  |
| 0.00   | 0.00   | 0.00   |