

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
 Data File : BG048446.D
 Acq On : 22 Mar 2021 15:47
 Operator : CG/JU
 Sample : M1718-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.648	386	393	401	rBV	653721	1016354	29.31%	6.791%
2	7.246	656	665	675	rBV	682542	1164764	33.59%	7.783%
3	8.104	803	811	817	rBV	178376	295091	8.51%	1.972%
4	9.267	1001	1009	1019	rBV	424631	741465	21.39%	4.954%
5	10.924	1282	1291	1298	rBV	221017	397754	11.47%	2.658%
6	13.368	1699	1707	1714	rVB	1134189	1723435	49.71%	11.516%
7	14.185	1842	1846	1853	rBV2	26923	37668	1.09%	0.252%
8	14.743	1934	1941	1948	rBV	401627	630334	18.18%	4.212%
9	16.229	2187	2194	2201	rBV	1161032	1751843	50.53%	11.706%
10	17.493	2403	2409	2415	rBV	584170	896707	25.86%	5.992%
11	18.374	2554	2559	2567	rBV2	151874	216038	6.23%	1.444%
12	18.891	2641	2647	2651	rBV2	19823	34693	1.00%	0.232%
13	19.144	2686	2690	2695	rVB	87185	105774	3.05%	0.707%
14	19.643	2771	2775	2779	rBV6	26712	37228	1.07%	0.249%
15	20.101	2847	2853	2859	rBV	2659814	3467173	100.00%	23.168%
16	21.411	3072	3076	3088	rBV	196125	374000	10.79%	2.499%
17	21.788	3133	3140	3146	rVB	594957	1007015	29.04%	6.729%
18	23.538	3433	3438	3444	rVB5	27157	52874	1.52%	0.353%
19	25.119	3697	3707	3718	rVB	358087	1015281	29.28%	6.784%




Sum of corrected areas: 14965491

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048446.D
Acq On : 22 Mar 2021 15:47
Operator : CG/JU
Sample : M1718-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

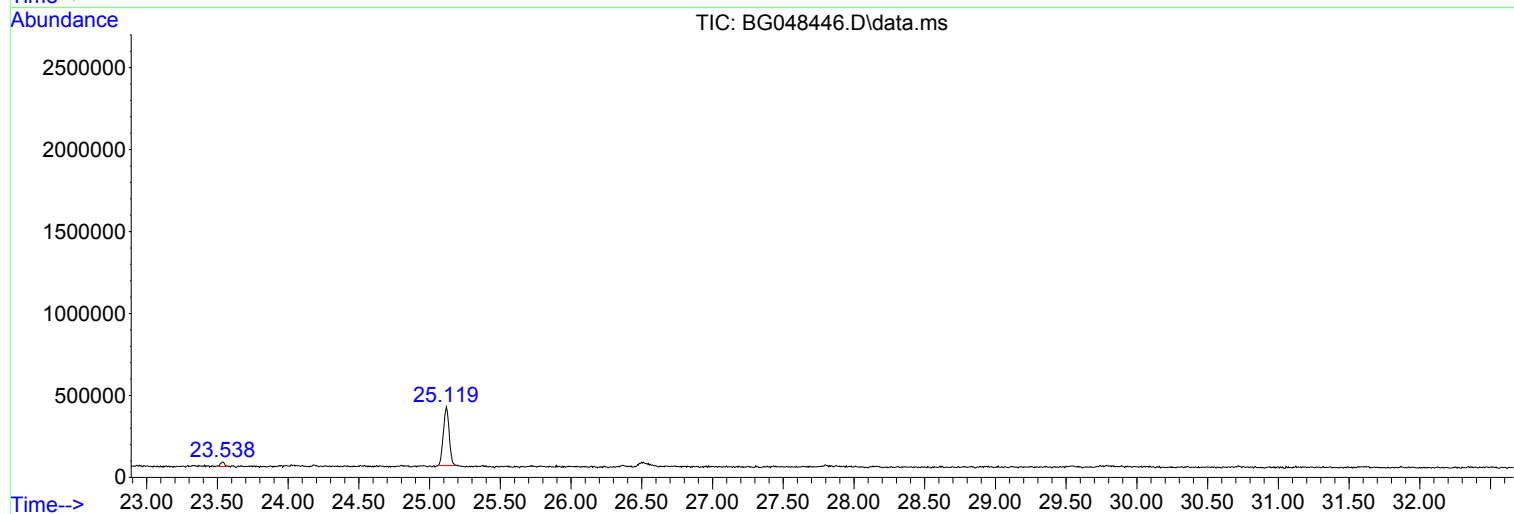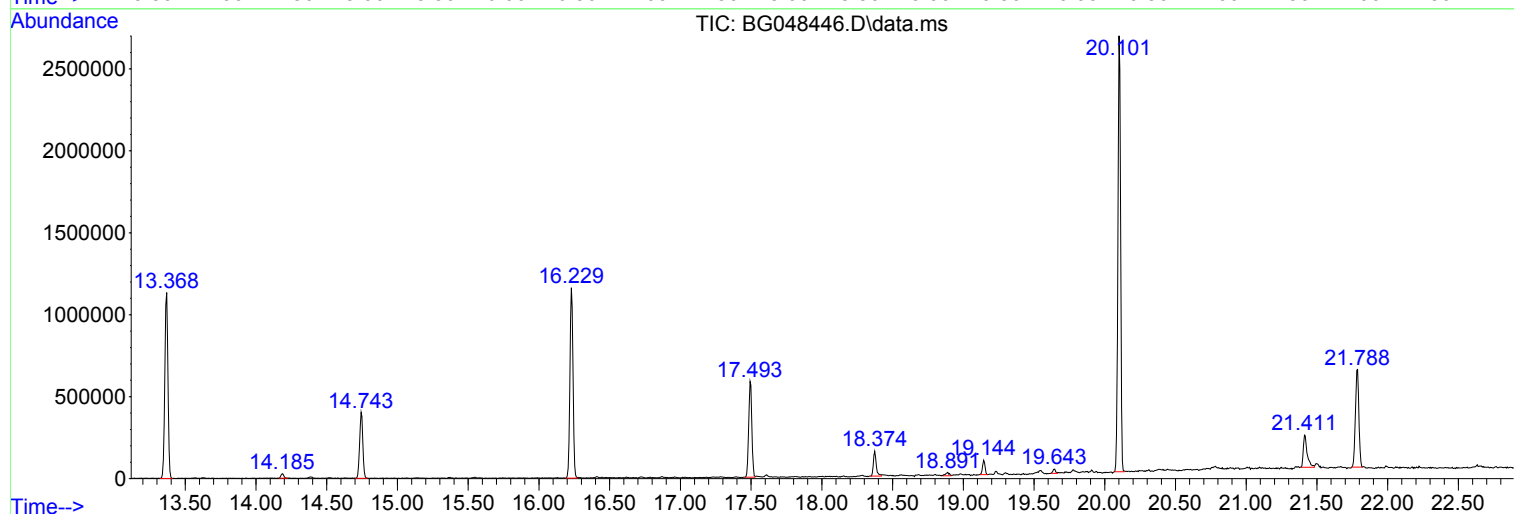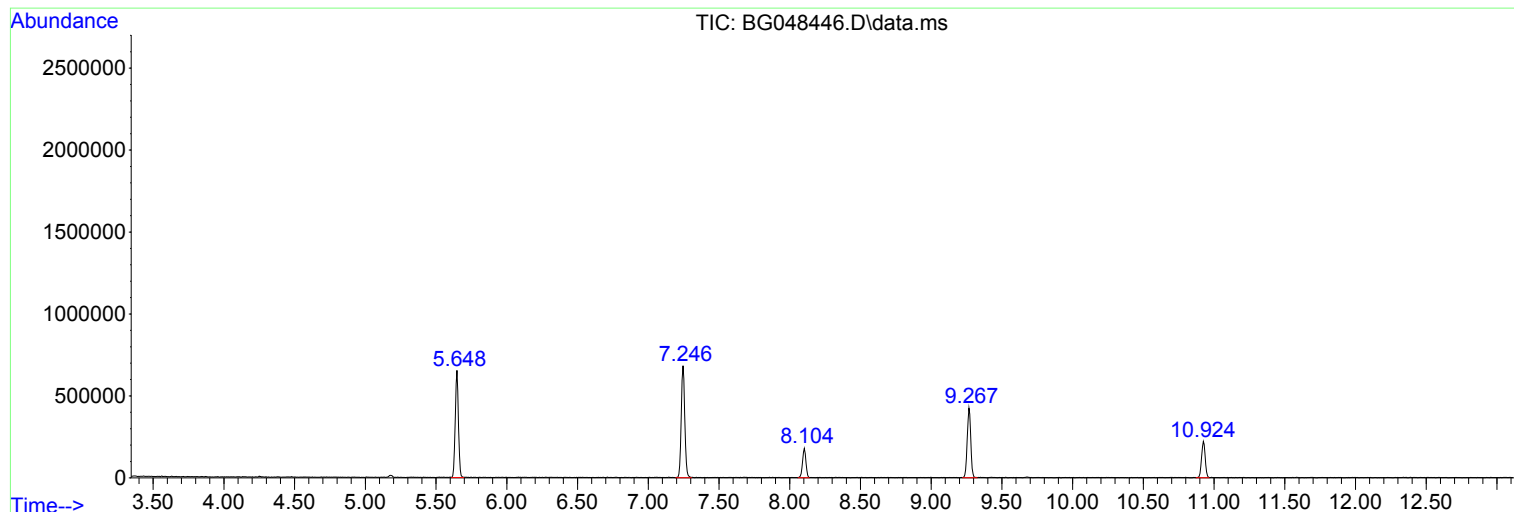

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048446.D
Acq On : 22 Mar 2021 15:47
Operator : CG/JU
Sample : M1718-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048446.D
Acq On : 22 Mar 2021 15:47
Operator : CG/JU
Sample : M1718-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------