

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
 Data File : BG048448.D
 Acq On : 22 Mar 2021 17:07
 Operator : CG/JU
 Sample : M1718-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.646	386	393	402	rVB	705479	1121861	33.20%	7.192%
2	7.250	658	666	676	rVB	740904	1303064	38.56%	8.354%
3	8.102	803	811	818	rBV2	192959	325322	9.63%	2.086%
4	9.266	1002	1009	1018	rVB	457320	827689	24.50%	5.306%
5	10.922	1283	1291	1298	rBV	251252	448968	13.29%	2.878%
6	13.367	1700	1707	1714	rBV	1244059	1905037	56.38%	12.213%
7	14.189	1843	1847	1852	rVB	36891	50690	1.50%	0.325%
8	14.741	1934	1941	1950	rVB	447840	706688	20.91%	4.531%
9	16.228	2187	2194	2210	rBV	1272570	1932825	57.20%	12.392%
10	17.497	2403	2410	2415	rBV	643789	965758	28.58%	6.192%
11	18.373	2555	2559	2565	rBV2	107083	145952	4.32%	0.936%
12	19.148	2684	2691	2696	rBV	115898	173251	5.13%	1.111%
13	19.236	2702	2706	2709	rBV3	28106	42205	1.25%	0.271%
14	19.777	2795	2798	2805	rVB6	24244	36978	1.09%	0.237%
15	20.106	2846	2854	2860	rBV	2542193	3378918	100.00%	21.663%
16	21.416	3072	3077	3086	rBV4	133110	254924	7.54%	1.634%
17	21.786	3134	3140	3147	rBV2	604946	1007350	29.81%	6.458%
18	25.118	3698	3707	3716	rVB2	355927	970362	28.72%	6.221%




Sum of corrected areas: 15597842

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048448.D
Acq On : 22 Mar 2021 17:07
Operator : CG/JU
Sample : M1718-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

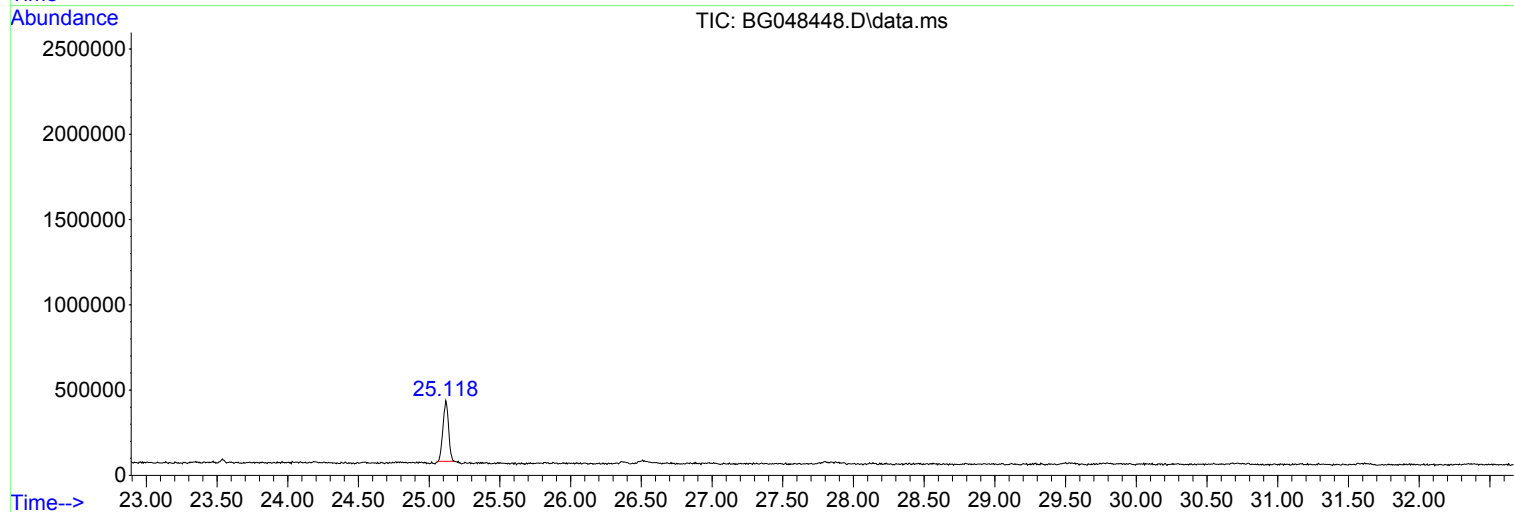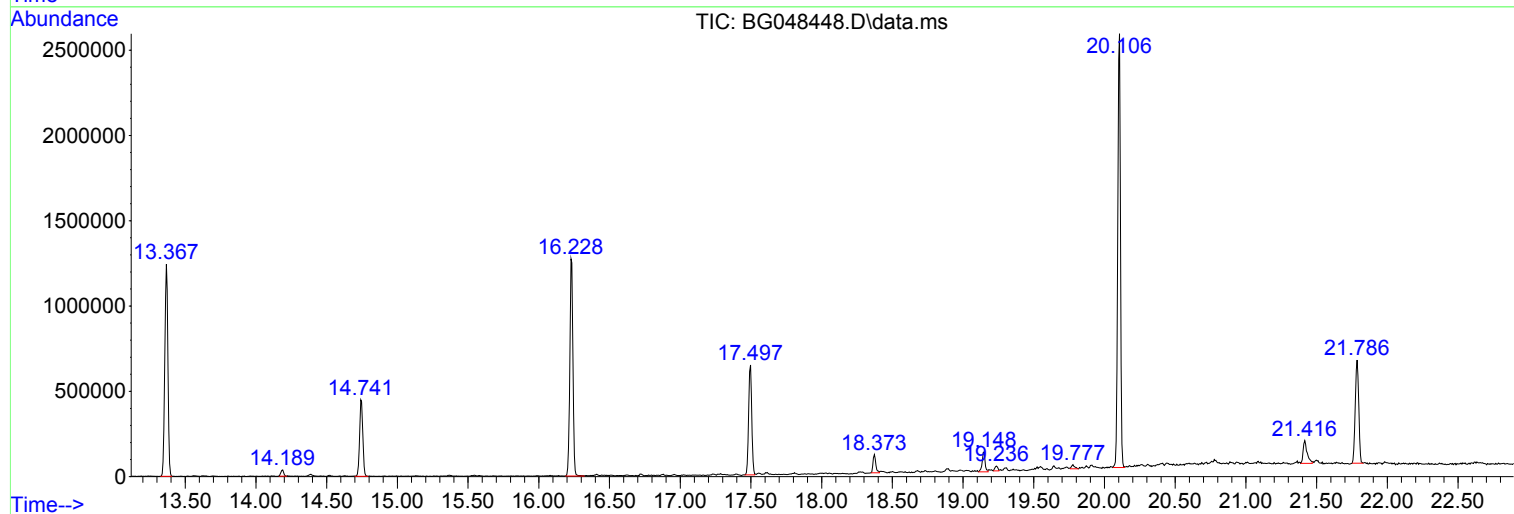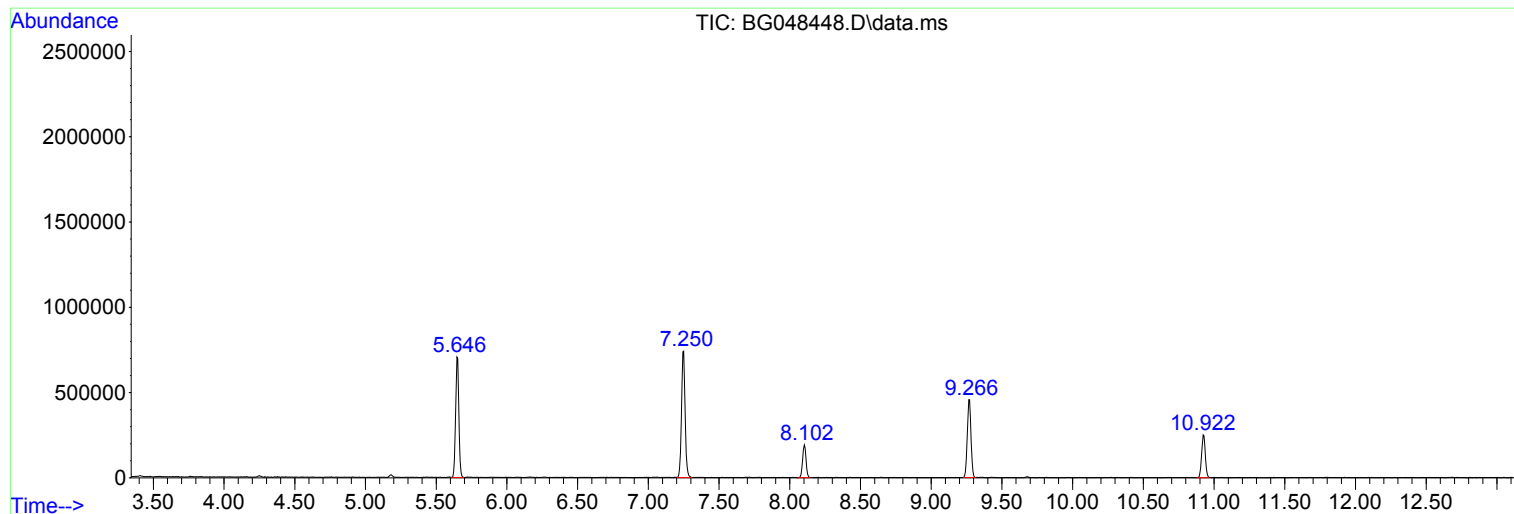

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048448.D
Acq On : 22 Mar 2021 17:07
Operator : CG/JU
Sample : M1718-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048448.D
Acq On : 22 Mar 2021 17:07
Operator : CG/JU
Sample : M1718-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BACKFILL-ASHCROFT-REAR-05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------