

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032221\  
 Data File : BG048452.D  
 Acq On : 22 Mar 2021 21:15  
 Operator : CG/JU  
 Sample : PB135234BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB135234BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048452.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.652       | 386           | 394         | 405          | rBV      | 1124202        | 1823830       | 32.41%          | 8.917%        |
| 2         | 7.250       | 657           | 666         | 676          | rBV      | 1152352        | 1937062       | 34.42%          | 9.470%        |
| 3         | 8.102       | 804           | 811         | 819          | rVB      | 192979         | 327971        | 5.83%           | 1.603%        |
| 4         | 9.271       | 1001          | 1010        | 1020         | rBV      | 714617         | 1275205       | 22.66%          | 6.234%        |
| 5         | 10.922      | 1283          | 1291        | 1299         | rBV      | 245178         | 431459        | 7.67%           | 2.109%        |
| 6         | 13.367      | 1700          | 1707        | 1714         | rBV      | 1847295        | 2832875       | 50.34%          | 13.850%       |
| 7         | 14.741      | 1934          | 1941        | 1949         | rBV      | 402865         | 637035        | 11.32%          | 3.114%        |
| 8         | 16.234      | 2186          | 2195        | 2202         | rBV      | 1660320        | 2599078       | 46.18%          | 12.707%       |
| 9         | 17.491      | 2402          | 2409        | 2419         | rVB      | 571933         | 876498        | 15.57%          | 4.285%        |
| 10        | 20.106      | 2847          | 2854        | 2861         | rBV      | 4337417        | 5627735       | 100.00%         | 27.514%       |
| 11        | 21.780      | 3133          | 3139        | 3147         | rVB      | 629632         | 1060143       | 18.84%          | 5.183%        |
| 12        | 25.112      | 3697          | 3706        | 3719         | rVB2     | 372951         | 1025362       | 18.22%          | 5.013%        |




Sum of corrected areas: 20454253

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032221\  
Data File : BG048452.D  
Acq On : 22 Mar 2021 21:15  
Operator : CG/JU  
Sample : PB135234BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135234BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

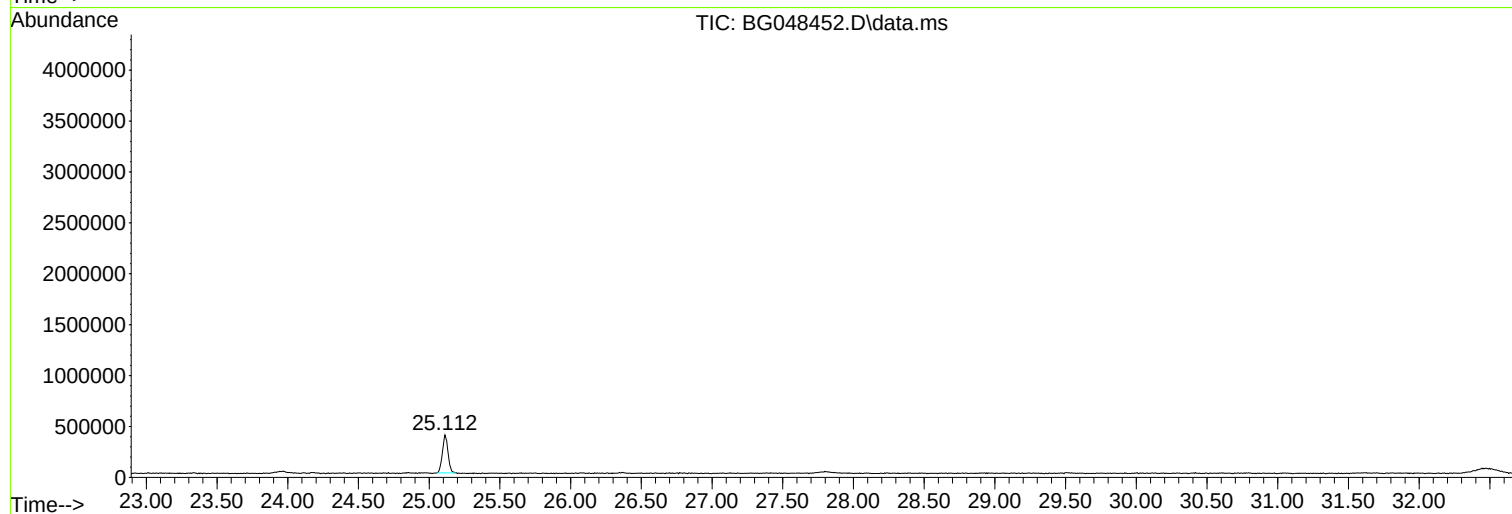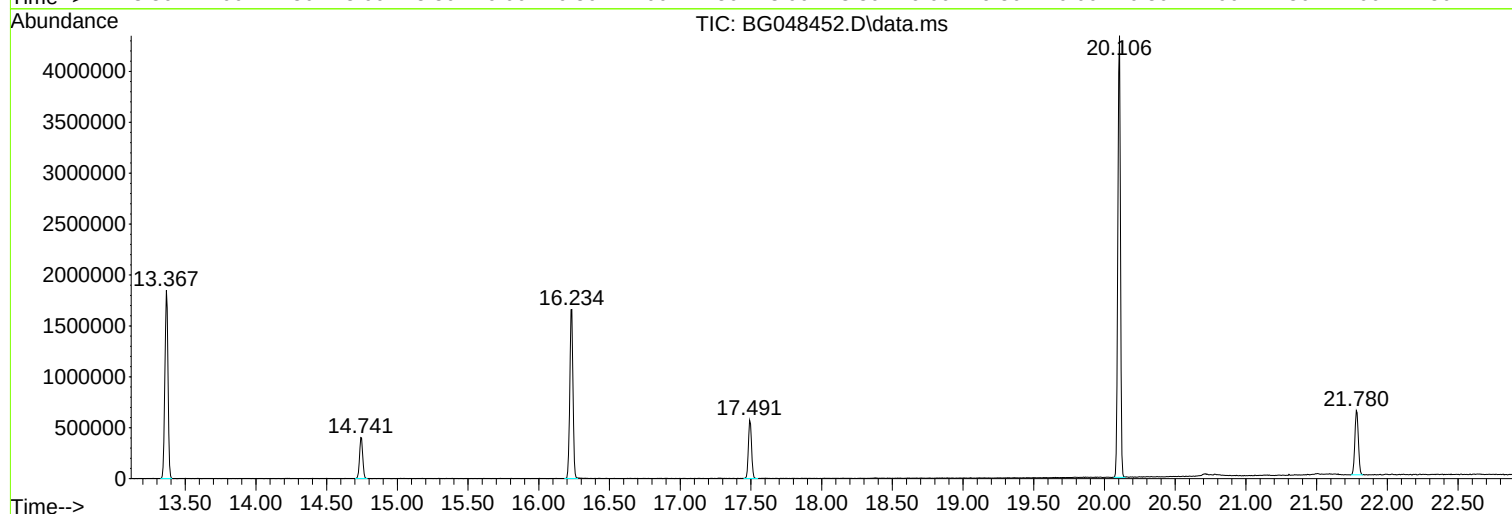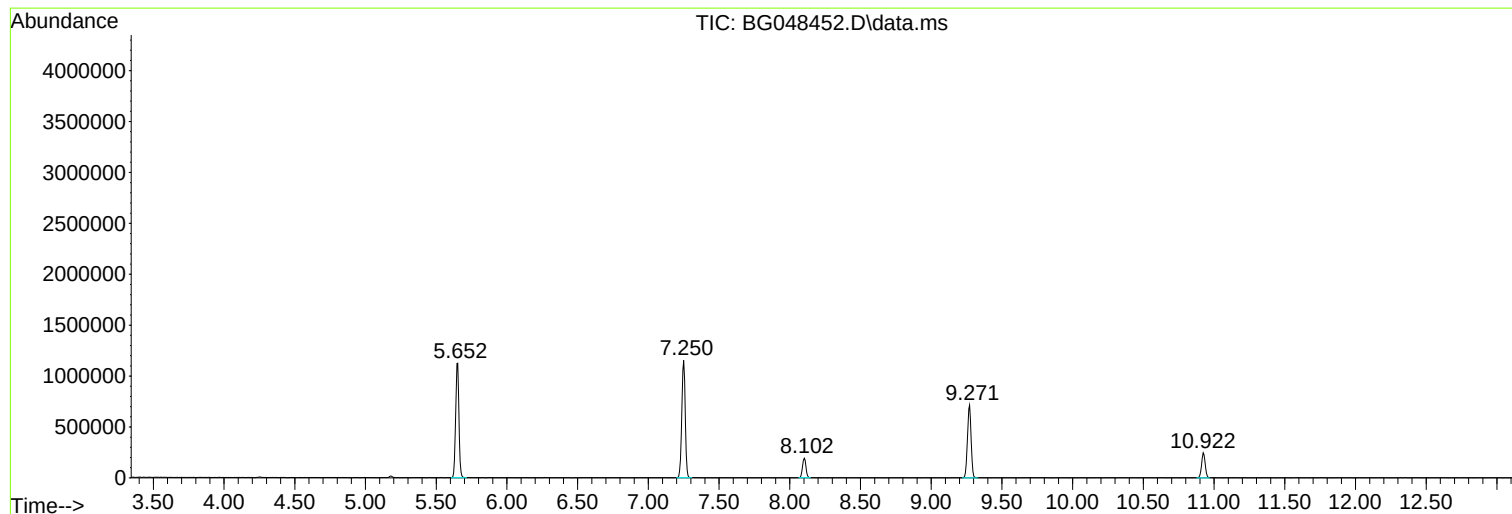

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032221\  
Data File : BG048452.D  
Acq On : 22 Mar 2021 21:15  
Operator : CG/JU  
Sample : PB135234BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135234BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032221\  
Data File : BG048452.D  
Acq On : 22 Mar 2021 21:15  
Operator : CG/JU  
Sample : PB135234BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135234BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|