
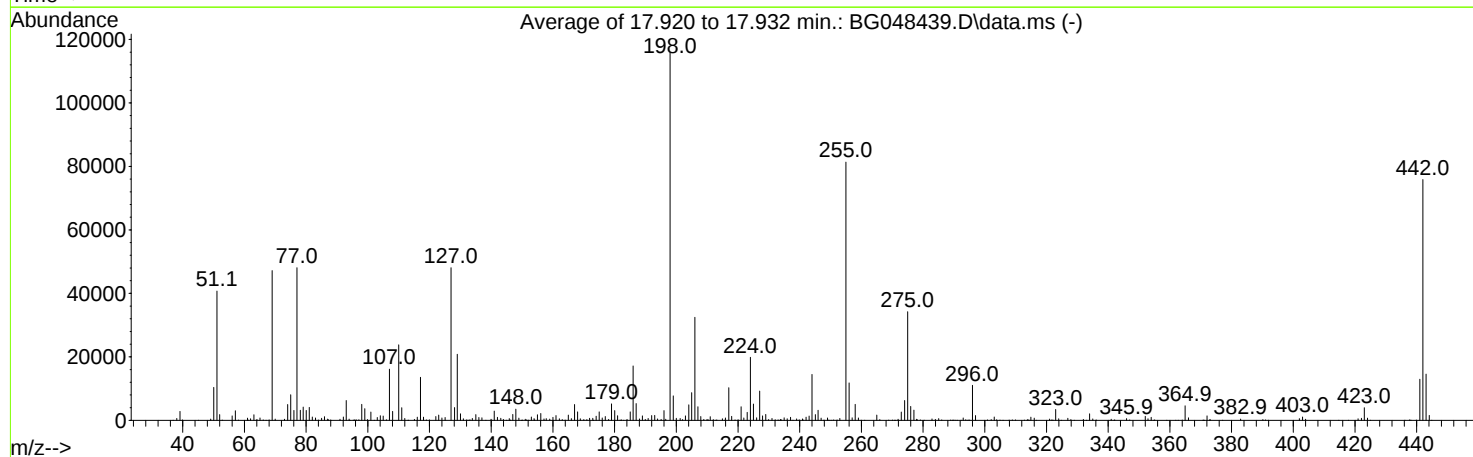


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
 Data File : BG048439.D
 Acq On : 22 Mar 2021 9:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 22 11:22:24 2021

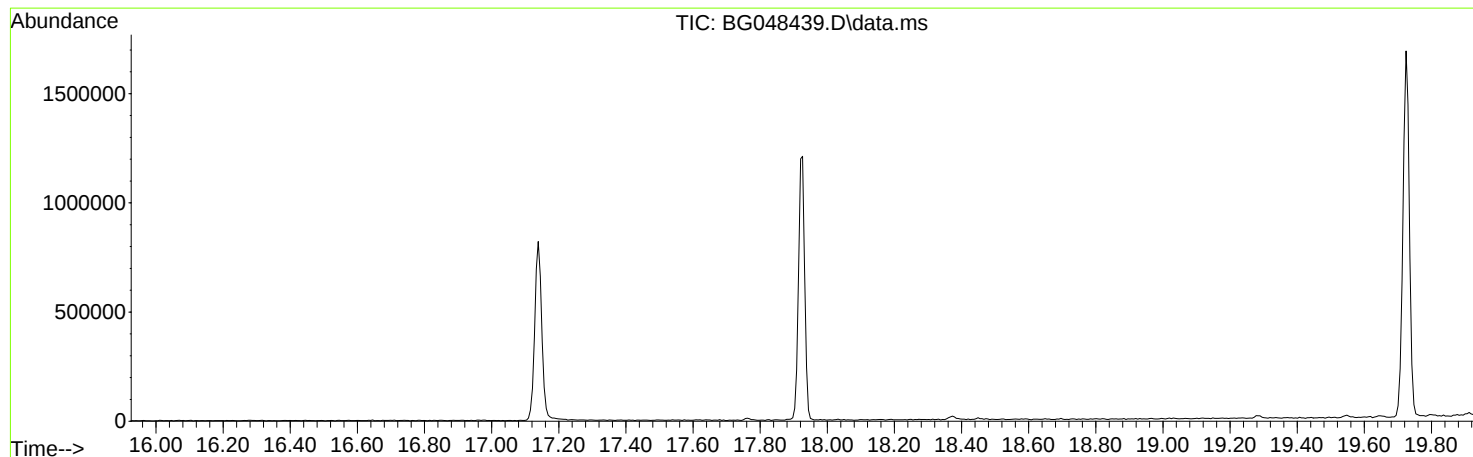

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	40707	PASS
68	69	0.00	2	0.3	150	PASS
69	198	0.00	100	40.7	47187	PASS
70	69	0.00	2	0.9	402	PASS
127	198	10	80	41.5	48091	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	115883	PASS
199	198	5	9	6.7	7707	PASS
275	198	10	60	29.5	34232	PASS
365	198	1	100	4.0	4611	PASS
441	198	0.01	100	11.2	12963	PASS
442	198	50	100	65.4	75843	PASS
443	442	15	24	19.2	14585	PASS

Instrument :
BNA_G
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2021	BNA_G	<u>BG048439.D</u>
Compound Name	Response	Retention Time
DDT	427816	20.96
DDD	7413	20.51
DDE	746	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8159	435975	1.87

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048439.D
Acq On : 22 Mar 2021 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 22 10:58:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration

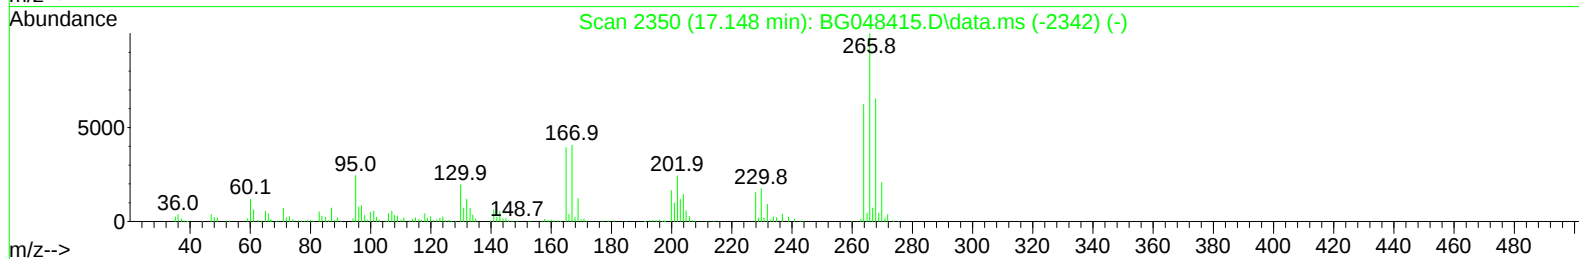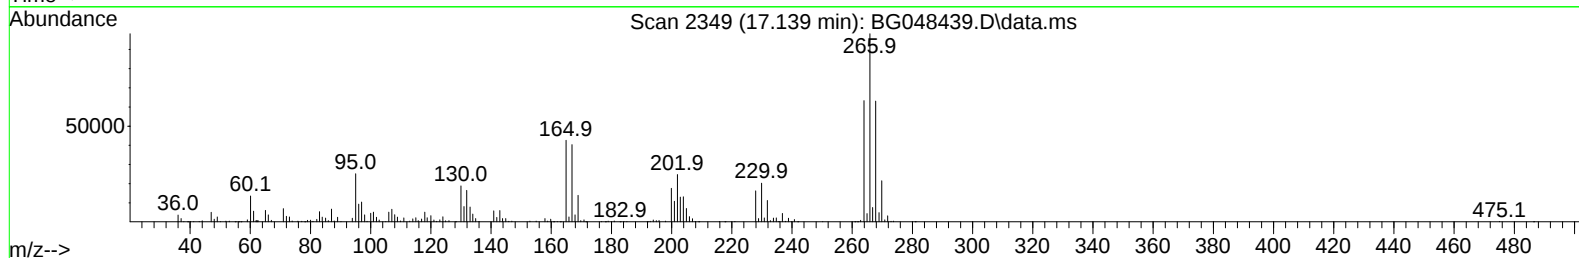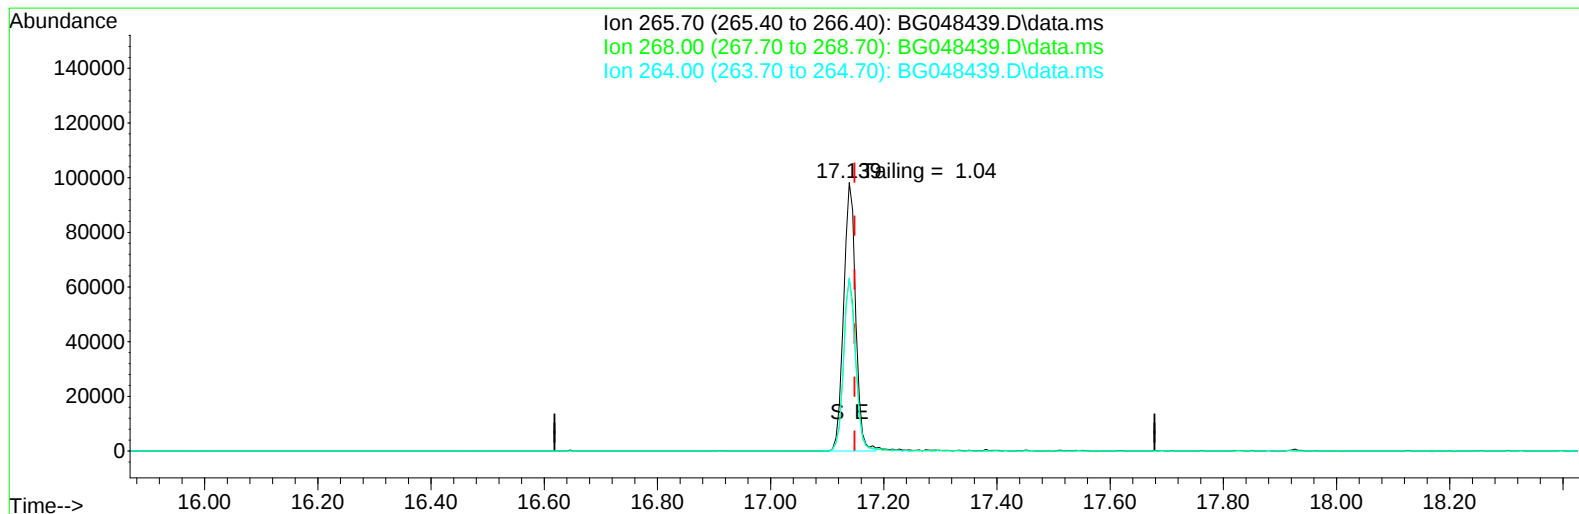

TIC: BG048439.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.009) 210849.83 ng




response 145653

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.25
264.00	61.60	64.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048439.D
Acq On : 22 Mar 2021 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 22 10:58:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration

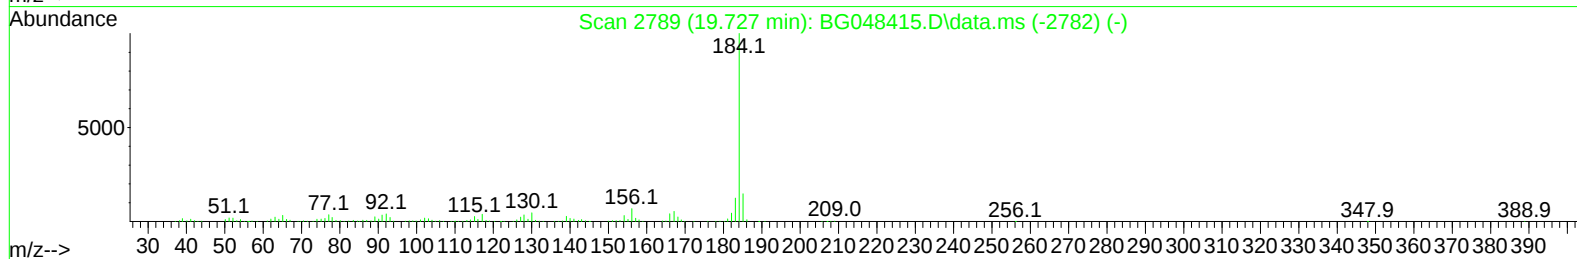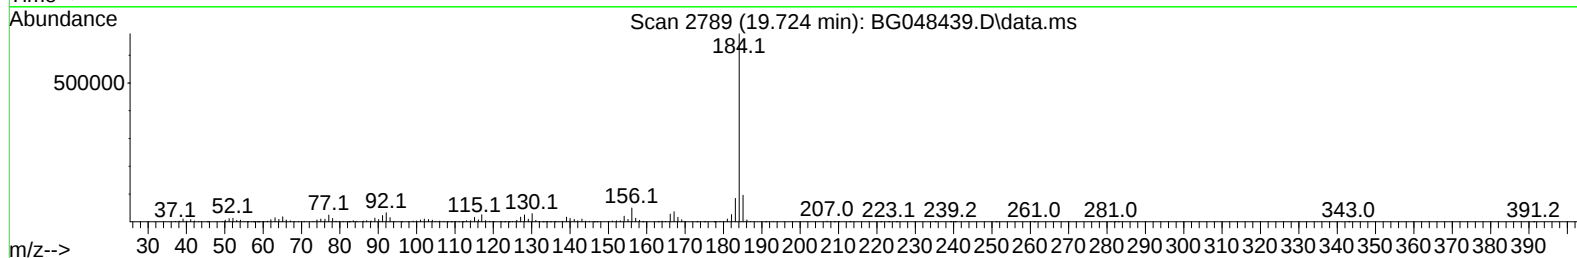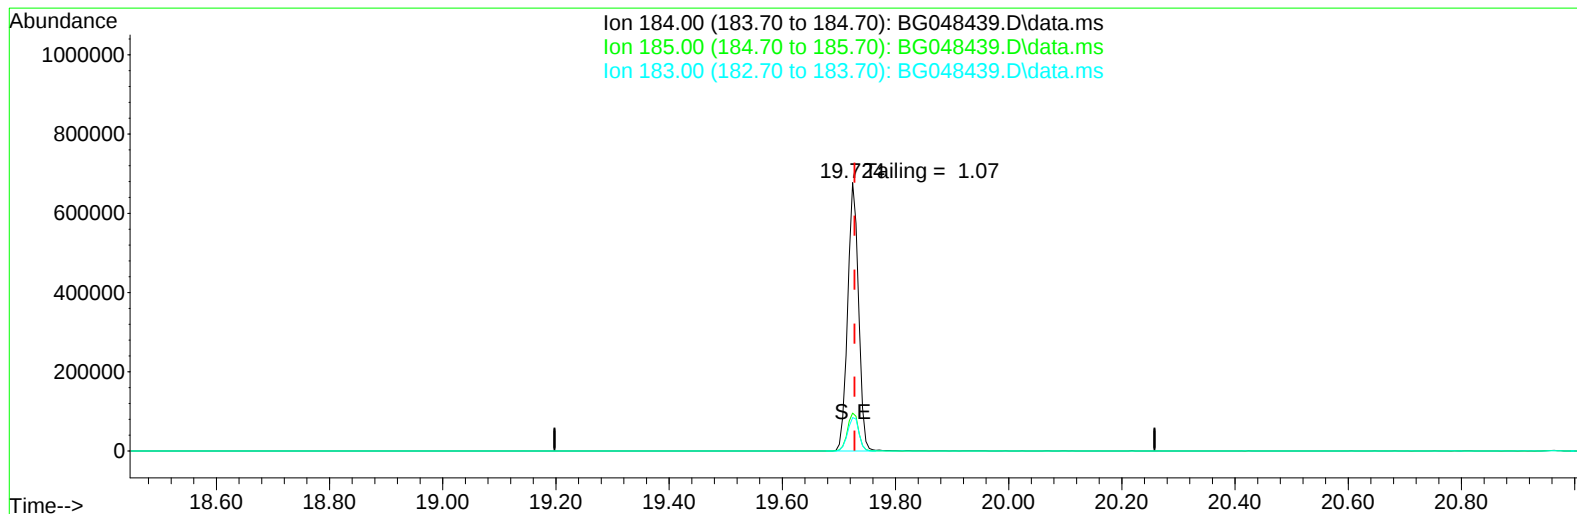

TIC: BG048439.D\data.ms

(77) Benzidine

19.724min (-0.003) 449969.80 ng

response 903077

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.16
183.00	13.20	12.47
0.00	0.00	0.00