
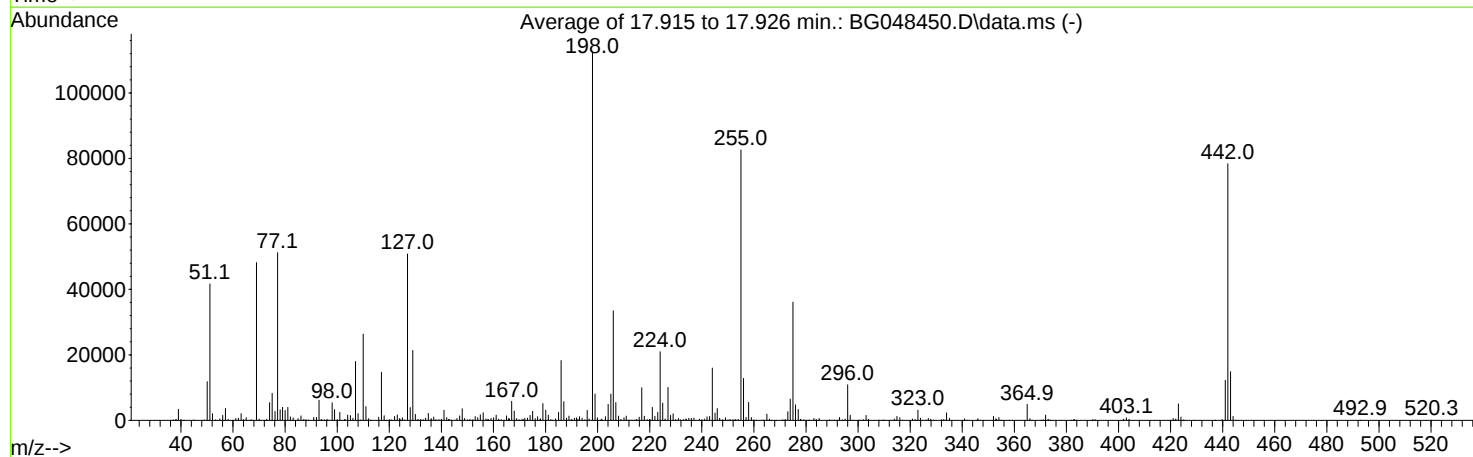


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
 Data File : BG048450.D
 Acq On : 22 Mar 2021 19:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 22 11:22:24 2021

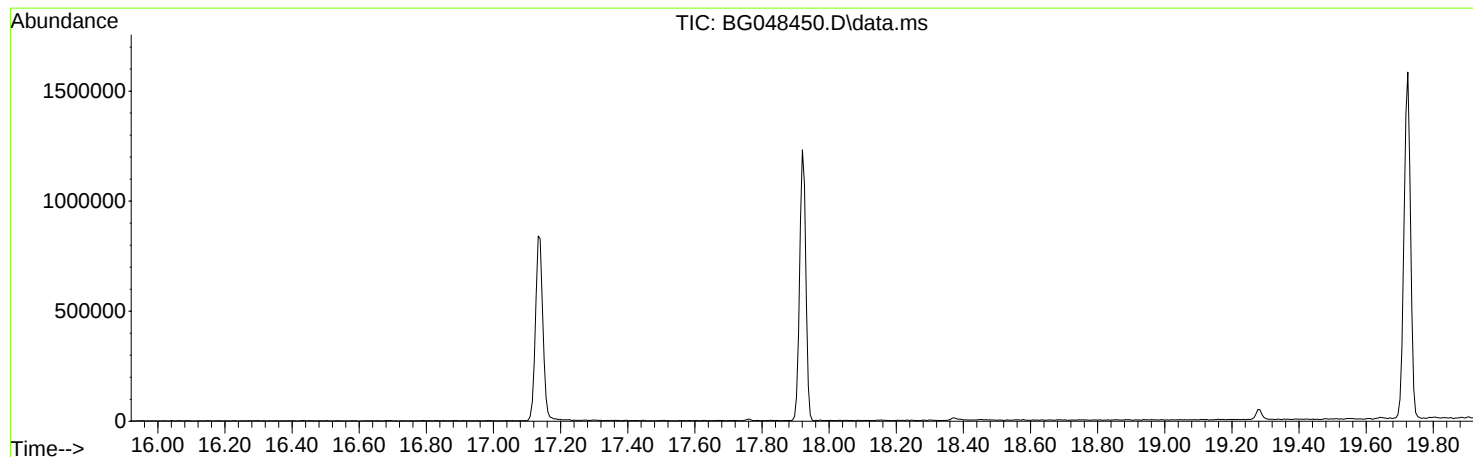

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	41667	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.9	48184	PASS
70	69	0.00	2	0.8	375	PASS
127	198	10	80	45.2	50821	PASS
197	198	0.00	2	0.4	447	PASS
198	198	100	100	100.0	112339	PASS
199	198	5	9	7.2	8077	PASS
275	198	10	60	32.2	36117	PASS
365	198	1	100	4.3	4873	PASS
441	198	0.01	100	10.9	12224	PASS
442	198	50	100	69.8	78392	PASS
443	442	15	24	19.0	14865	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/22/2021	BNA_G	<u>BG048450.D</u>
Compound Name	Response	Retention Time
DDT	461931	20.958
DDD	12830	20.511
DDE	889	20.006
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13719	475650	2.88

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
 Data File : BG048450.D
 Acq On : 22 Mar 2021 19:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 09:03:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 22 11:22:24 2021
 Response via : Initial Calibration

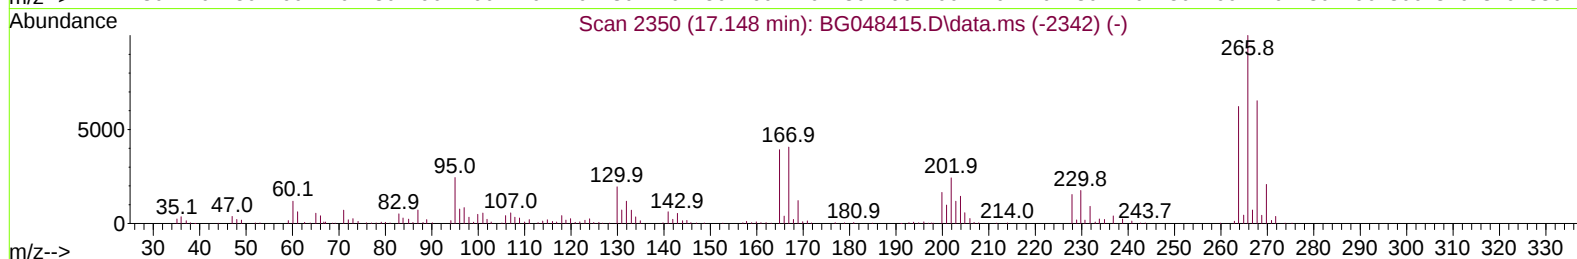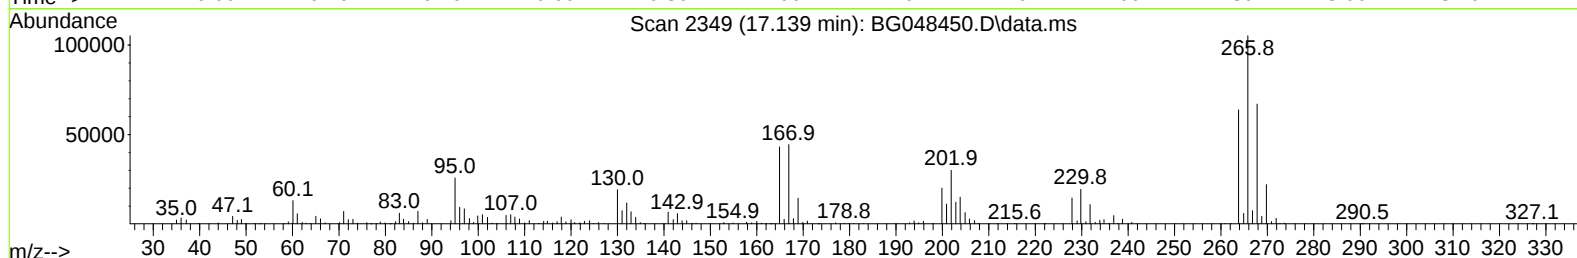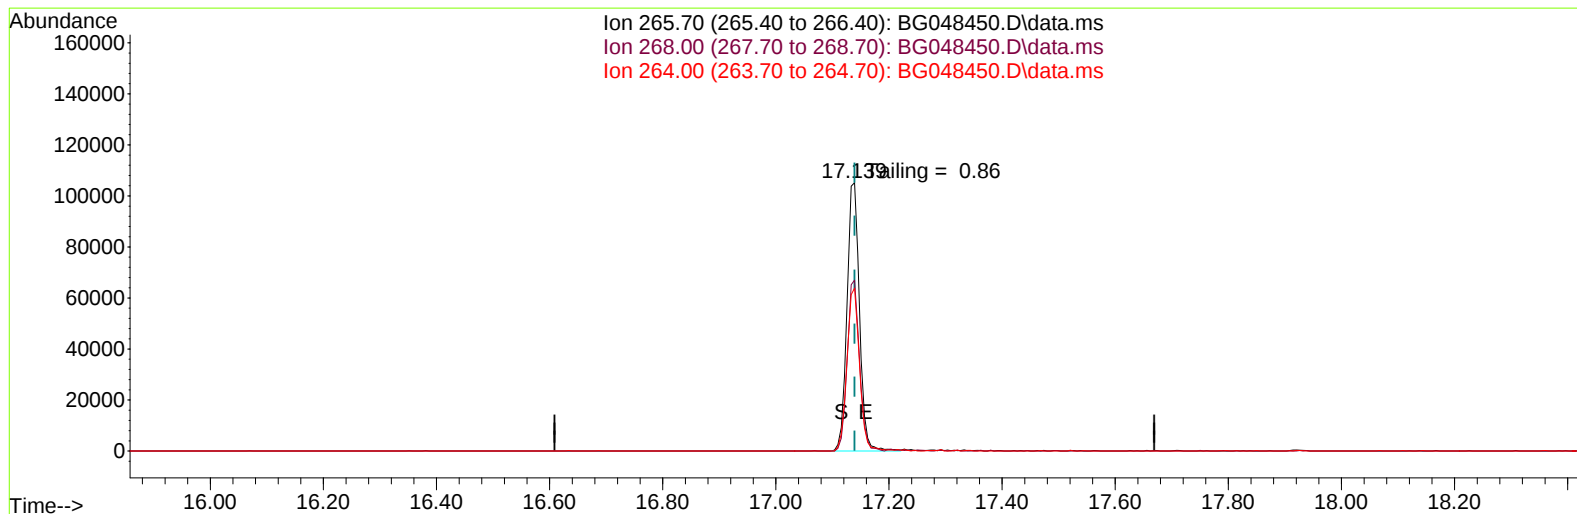

TIC: BG048450.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.000) 260802.64 ng




response 161442

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.68
264.00	61.60	60.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032221\
Data File : BG048450.D
Acq On : 22 Mar 2021 19:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 23 09:03:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 22 11:22:24 2021
Response via : Initial Calibration

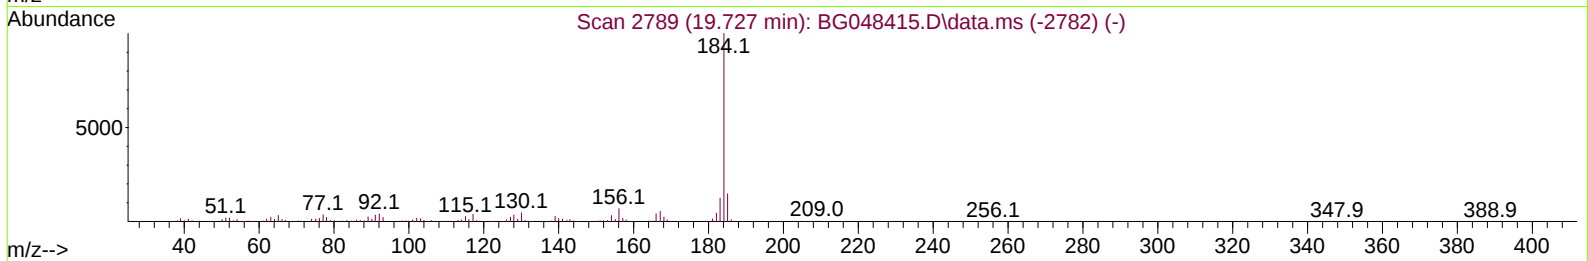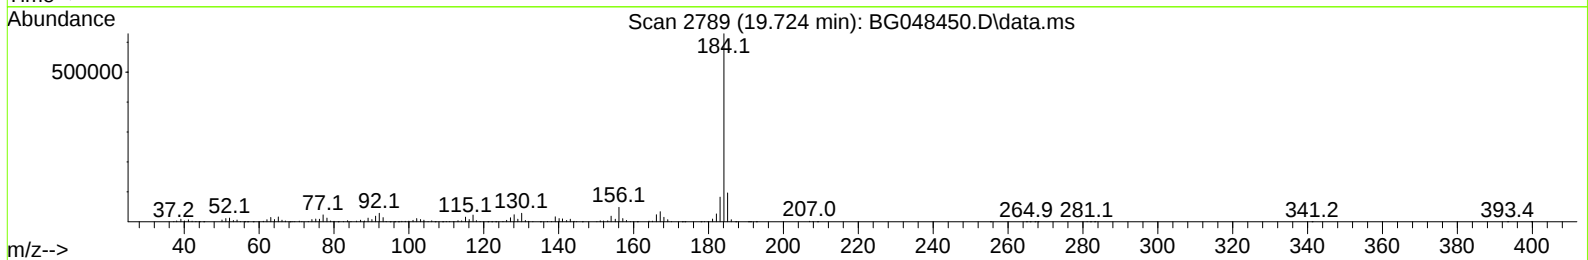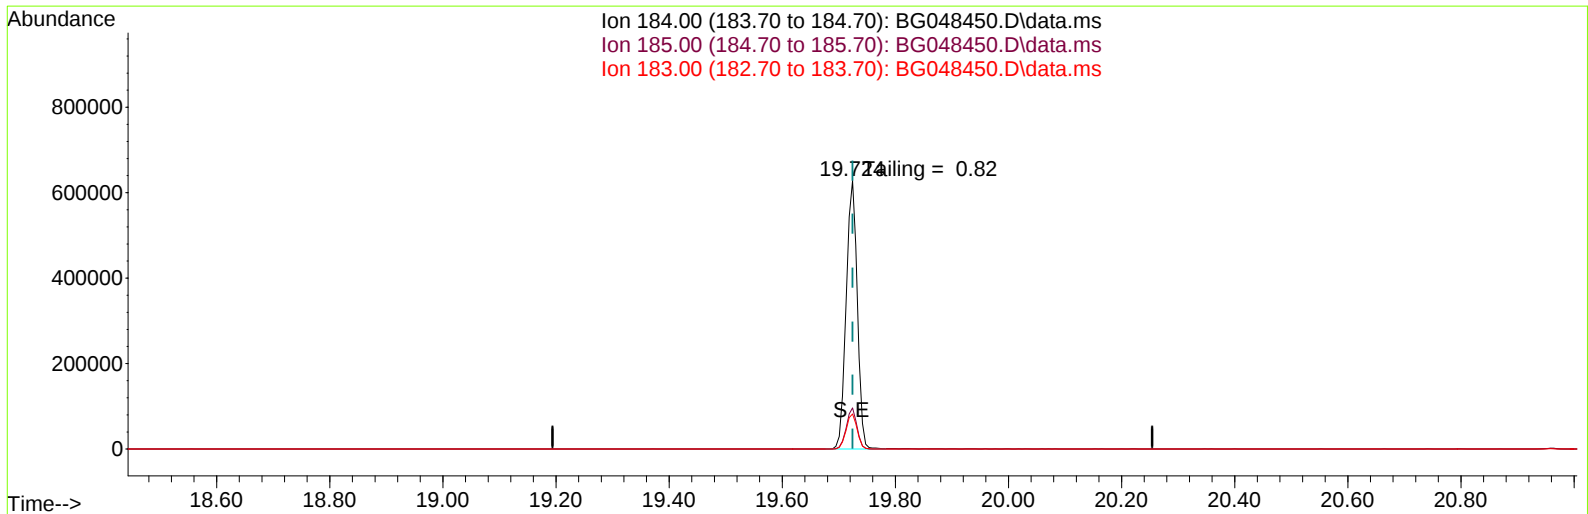

TIC: BG048450.D\data.ms

(77) Benzidine

19.724min (-0.000) 55160.16 ng

response 857550

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.32
183.00	13.20	13.10
0.00	0.00	0.00