
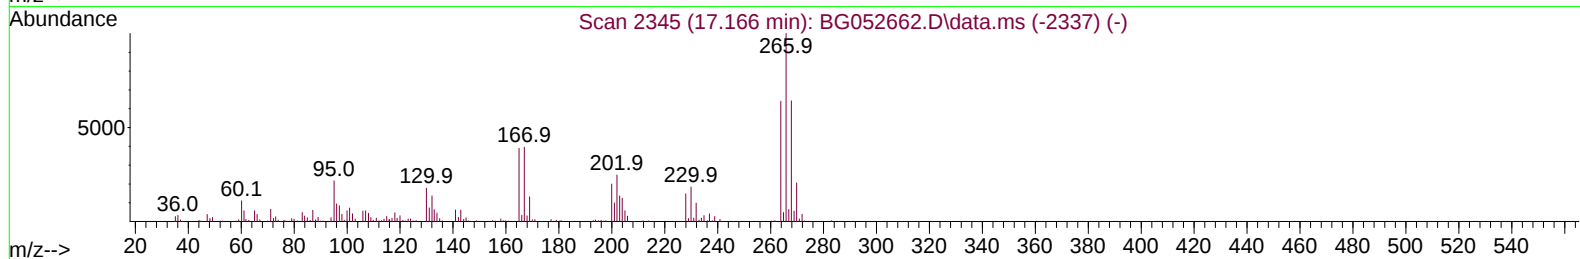
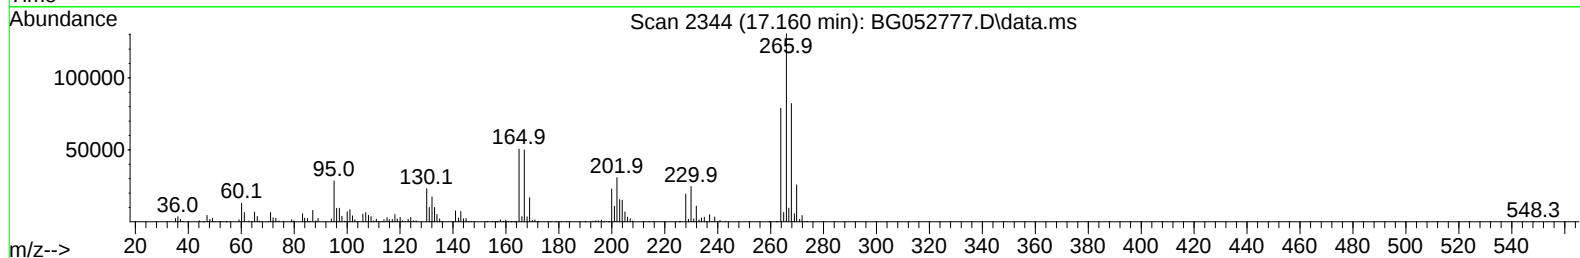


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
 Data File : BG052777.D
 Acq On : 22 Mar 2022 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 18:41:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

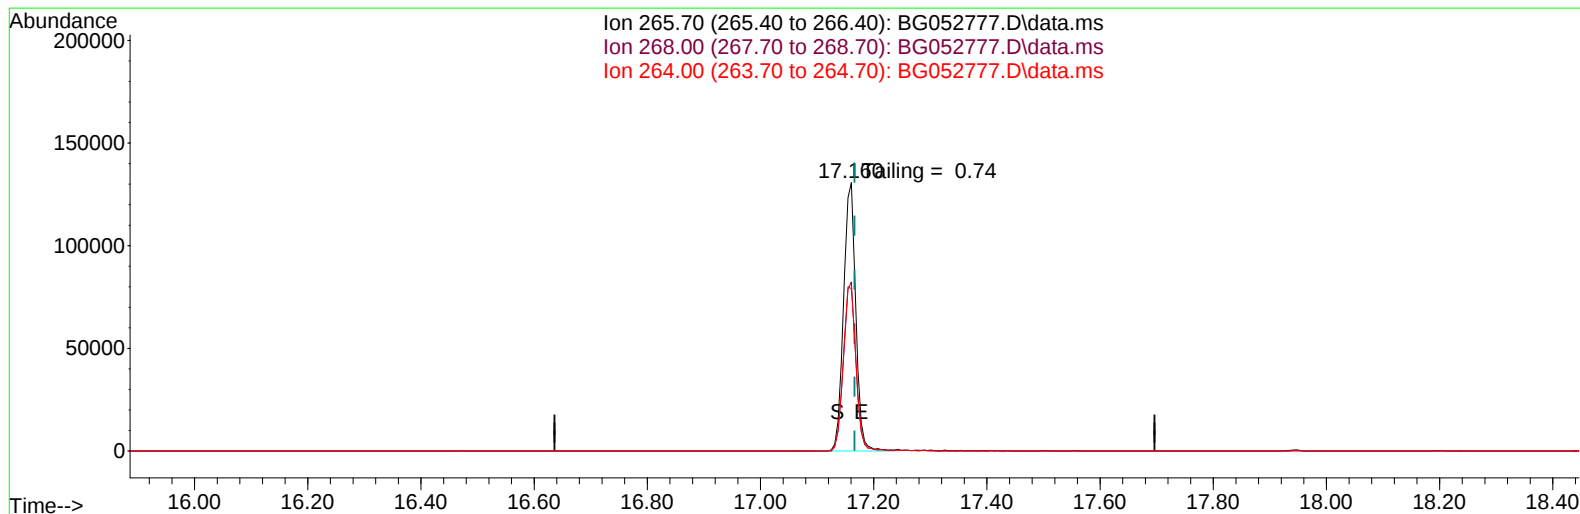




TIC: BG052777.D\data.ms

(70) Pentachlorophenol (C)**17.160min (-0.006) 29586.41 ng****response 195998**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	62.95
264.00	56.60	60.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
 Data File : BG052777.D
 Acq On : 22 Mar 2022 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 18:41:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

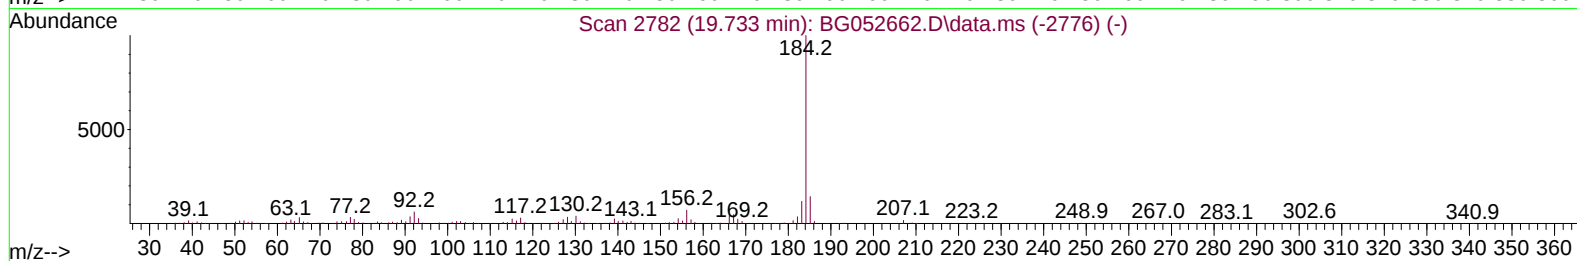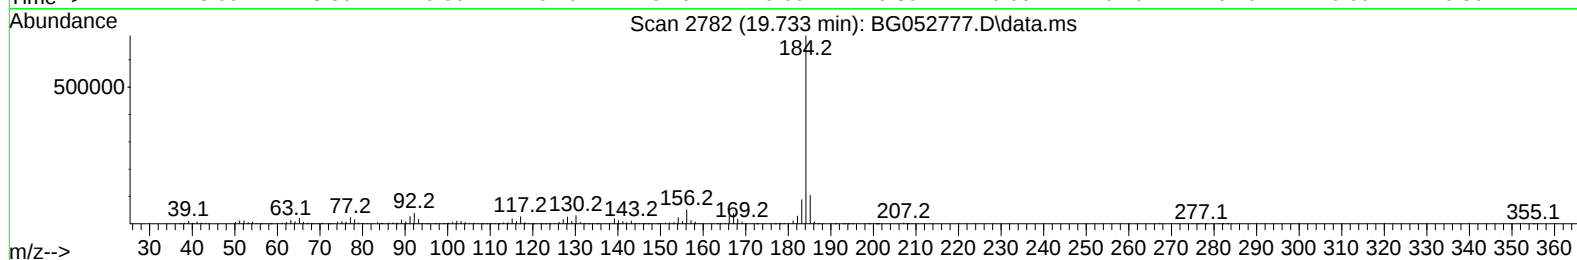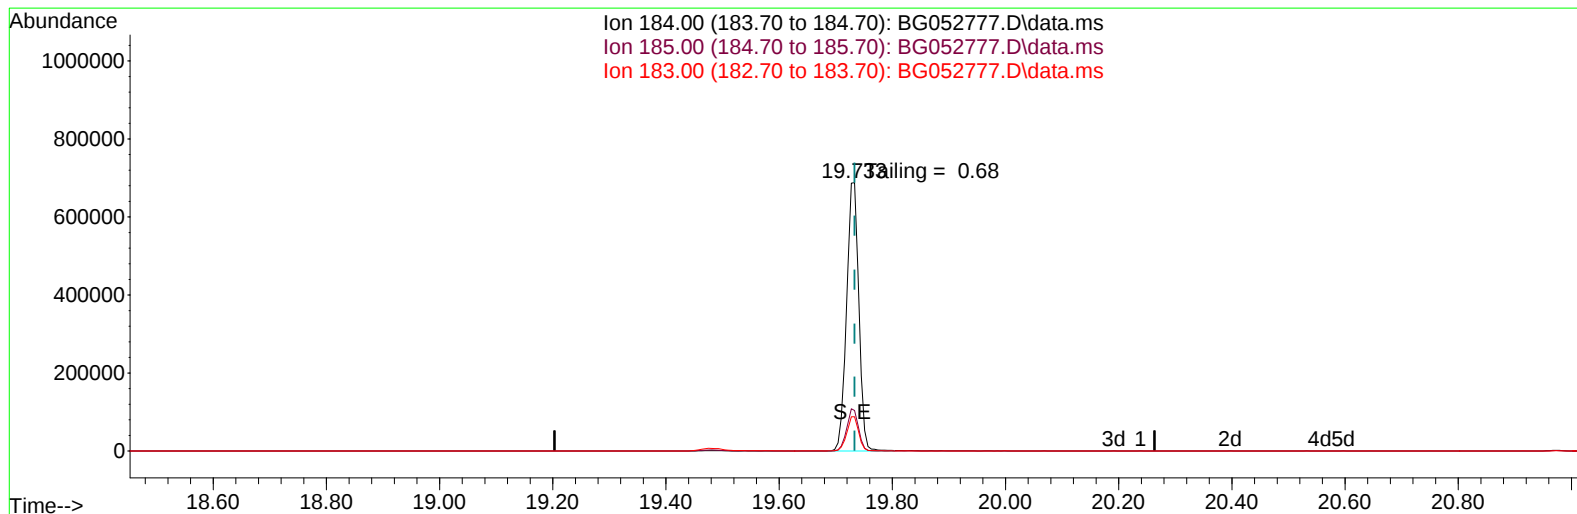

TIC: BG052777.D\data.ms

(77) Benzidine

19.733min (+ 0.000) 734572.27 ng m

response 1042035

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.11
183.00	11.80	12.79
0.00	0.00	0.00