

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
 Data File : BG052788.D
 Acq On : 22 Mar 2022 16:54
 Operator : CG/JU
 Sample : N1974-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B-3RE

Quant Time: Mar 22 17:37:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.142	152	37369	20.000	ng	-0.02
21) Naphthalene-d8	10.956	136	152252	20.000	ng	-0.02
39) Acenaphthene-d10	14.762	164	70942	20.000	ng	-0.01
64) Phenanthrene-d10	17.506	188	250778	20.000	ng	-0.01
76) Chrysene-d12	21.794	240	193374	20.000	ng	-0.02
86) Perylene-d12	25.107	264	41561	20.000	ng	#-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.704	112	258833	120.624	ng	0.00
7) Phenol-d6	7.290	99	289886	89.610	ng	0.00
23) Nitrobenzene-d5	9.305	82	285188	94.013	ng	-0.01
42) 2,4,6-Tribromophenol	16.249	330	204043	214.045	ng	-0.01
45) 2-Fluorobiphenyl	13.394	172	621082	129.120	ng	-0.01
79) Terphenyl-d14	20.114	244	1186063	109.106	ng	-0.01
Target Compounds						
32) Benzoic acid	10.174	122	11943	12.250	ng	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
Data File : BG052788.D
Acq On : 22 Mar 2022 16:54
Operator : CG/JU
Sample : N1974-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B-3RE

Quant Time: Mar 22 17:37:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 15:56:10 2022
Response via : Initial Calibration




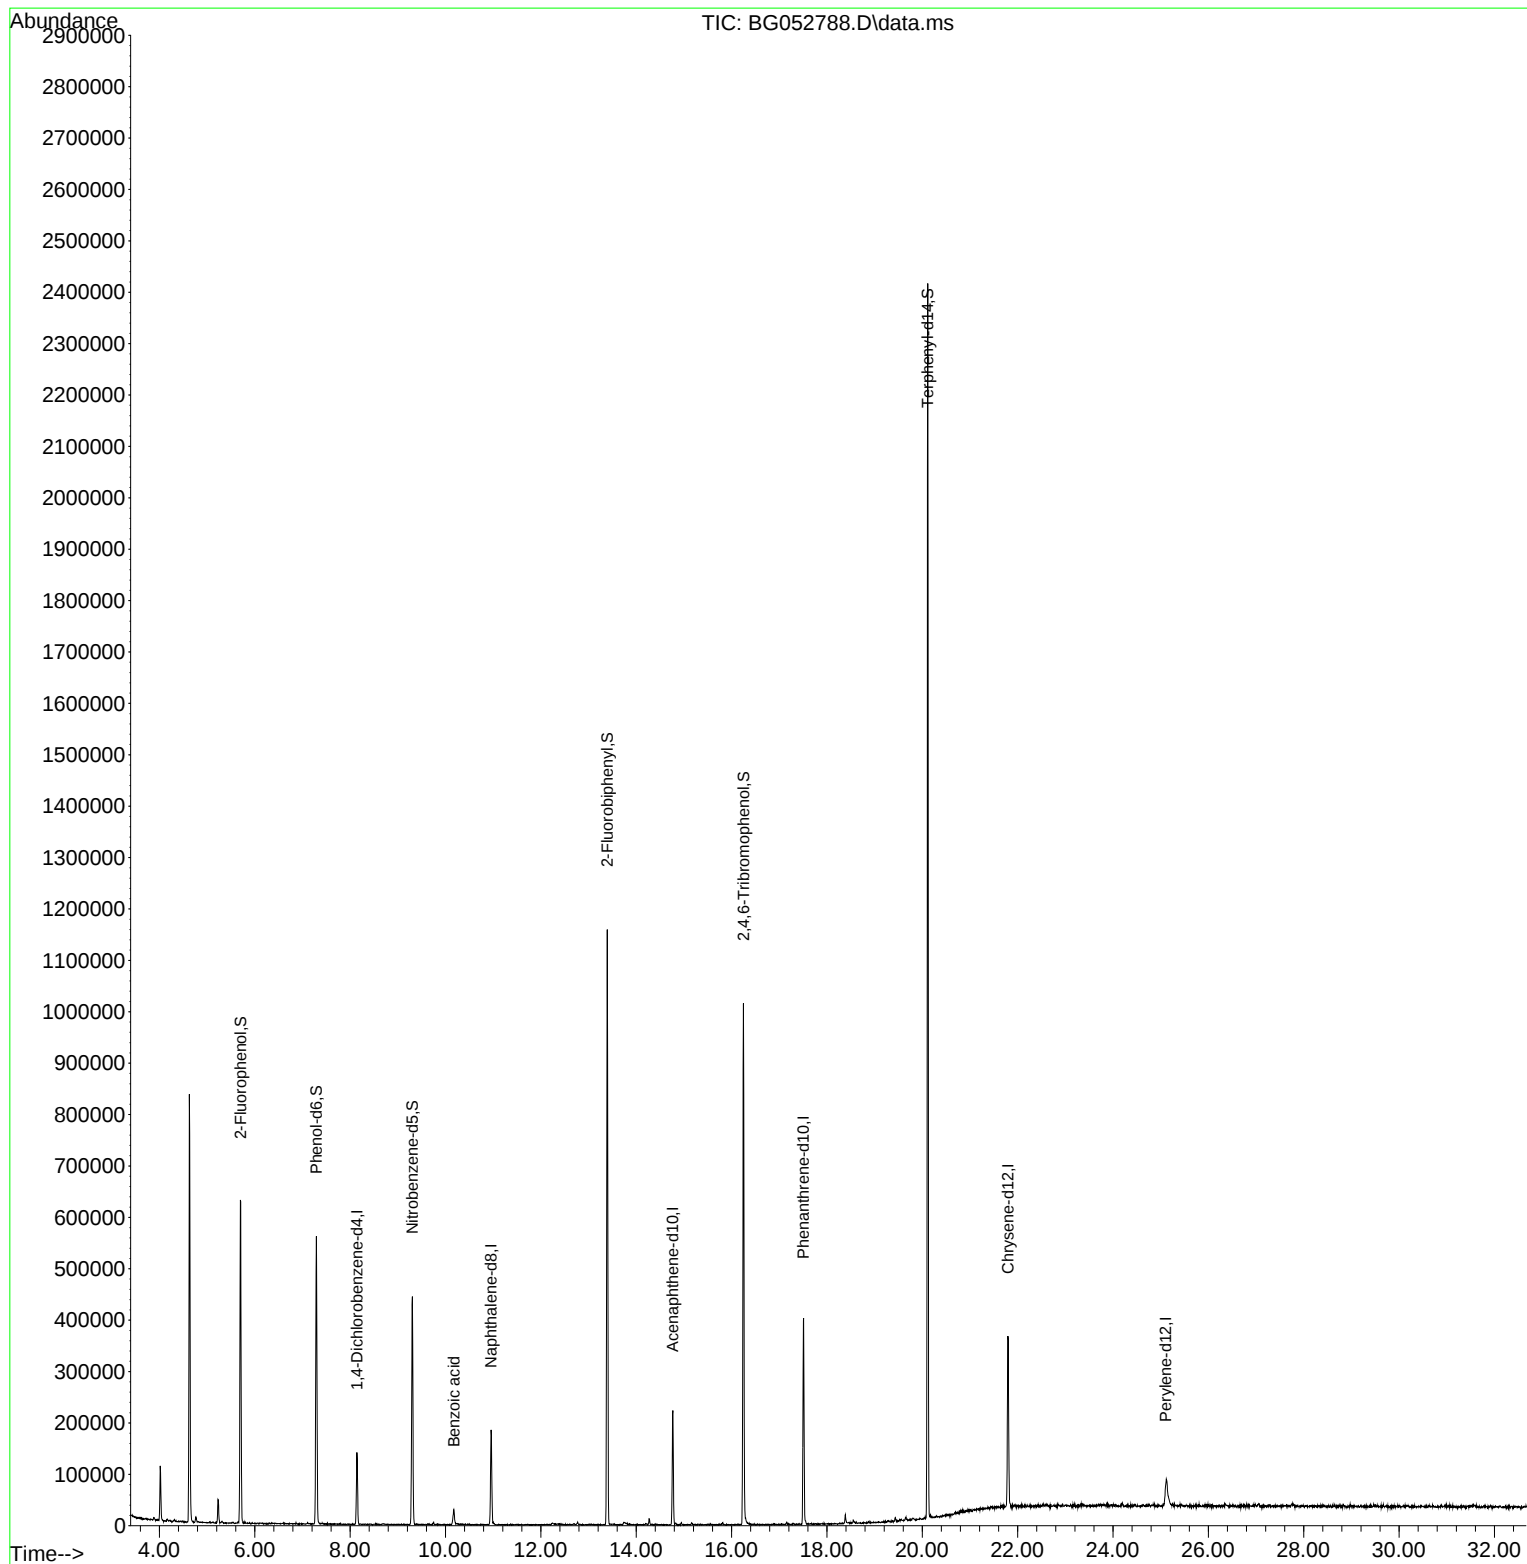


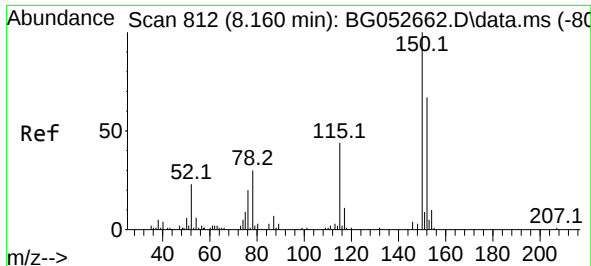

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.142 min Scan# 809
Delta R.T. -0.018 min
Lab File: BG052788.D
Acq: 22 Mar 2022 16:54




Instrument :
BNA_G
ClientSampleId :
B-3RE

Tgt Ion:152 Resp: 37369
Ion Ratio Lower Upper
152 100
150 156.9 114.6 172.0
115 60.6 45.9 68.9

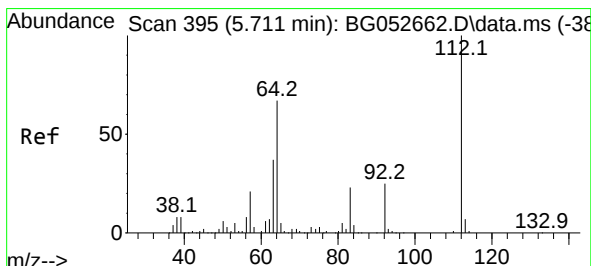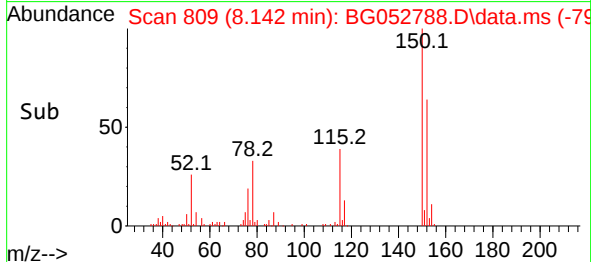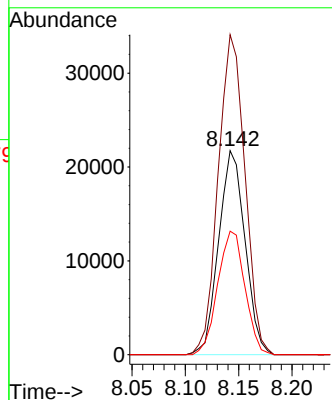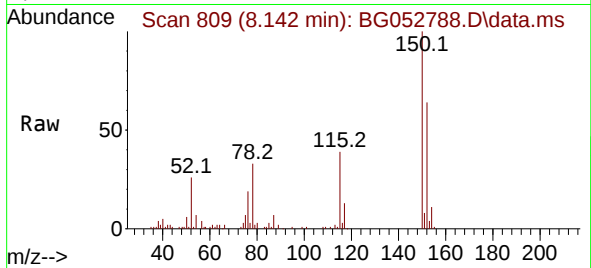

#5
2-Fluorophenol
Concen: 120.624 ng
RT: 5.704 min Scan# 394
Delta R.T. -0.007 min
Lab File: BG052788.D
Acq: 22 Mar 2022 16:54

Tgt Ion:112 Resp: 258833
Ion Ratio Lower Upper
112 100
64 70.1 48.0 72.0
63 39.9 26.5 39.7#


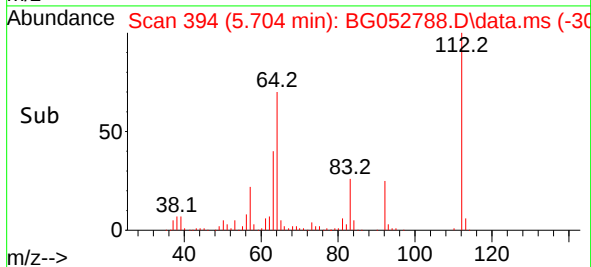
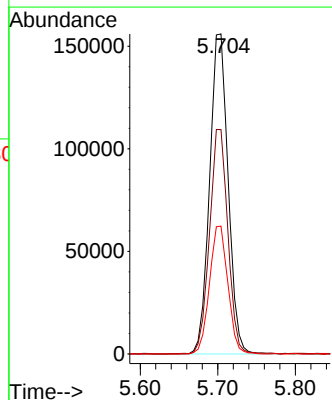
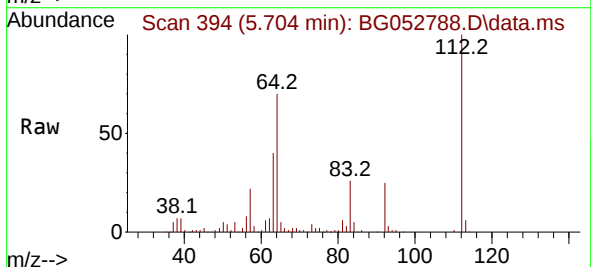




#7
Phenol-d6
Concen: 89.610 ng
RT: 7.290 min Scan# 60
Delta R.T. -0.007 min
Lab File: BG052788.D
Acq: 22 Mar 2022 16:54




Instrument :
BNA_G
ClientSampleId :
B-3RE


Tgt Ion: 99 Resp: 289886
Ion Ratio Lower Upper
99 100
42 20.3 14.7 22.1
71 43.1 29.2 43.8

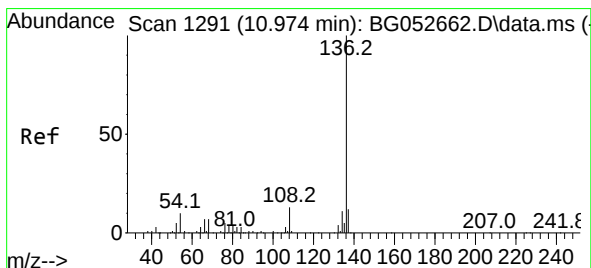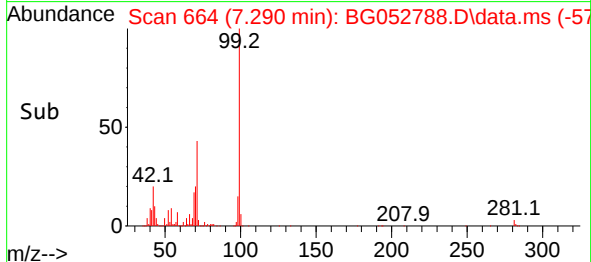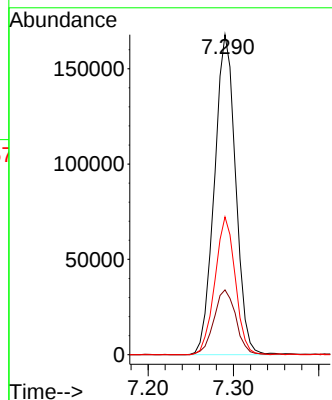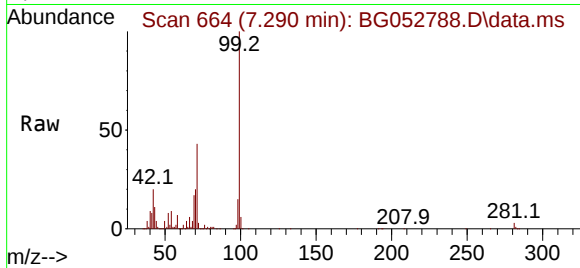

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.956 min Scan# 1288
Delta R.T. -0.018 min
Lab File: BG052788.D
Acq: 22 Mar 2022 16:54

Tgt Ion: 136 Resp: 152252
Ion Ratio Lower Upper
136 100
137 11.6 9.4 14.2
54 9.5 6.4 9.6
68 6.9 5.0 7.6

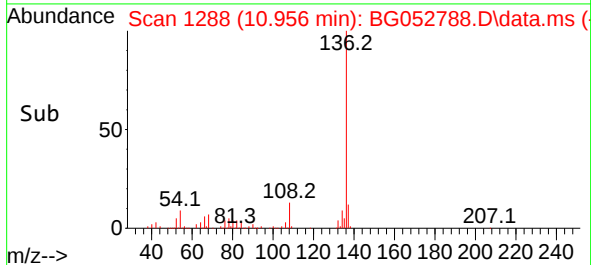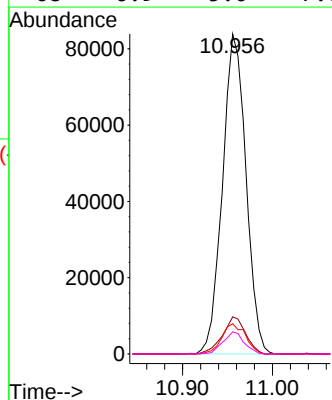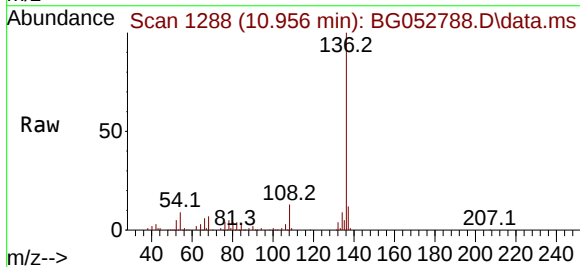

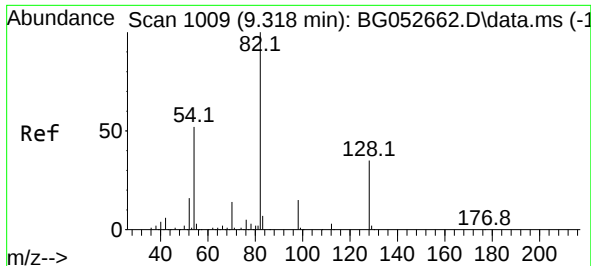

#23

Nitrobenzene-d5

Concen: 94.013 ng

RT: 9.305 min Scan# 1

Delta R.T. -0.013 min

Lab File: BG052788.D

Acq: 22 Mar 2022 16:54

Instrument :

BNA_G

ClientSampleId :

B-3RE





Tgt Ion: 82 Resp: 285188

Ion Ratio Lower Upper

82 100

128 36.0 31.3 46.9

54 49.8 37.8 56.8

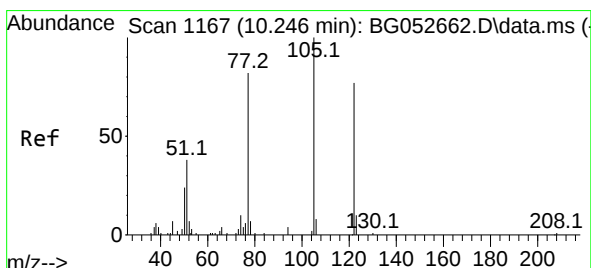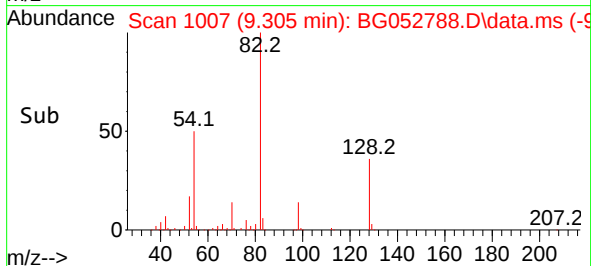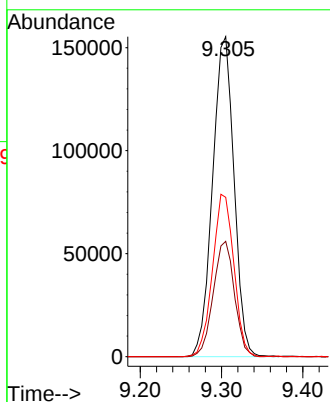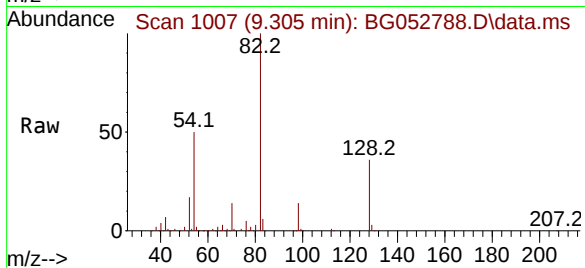

#32

Benzoic acid

Concen: 12.250 ng

RT: 10.174 min Scan# 1155

Delta R.T. -0.072 min

Lab File: BG052788.D

Acq: 22 Mar 2022 16:54




Tgt Ion: 122 Resp: 11943


Ion Ratio Lower Upper

122 100

105 121.4 112.8 152.8

77 101.0 78.4 118.4


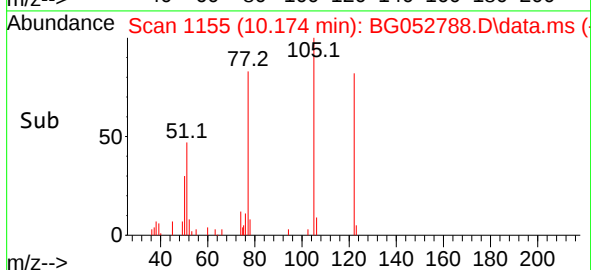
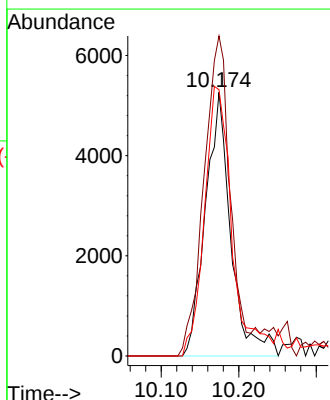
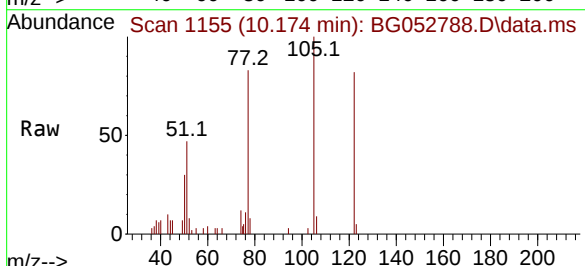


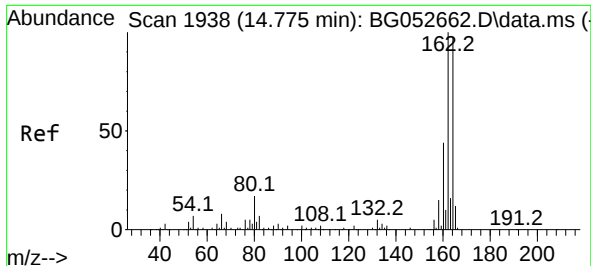

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.762 min Scan# 1936
Delta R.T. -0.013 min
Lab File: BG052788.D
Acq: 22 Mar 2022 16:54




Instrument :
BNA_G
ClientSampleId :
B-3RE


Tgt Ion:164 Resp: 70942
Ion Ratio Lower Upper
164 100
162 103.1 80.0 120.0
160 43.8 38.8 58.2

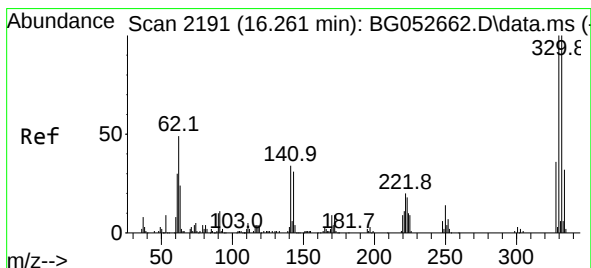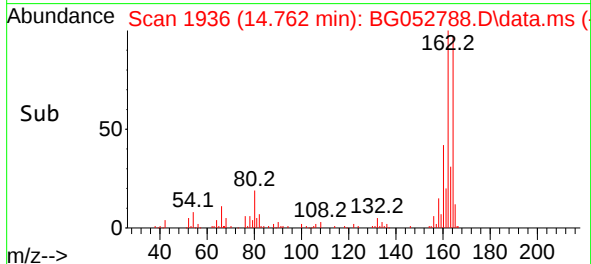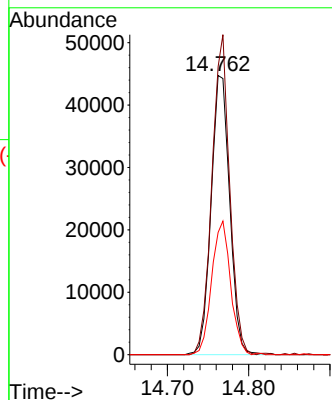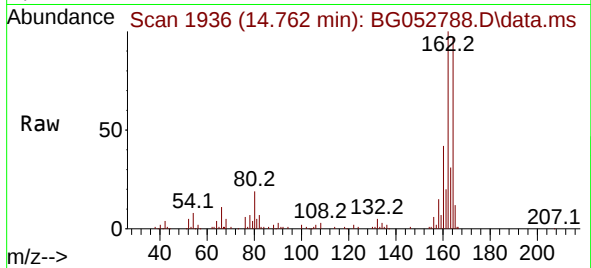

#42
2,4,6-Tribromophenol
Concen: 214.045 ng
RT: 16.249 min Scan# 2189
Delta R.T. -0.013 min
Lab File: BG052788.D
Acq: 22 Mar 2022 16:54

Tgt Ion:330 Resp: 204043
Ion Ratio Lower Upper
330 100
332 95.2 75.8 113.6
141 34.3 24.6 36.8


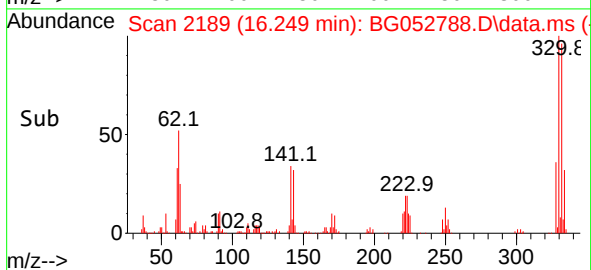
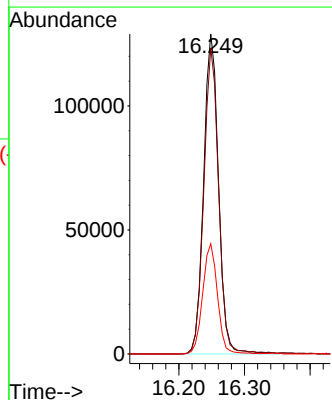
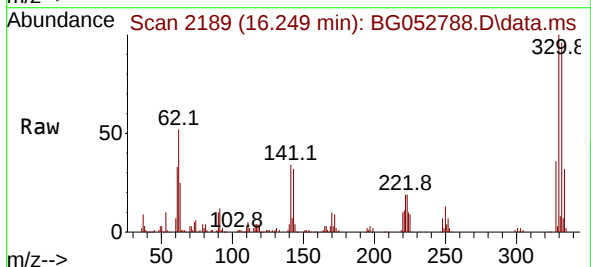


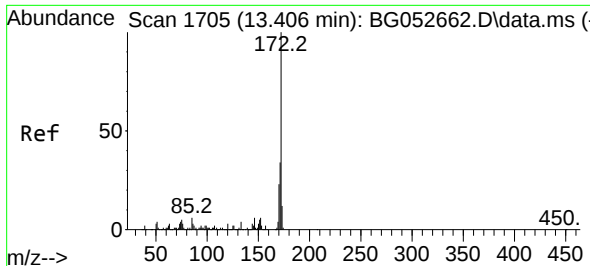

#45
2-Fluorobiphenyl
Concen: 129.120 ng
RT: 13.394 min Scan# 1703
Delta R.T. -0.013 min
Lab File: BG052788.D
Acq: 22 Mar 2022 16:54




Instrument :
BNA_G
ClientSampleId :
B-3RE


Tgt Ion:172 Resp: 621082
Ion Ratio Lower Upper
172 100
171 35.6 28.3 42.5
170 23.2 18.0 27.0

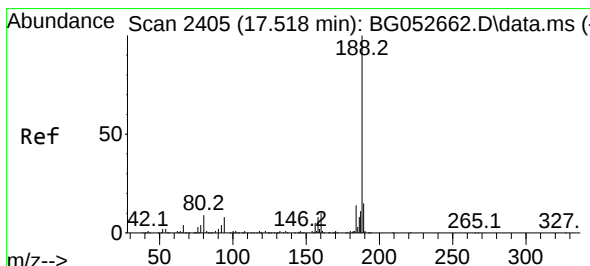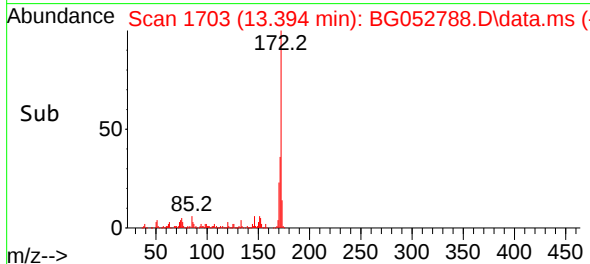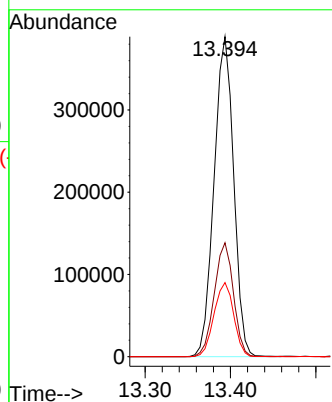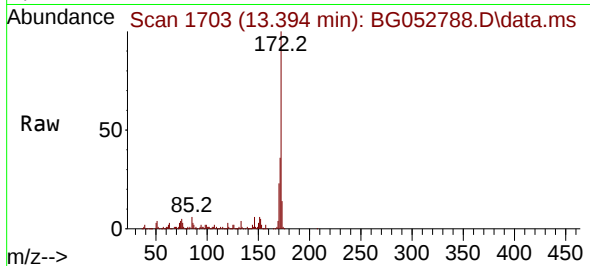

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.506 min Scan# 2403
Delta R.T. -0.013 min
Lab File: BG052788.D
Acq: 22 Mar 2022 16:54

Tgt Ion:188 Resp: 250778
Ion Ratio Lower Upper
188 100
94 6.9 5.7 8.5
80 8.5 7.2 10.8

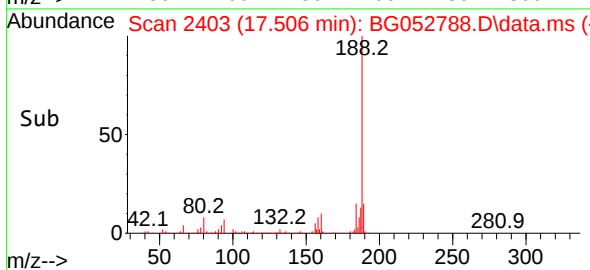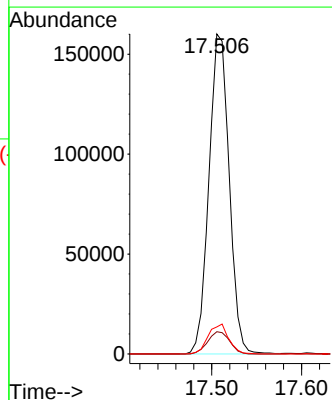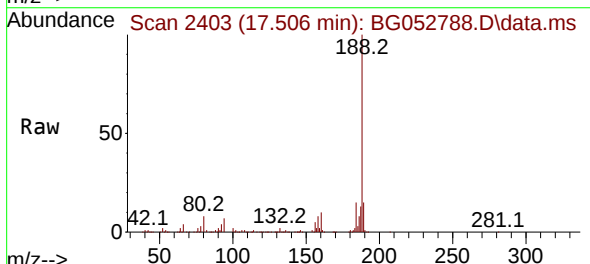

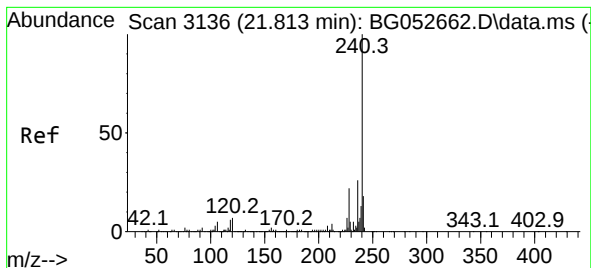

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.794 min Scan# 31

Delta R.T. -0.019 min

Lab File: BG052788.D

Acq: 22 Mar 2022 16:54

Instrument :

BNA_G

ClientSampleId :

B-3RE





Tgt Ion:240 Resp: 193374

Ion Ratio Lower Upper

240 100

120 6.9 5.4 8.0

236 26.7 19.8 29.6

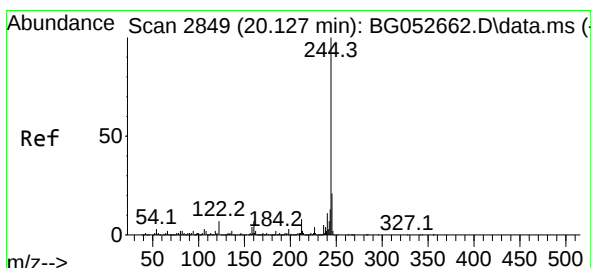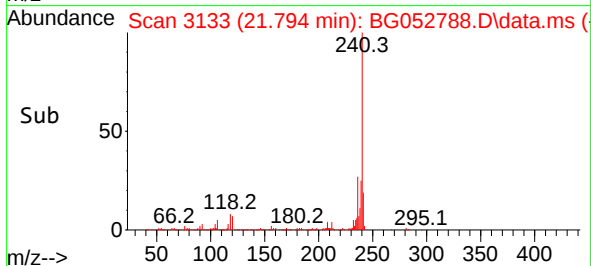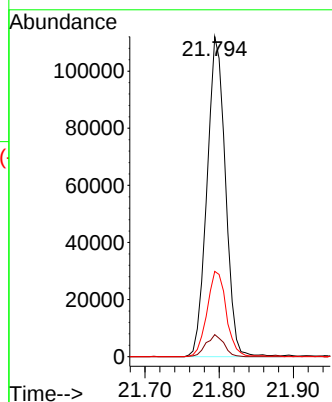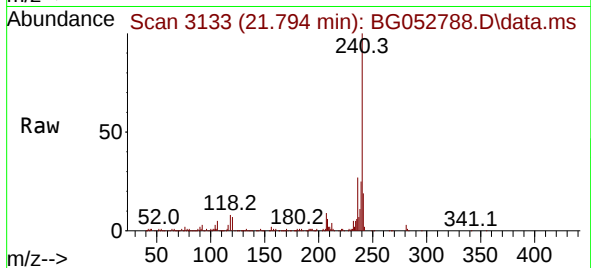

#79

Terphenyl-d14

Concen: 109.106 ng

RT: 20.114 min Scan# 2847

Delta R.T. -0.013 min

Lab File: BG052788.D

Acq: 22 Mar 2022 16:54




Tgt Ion:244 Resp: 1186063


Ion Ratio Lower Upper

244 100

212 8.0 5.4 8.2

122 7.0 5.8 8.6

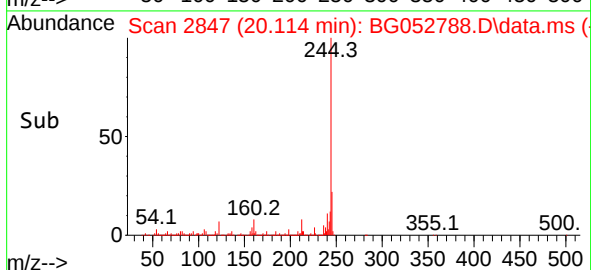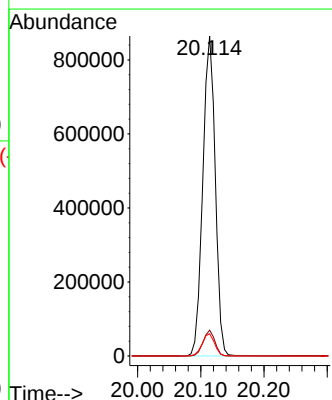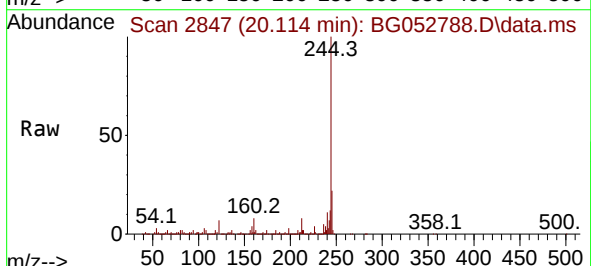

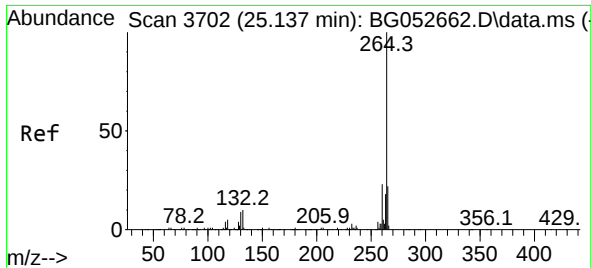

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.107 min Scan# 30
 Delta R.T. -0.030 min
 Lab File: BG052788.D
 Acq: 22 Mar 2022 16:54

Instrument :
 BNA_G
 ClientSampleId :
 B-3RE

Tgt Ion:264 Resp: 41561
 Ion Ratio Lower Upper
 264 100
 260 24.2 18.2 27.2
 265 25.6 15.1 22.7#

