

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
 Data File : BG052779.D
 Acq On : 22 Mar 2022 10:35
 Operator : CG/JU
 Sample : PB143455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143455BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.702	385	394	404	rBV	916086	1472538	36.01%	9.150%
2	7.294	657	665	677	rBV	933038	1606205	39.27%	9.981%
3	8.146	803	810	819	rVB	164945	281069	6.87%	1.747%
4	9.303	999	1007	1017	rBV	574131	1025460	25.07%	6.372%
5	10.960	1282	1289	1297	rVB	217328	396734	9.70%	2.465%
6	13.392	1694	1703	1713	rVB	1556188	2392759	58.51%	14.869%
7	14.766	1926	1937	1944	rBV	381692	575738	14.08%	3.578%
8	16.247	2182	2189	2205	rBV	1205803	1886183	46.12%	11.721%
9	17.510	2397	2404	2412	rVB	482547	741709	18.14%	4.609%
10	20.112	2841	2847	2858	rBV	3040751	4089674	100.00%	25.413%
11	21.798	3127	3134	3142	rBV2	484535	824963	20.17%	5.126%
12	25.117	3688	3699	3709	rBV2	274127	799495	19.55%	4.968%




Sum of corrected areas: 16092527

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
Data File : BG052779.D
Acq On : 22 Mar 2022 10:35
Operator : CG/JU
Sample : PB143455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143455BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

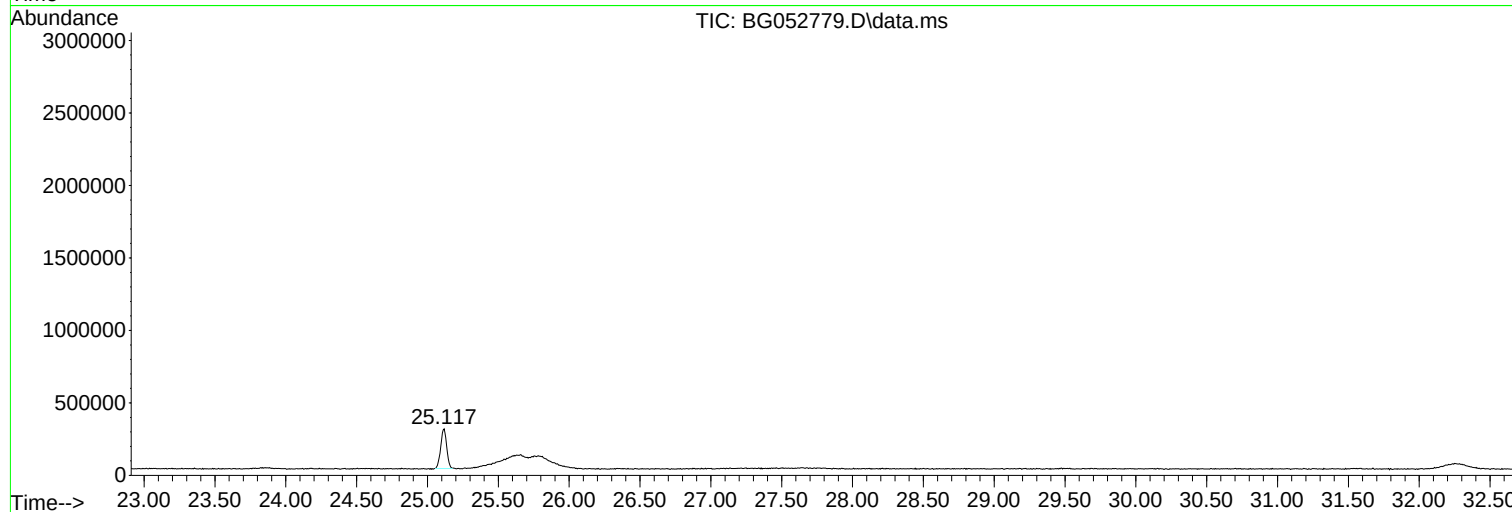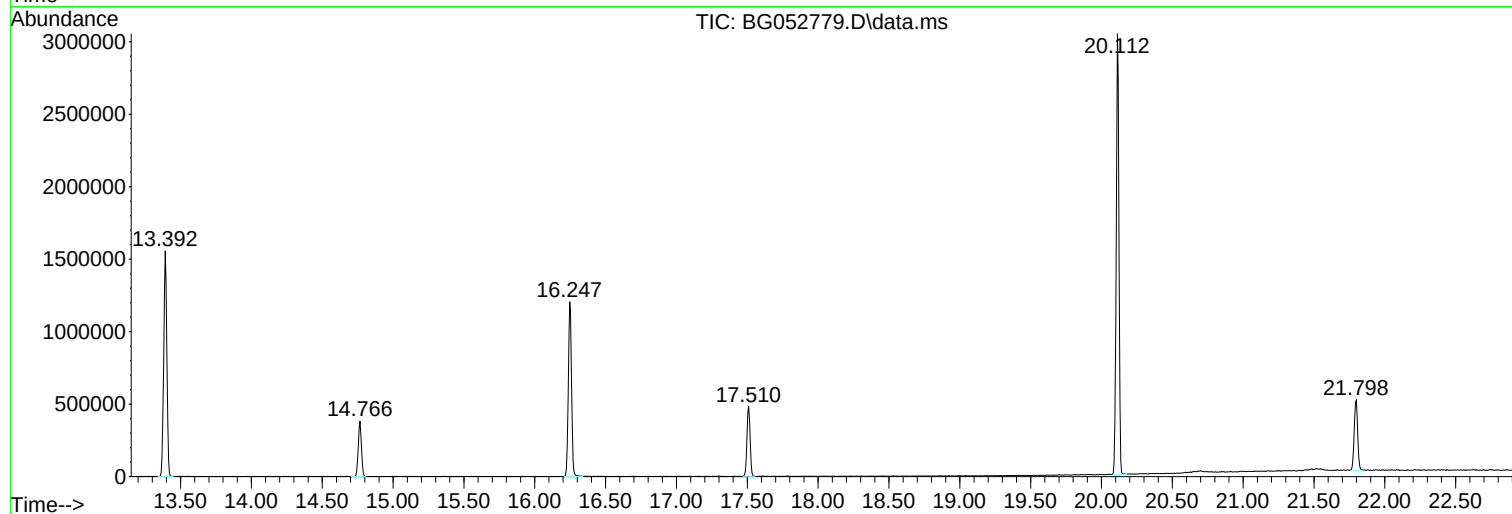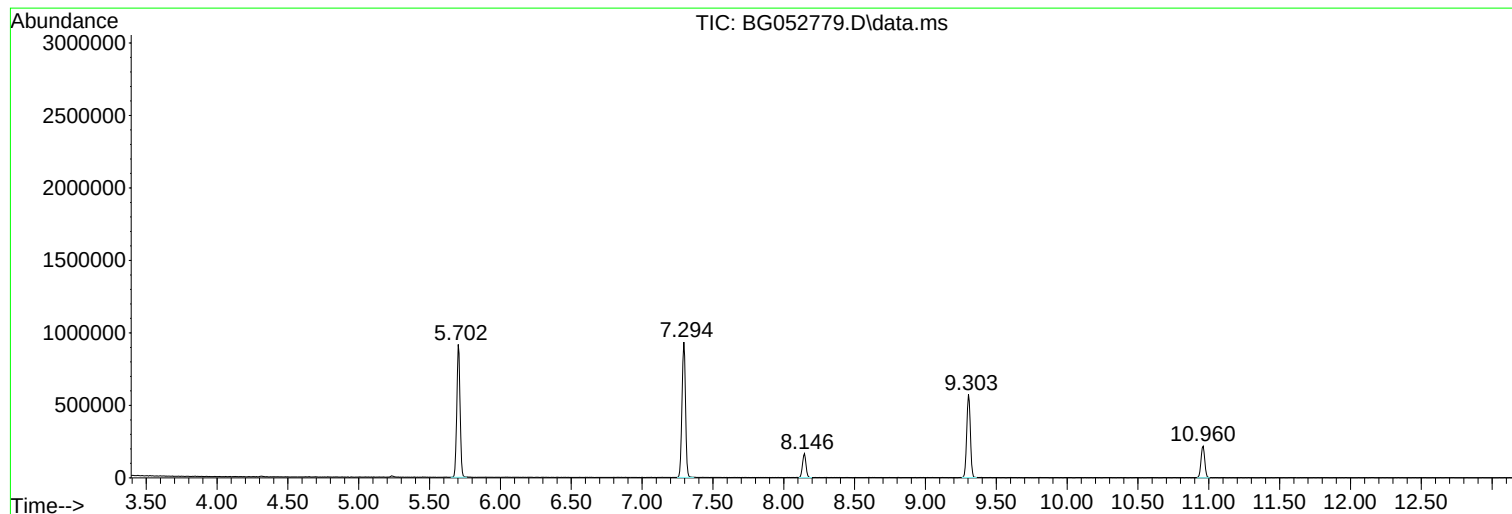

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
Data File : BG052779.D
Acq On : 22 Mar 2022 10:35
Operator : CG/JU
Sample : PB143455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143455BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
Data File : BG052779.D
Acq On : 22 Mar 2022 10:35
Operator : CG/JU
Sample : PB143455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143455BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------