
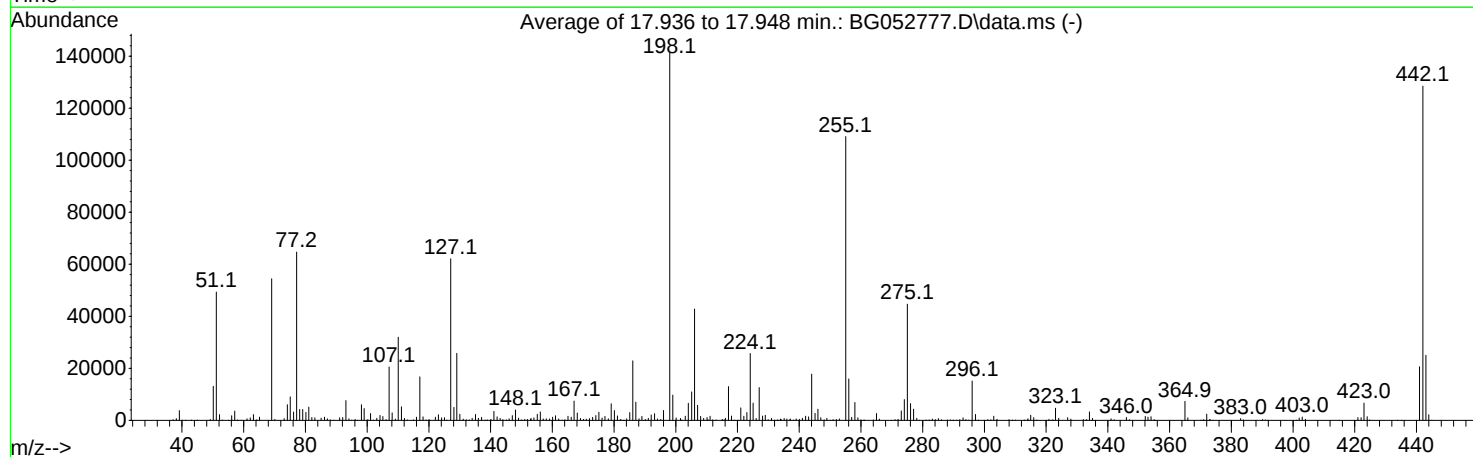


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
 Data File : BG052777.D
 Acq On : 22 Mar 2022 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 15 15:56:10 2022

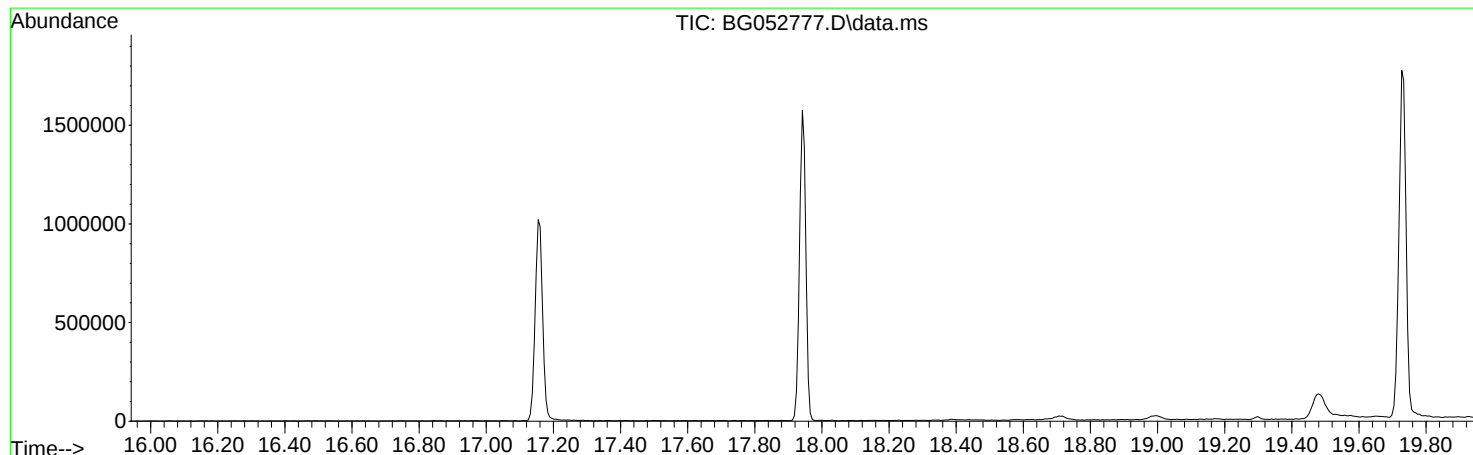




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	49320	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.5	54429	PASS
70	69	0.00	2	0.7	377	PASS
127	198	10	80	43.9	62131	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	141395	PASS
199	198	5	9	6.9	9743	PASS
275	198	10	60	31.6	44637	PASS
365	198	1	100	5.2	7312	PASS
441	198	0.01	100	14.6	20599	PASS
442	442	50	100	100.0	128477	PASS
443	442	15	24	19.5	25037	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
 Data File : BG052777.D
 Acq On : 22 Mar 2022 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 18:41:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

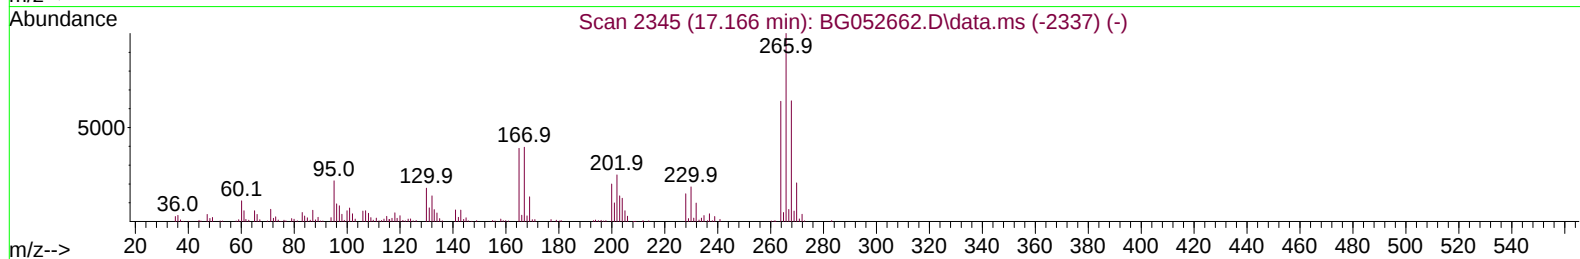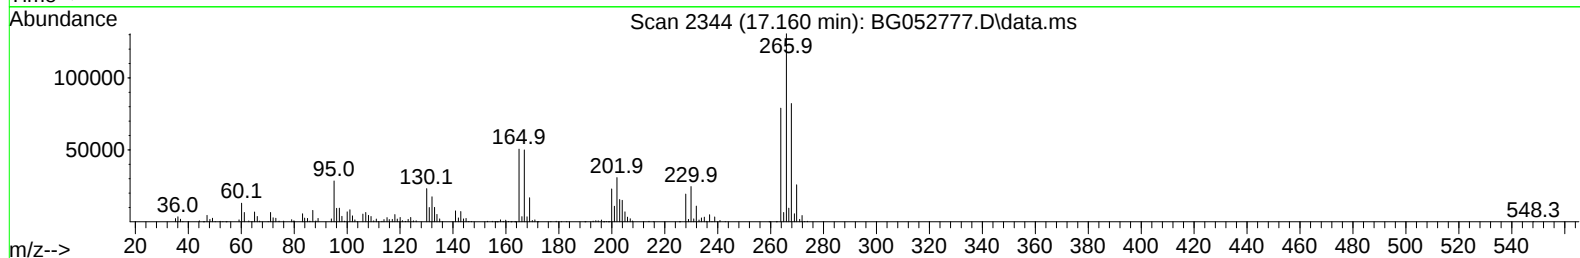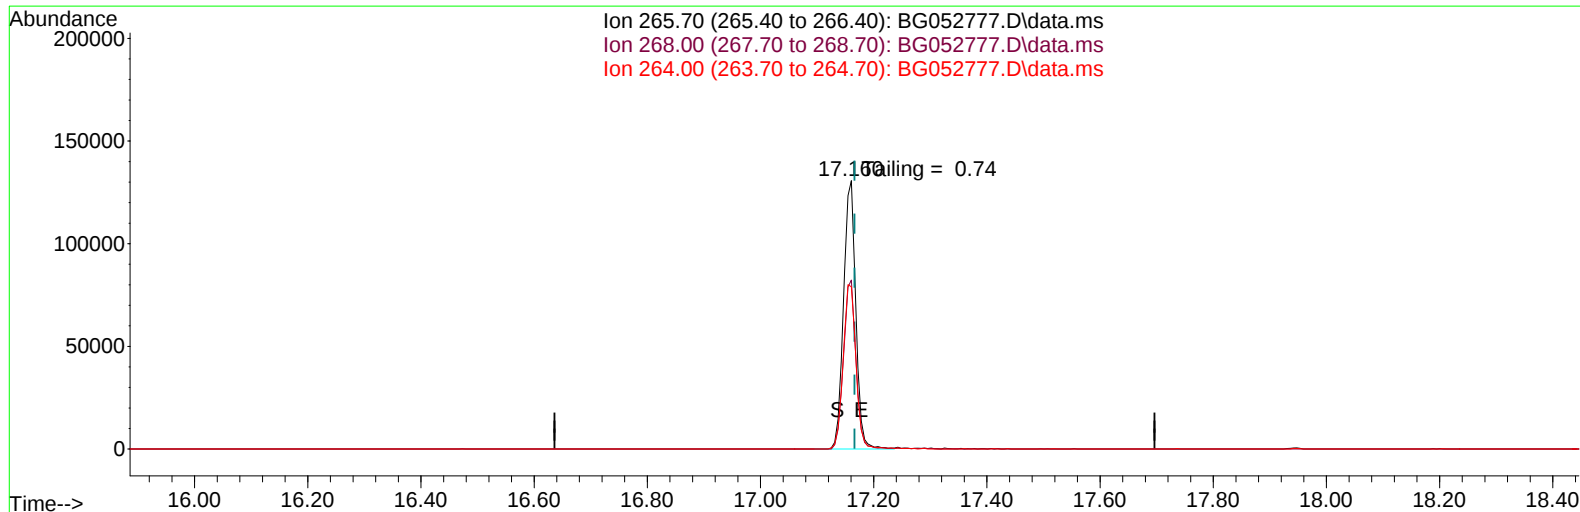

TIC: BG052777.D\data.ms

(70) Pentachlorophenol (C)

17.160min (-0.006) 29586.41 ng




response 195998

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	62.95
264.00	56.60	60.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032222\
Data File : BG052777.D
Acq On : 22 Mar 2022 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 22 18:41:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 15:56:10 2022
Response via : Initial Calibration

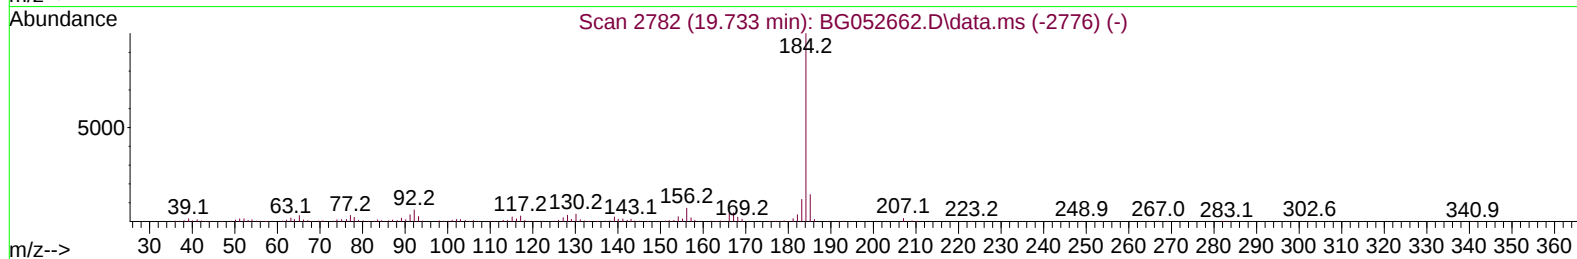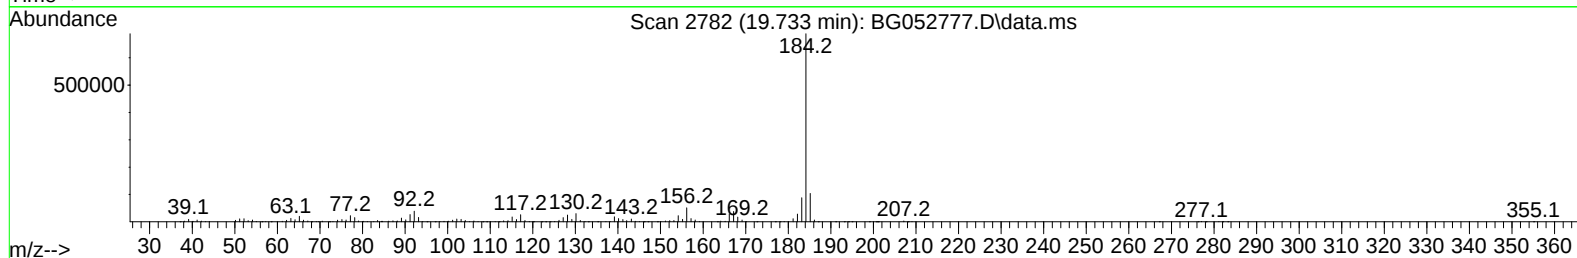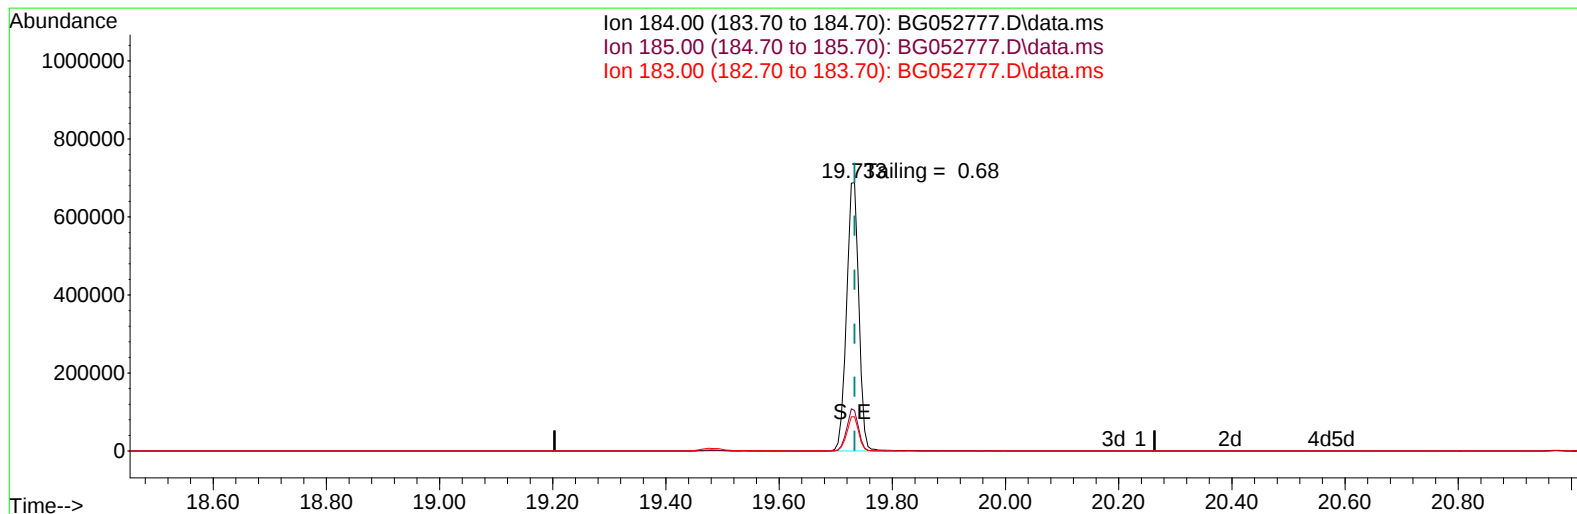

TIC: BG052777.D\data.ms

(77) Benzidine

19.733min (+ 0.000) 734572.27 ng m

response 1042035

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.11
183.00	11.80	12.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2022	BNA_G	BG052777.D
Compound Name	Response	Retention Time
DDT	490190	20.97
DDD	10245	20.52
DDE	477	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10722	500912	2.14

Instrument :
BNA_G
ClientSampleId :
DFTPP