

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032317\
 Data File : BG026397.D
 Acq On : 23 Mar 2017 11:19
 Operator : SJ/MA
 Sample : I2355-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 032117-PRRT-E-D-M

Quant Time: Mar 24 00:59:01 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 20 17:43:27 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	129408	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	528095	20.00	ng	0.00
38) Acenaphthene-d10	14.65	164	311792	20.00	ng	-0.01
63) Phenanthrene-d10	17.38	188	768115	20.00	ng	-0.01
75) Chrysene-d12	21.63	240	948449	20.00	ng	-0.01
86) Perylene-d12	24.80	264	903443	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	104217	14.29	ng	0.00
7) Phenol-d6	7.20	99	79435	8.12	ng	0.00
23) Nitrobenzene-d5	9.20	82	250377	28.51	ng	0.00
41) 2,4,6-Tribromophenol	16.13	330	119843	33.56	ng	-0.01
44) 2-Fluorobiphenyl	13.28	172	791471	35.60	ng	0.00
78) Terphenyl-d14	19.98	244	1138854	29.16	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032317\
Data File : BG026397.D
Acq On : 23 Mar 2017 11:19
Operator : SJ/MA
Sample : I2355-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
032117-PRRT-E-D-M

Quant Time: Mar 24 00:59:01 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

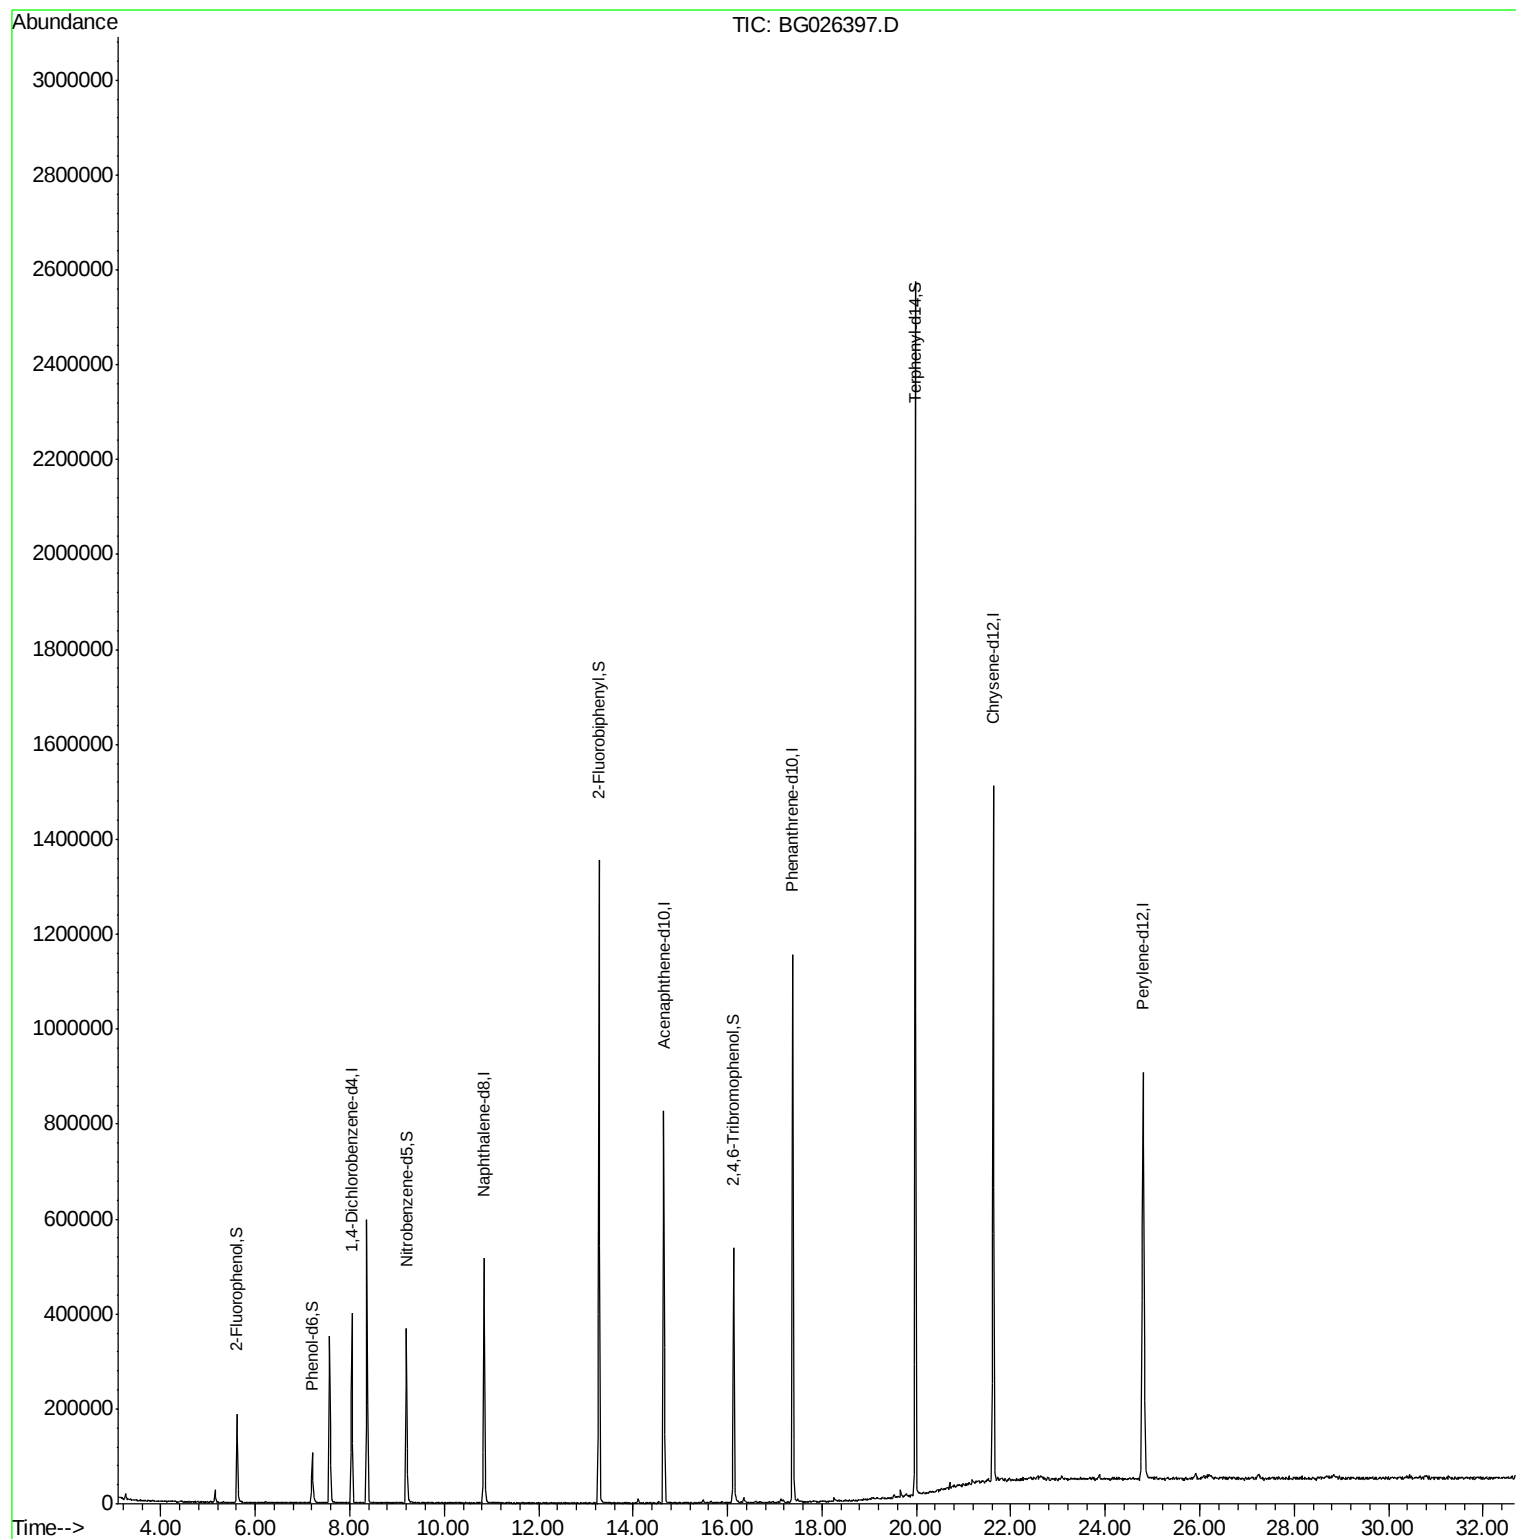

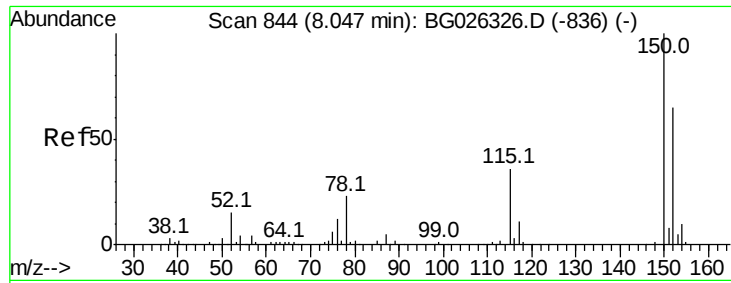


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.01 min
Lab File: BG026397.D
Acq: 23 Mar 2017 11:19

Instrument :
BNA_G
ClientSampleId :
032117-PRRT-E-D-M

Tot Ion:152 Resp: 129408
Ion Ratio Lower Upper
152 100
150 153.7 114.0 171.0
115 58.7 48.1 72.1

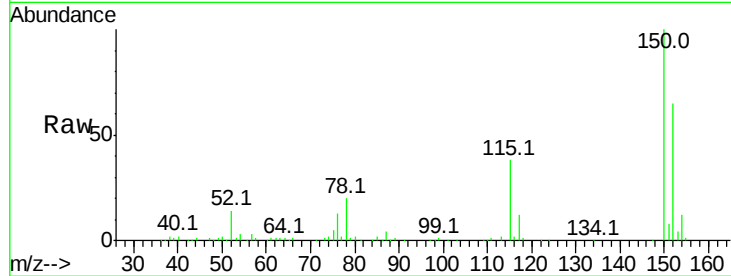


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

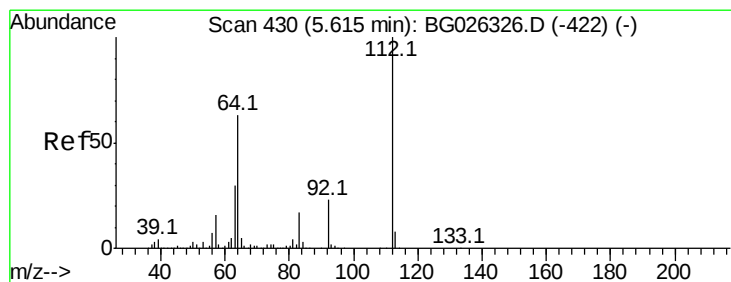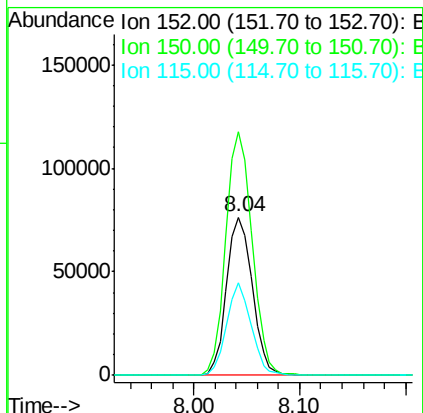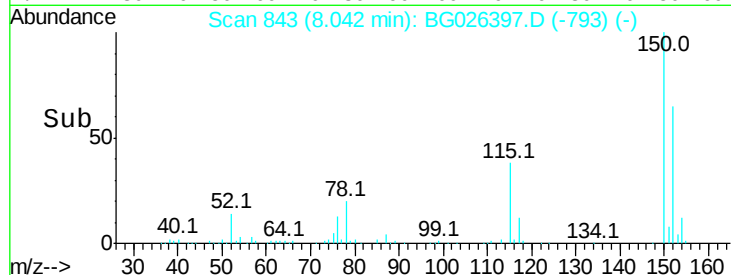



#5

2-Fluorophenol
Concen: 14.29 ng
RT: 5.62 min Scan# 430
Delta R.T. 0.00 min
Lab File: BG026397.D
Acq: 23 Mar 2017 11:19

Tgt Ion:112 Resp: 104217
Ion Ratio Lower Upper
112 100
64 54.8 61.8 92.6#
63 25.9 37.2 55.8#

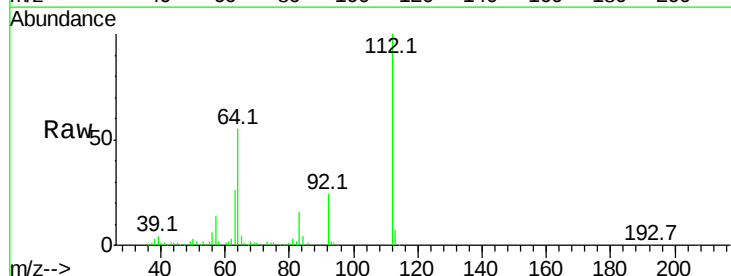

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

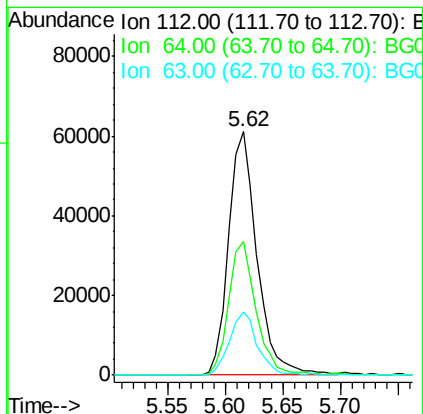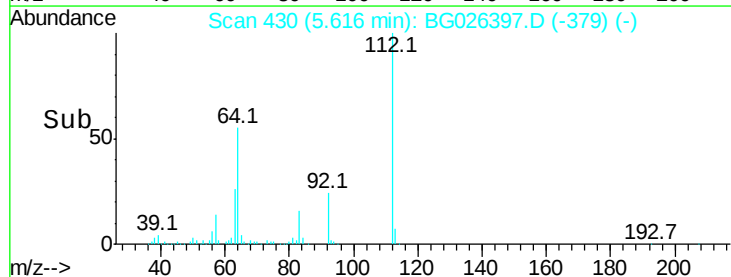



#7

Phenol-d6

Concen: 8.12 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.01 min

Lab File: BG026397.D

Acq: 23 Mar 2017 11:19

Instrument :

BNA_G

ClientSampleId :

032117-PRRT-E-D-M





Tot Ion: 99 Resp: 79435

Ion Ratio Lower Upper

99 100

42 10.3 20.5 30.7#

71 25.6 37.6 56.4#

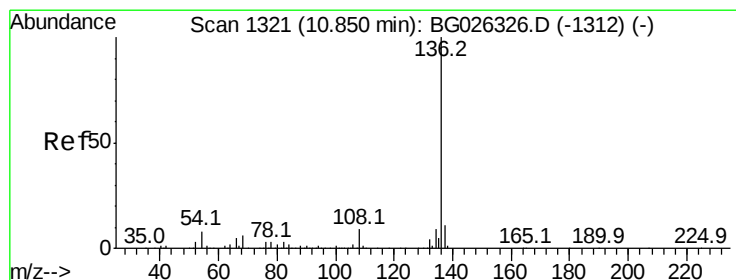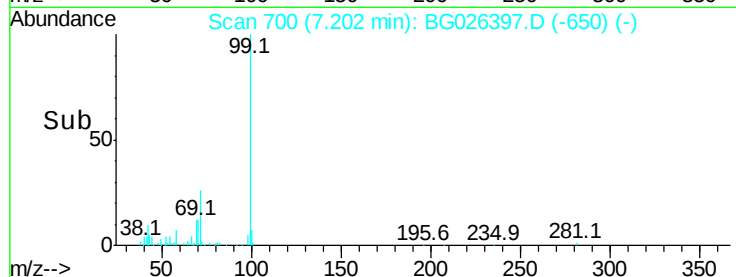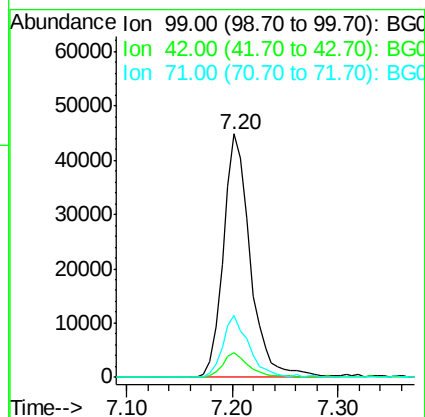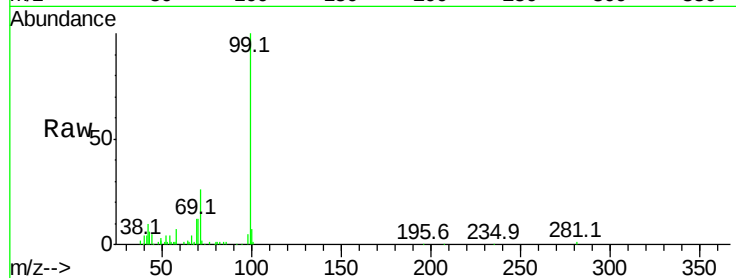

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.84 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BG026397.D

Acq: 23 Mar 2017 11:19

Tgt Ion: 136 Resp: 528095




Ion Ratio Lower Upper


136 100

137 11.0 8.9 13.3

54 5.7 9.3 13.9#

68 5.5 5.1 7.7

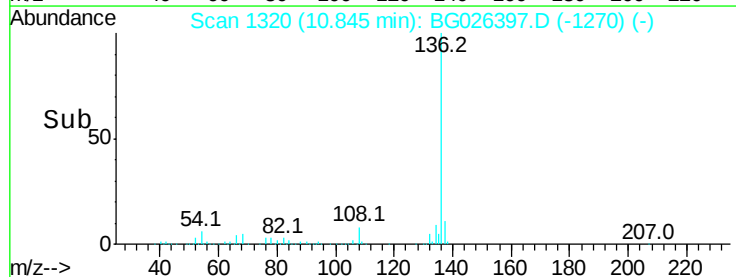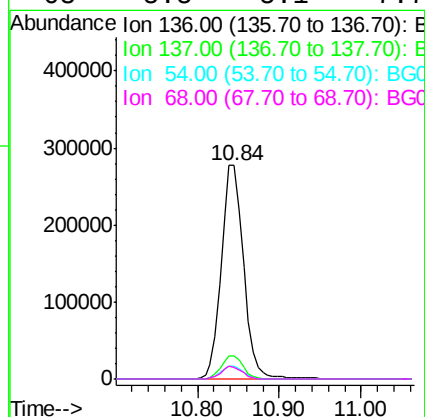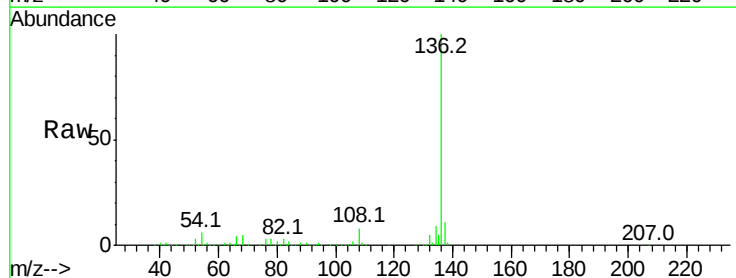

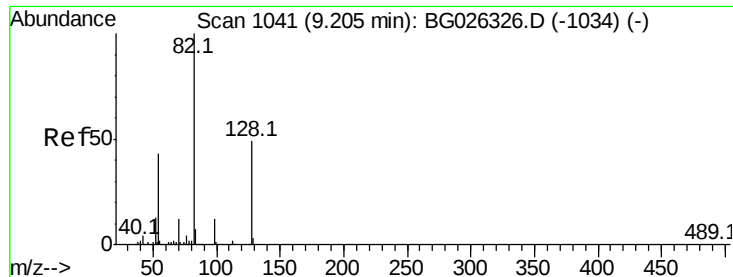

#23

Nitrobenzene-d5

Concen: 28.51 ng

RT: 9.20 min Scan# 1040

Delta R.T. -0.01 min

Lab File: BG026397.D

Acq: 23 Mar 2017 11:19

Instrument :

BNA_G

ClientSampleId :

032117-PRRT-E-D-M


Tot Ion: 82 Resp: 250377

Ion Ratio Lower Upper




82 100

128 52.1 26.4 39.6#

54 41.0 49.4 74.2#

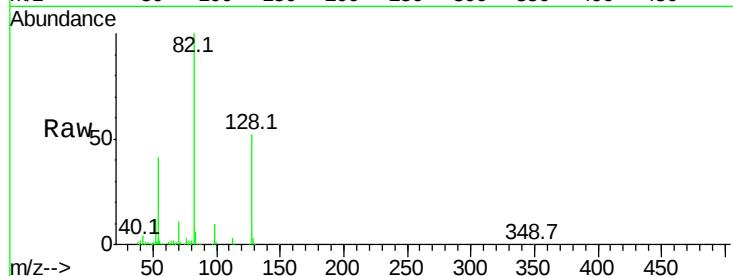

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

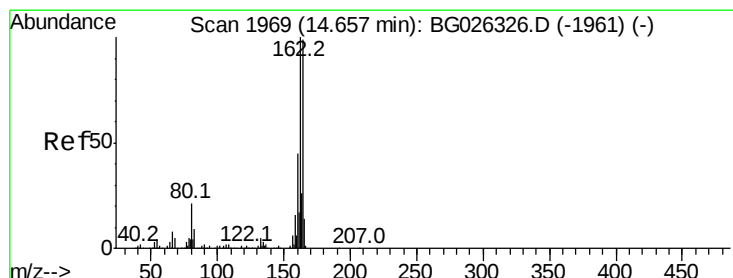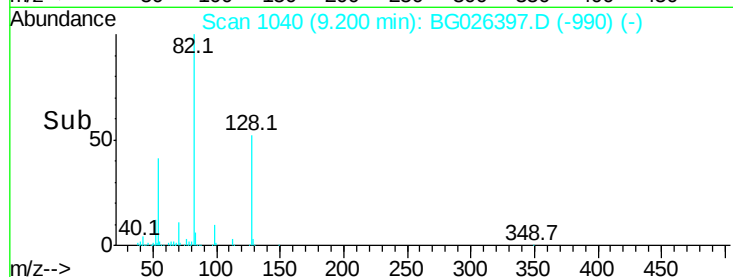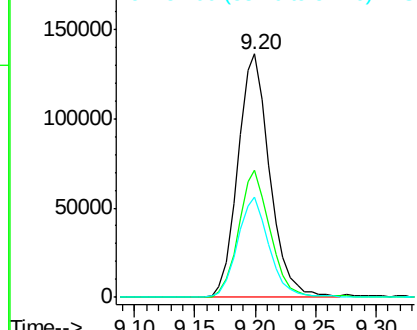

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.65 min Scan# 1967

Delta R.T. -0.01 min

Lab File: BG026397.D

Acq: 23 Mar 2017 11:19


Tgt Ion: 164 Resp: 311792

Ion Ratio Lower Upper



164 100


162 98.4 85.1 127.7

160 43.7 34.7 52.1

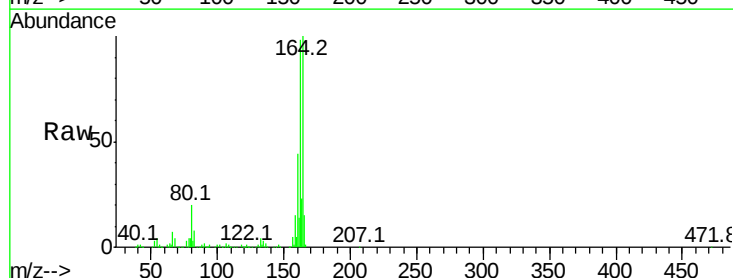

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

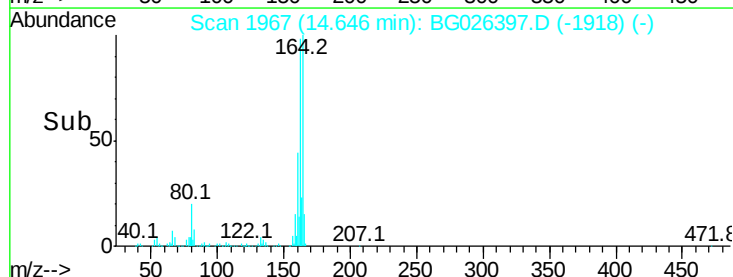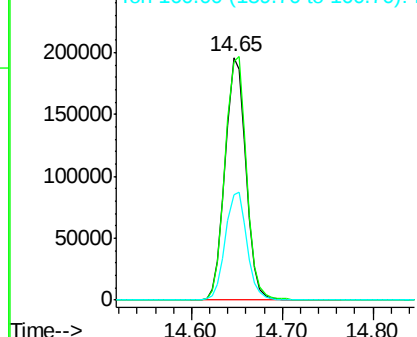


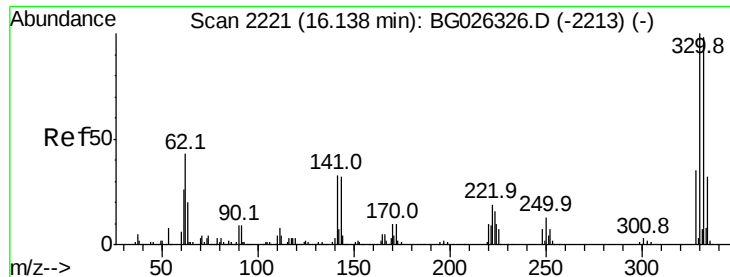




#41
 2,4,6-Tribromophenol
 Concen: 33.56 ng
 RT: 16.13 min Scan# 2219
 Delta R.T. -0.01 min
 Lab File: BG026397.D
 Acq: 23 Mar 2017 11:19

Instrument :
 BNA_G
 ClientSampleId :
 032117-PRRT-E-D-M

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.5	77.3	115.9
141	31.3	32.1	48.1#

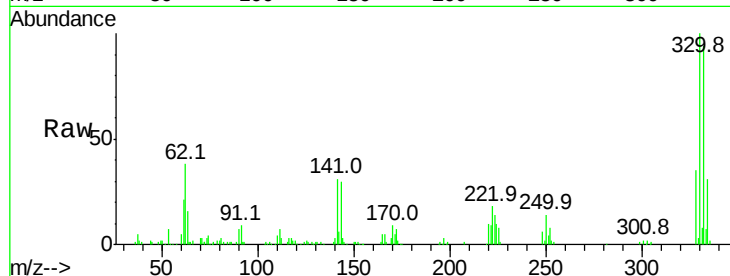


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

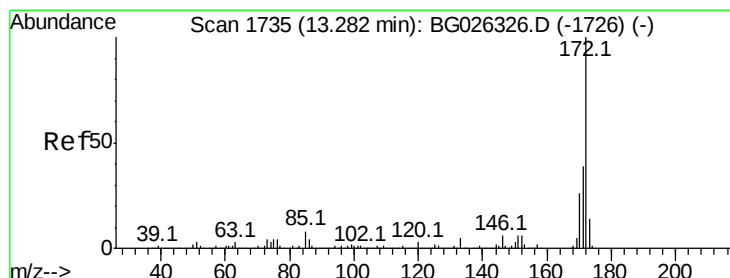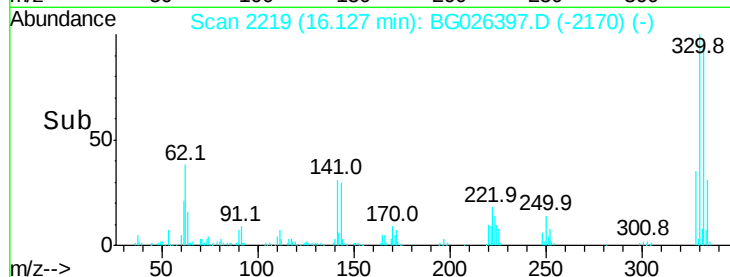
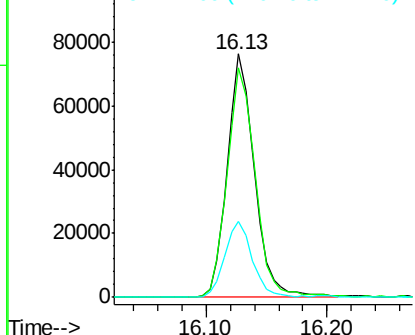



#44
 2-Fluorobiphenyl
 Concen: 35.60 ng
 RT: 13.28 min Scan# 1734
 Delta R.T. -0.01 min
 Lab File: BG026397.D
 Acq: 23 Mar 2017 11:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	32.2	48.2
170	24.2	21.8	32.6

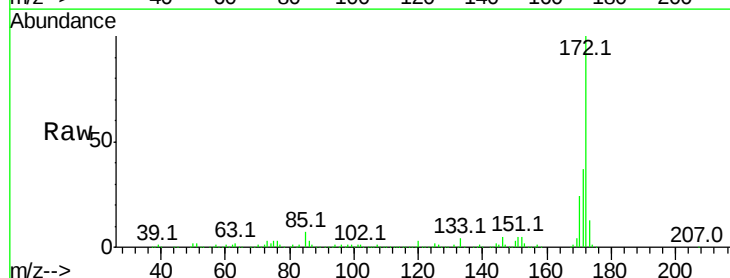

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

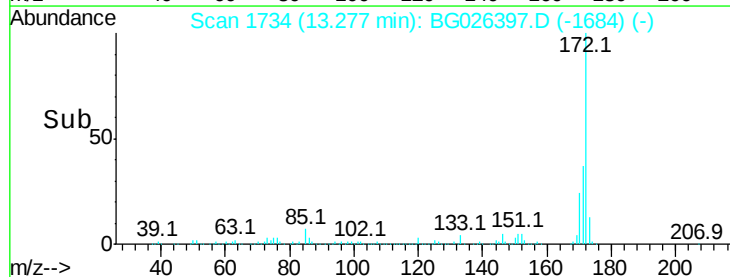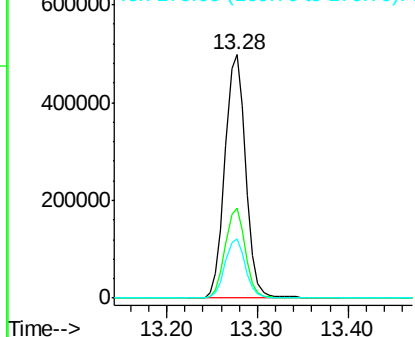


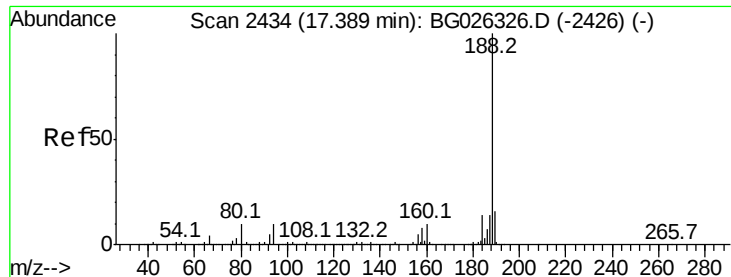




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.38 min Scan# 2432
Delta R.T. -0.01 min
Lab File: BG026397.D
Acq: 23 Mar 2017 11:19

Instrument :
BNA_G
ClientSampleId :
032117-PRRT-E-D-M

Tot Ion:188 Resp: 768115
Ion Ratio Lower Upper
188 100
94 8.7 5.8 8.8
80 9.4 7.5 11.3

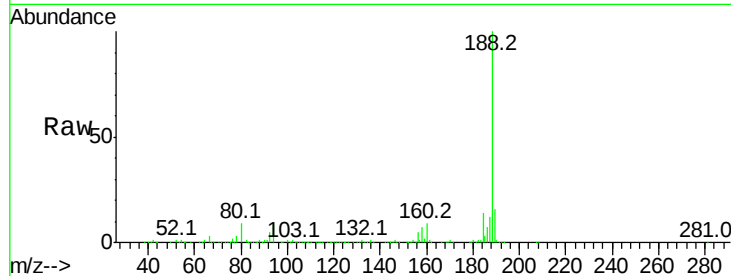


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

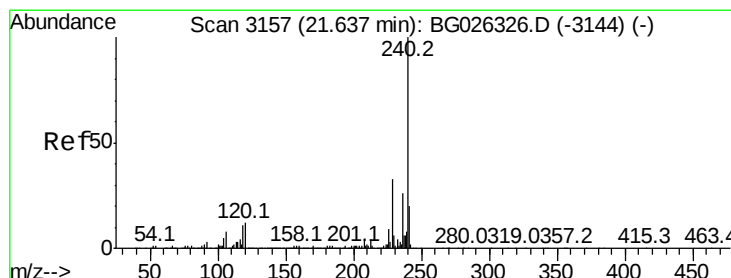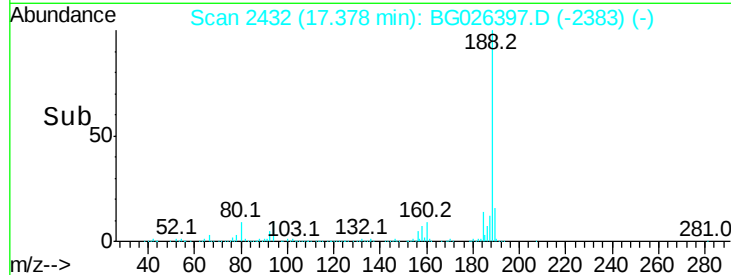
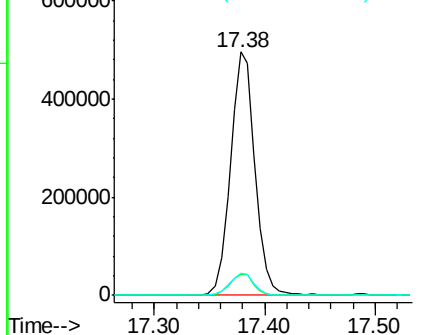



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.63 min Scan# 3155
Delta R.T. -0.01 min
Lab File: BG026397.D
Acq: 23 Mar 2017 11:19

Tgt Ion:240 Resp: 948449
Ion Ratio Lower Upper
240 100
120 11.5 5.7 8.5#
236 26.0 22.2 33.4

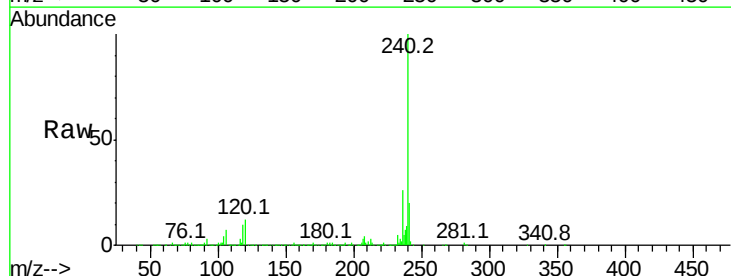

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

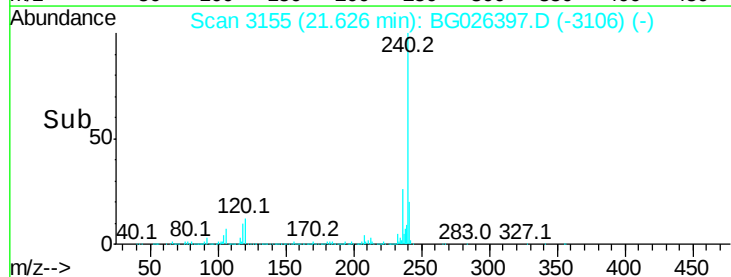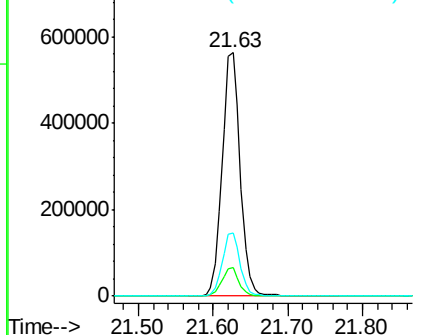

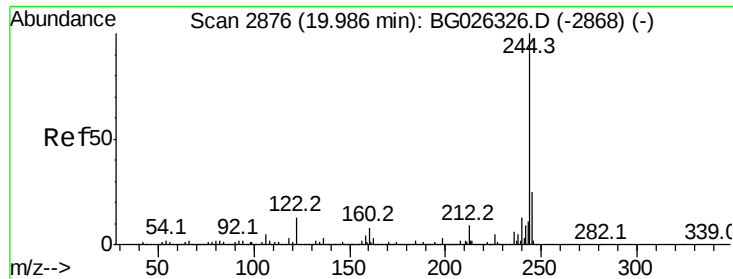

#78

Terphenyl-d14

Concen: 29.16 ng

RT: 19.98 min Scan# 2874

Delta R.T. -0.01 min

Lab File: BG026397.D

Acq: 23 Mar 2017 11:19

Instrument :

BNA_G

ClientSampleId :

032117-PRRT-E-D-M


Tot Ion:244 Resp: 1138854

Ion Ratio Lower Upper

244 100

212 7.0 10.0 15.0#




122 11.4 8.6 12.8

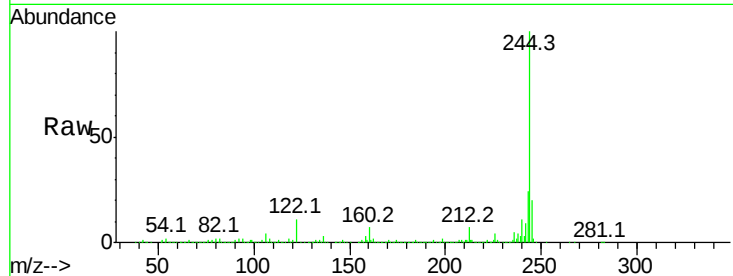

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

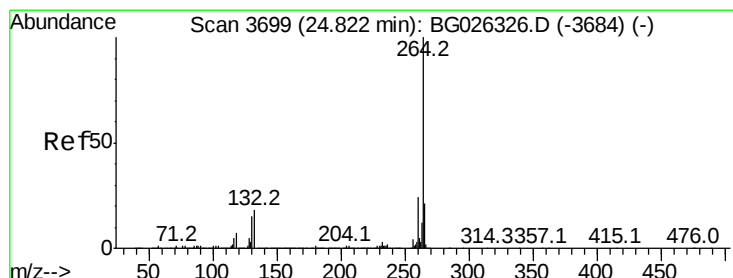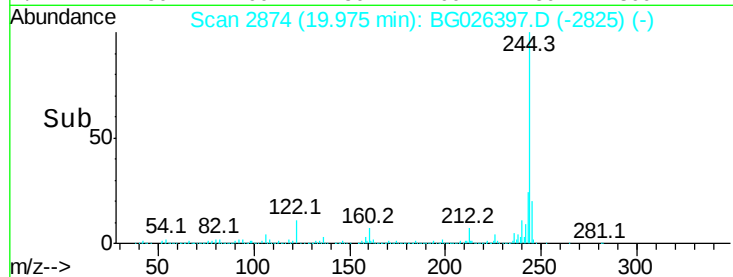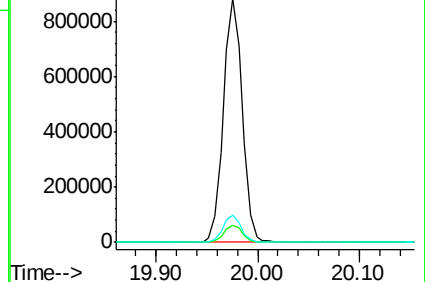

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.80 min Scan# 3695

Delta R.T. -0.02 min

Lab File: BG026397.D

Acq: 23 Mar 2017 11:19


Tgt Ion:264 Resp: 903443

Ion Ratio Lower Upper

264 100

260 23.7 21.8 32.8

265 21.8 18.2 27.4

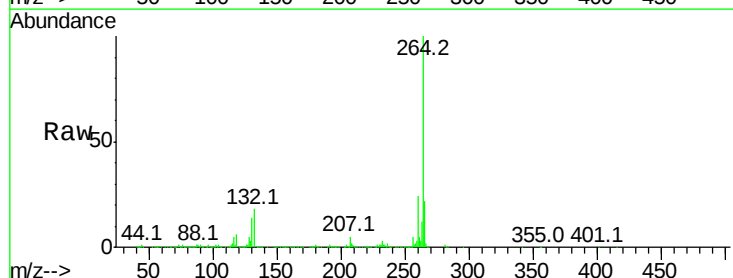

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

