
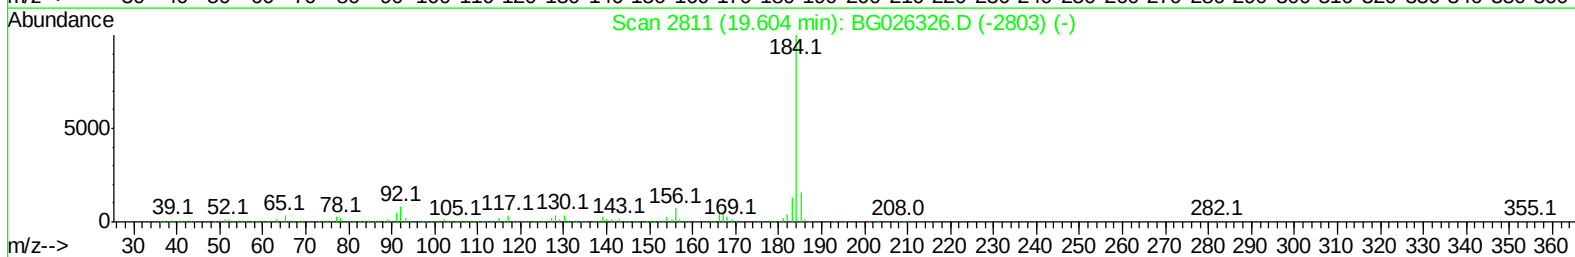
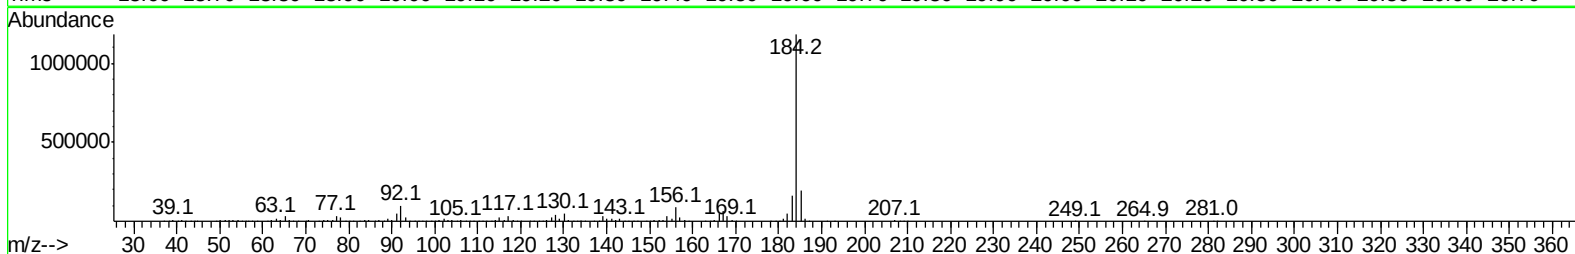


Data Path : Z:\HPCHEM1\BNA G\Data\BG032317\
Data File : BG026394.D
Acq On : 23 Mar 2017 9:21
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 08:37:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

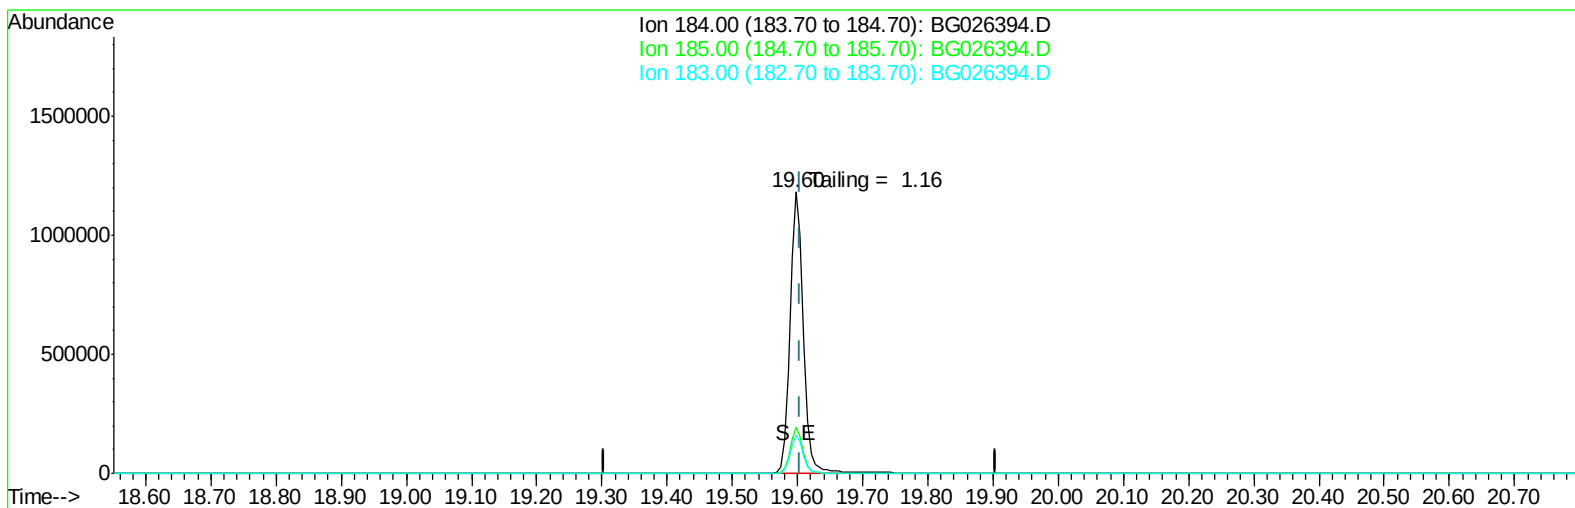

TIC: BG026394.D

(76) Benzidine




19.597min (-0.007) 8035.09ng

response 1672195

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.24
183.00	13.80	13.60
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG032317\
Data File : BG026394.D
Acq On : 23 Mar 2017 9:21
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 24 08:37:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

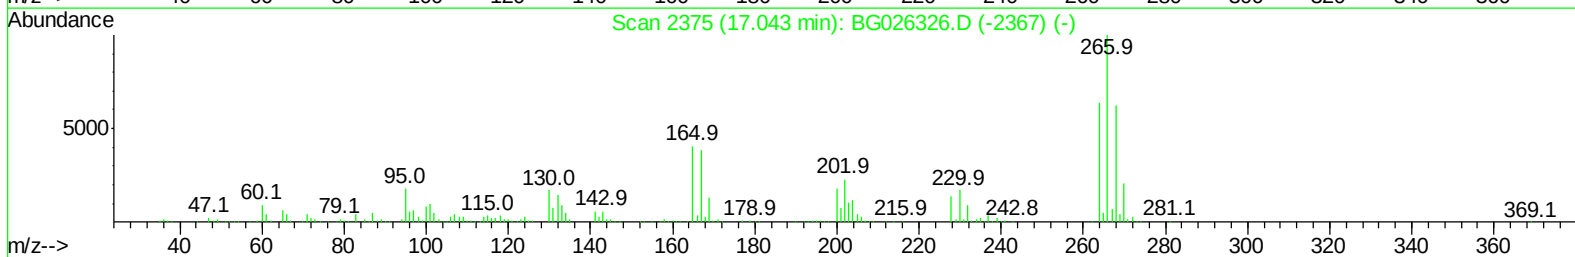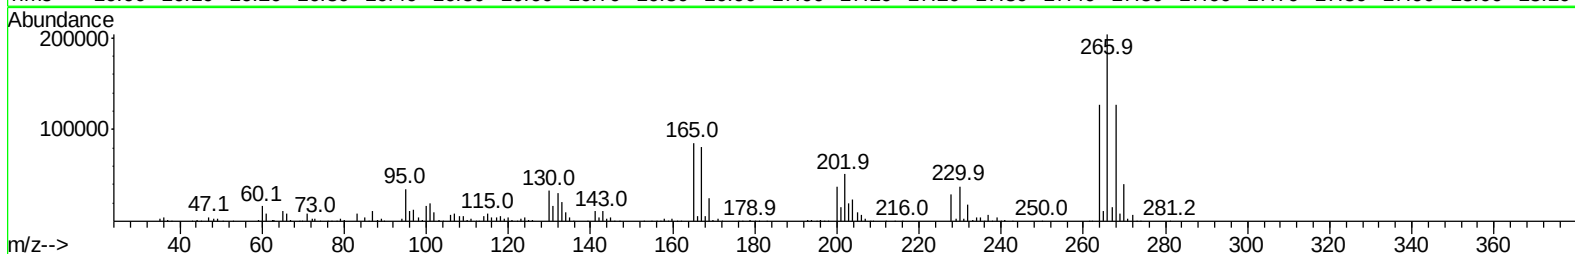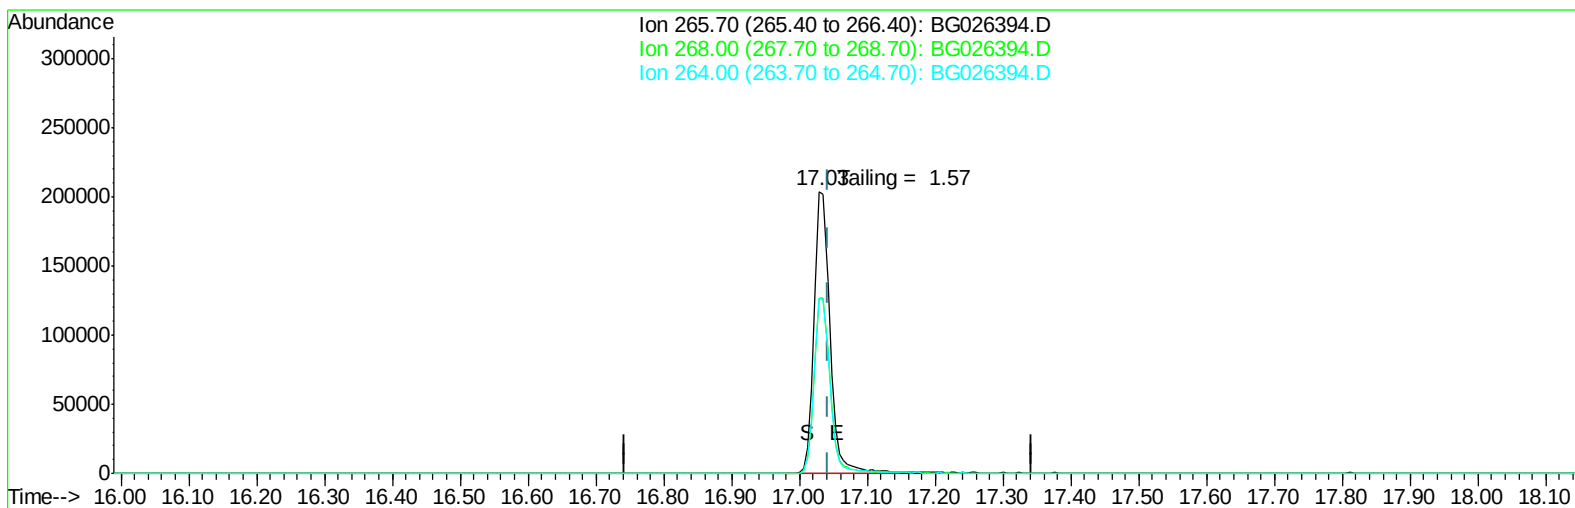

TIC: BG026394.D

(69) Pentachlorophenol (C)

17.029min (-0.013) 0.00ng

response 328572

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.14
264.00	62.60	62.20
0.00	0.00	0.00