


Data Path : Z:\HPCHEM1\BNA G\Data\BG032317\
 Data File : BG026394.D
 Acq On : 23 Mar 2017 9:21
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 20 17:43:27 2017

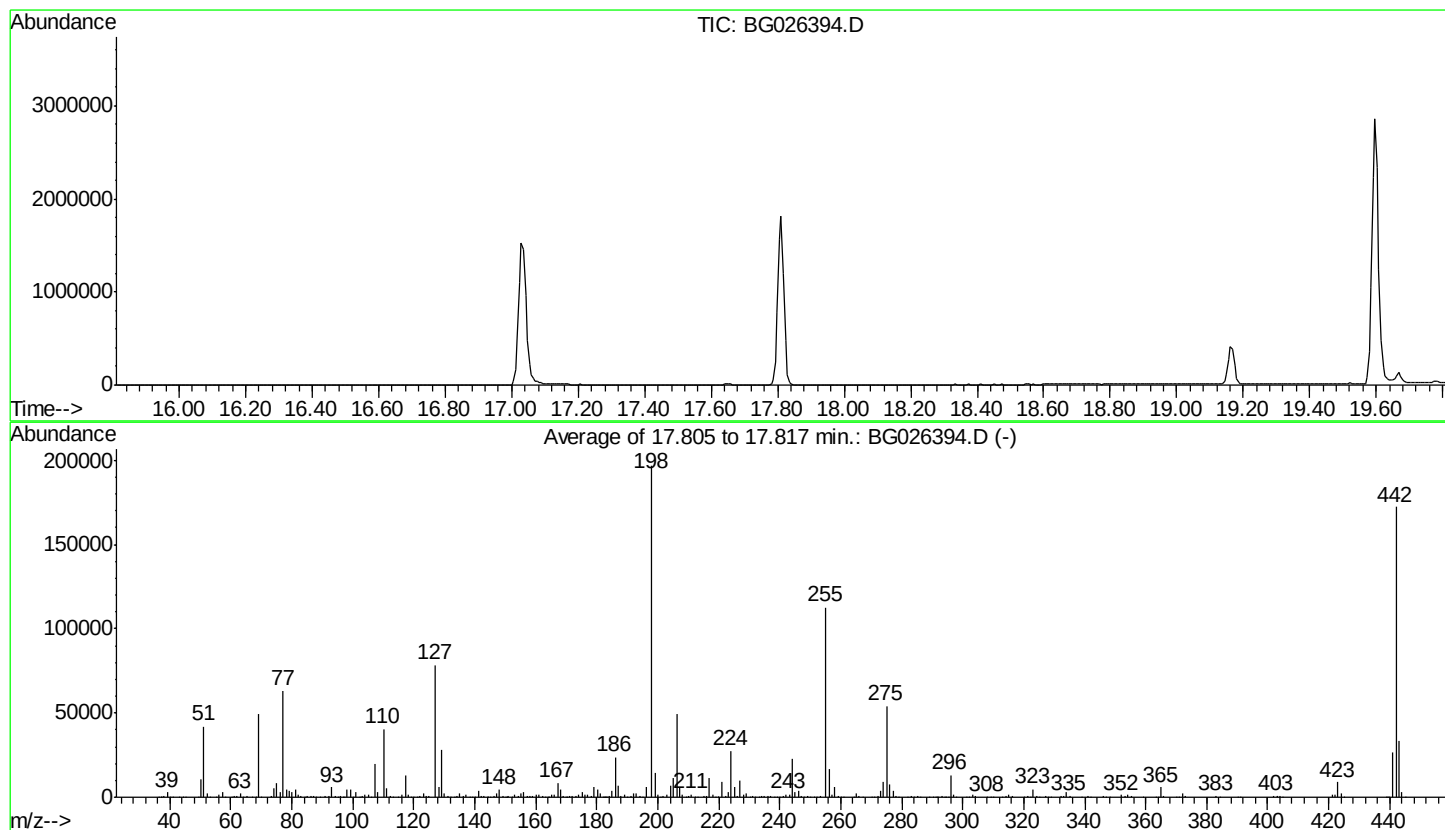

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.3	41853	PASS
68	69	0.00	2	0.5	223	PASS
69	198	0.00	100	25.0	49104	PASS
70	69	0.00	2	0.8	372	PASS
127	198	10	80	39.8	78376	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	196757	PASS
199	198	5	9	7.3	14341	PASS
275	198	10	60	27.4	54008	PASS
365	198	1	100	3.0	5941	PASS
441	442	0.01	24	15.6	26861	PASS
442	198	50	100	87.6	172266	PASS
443	442	15	24	19.6	33800	PASS