

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032321\
 Data File : BG048478.D
 Acq On : 23 Mar 2021 20:32
 Operator : CG/JU
 Sample : M1555-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B2B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.177	306	313	321	rBV3	22843	39087	1.42%	0.228%
2	5.653	386	394	405	rBV	625612	1014238	36.84%	5.917%
3	7.251	657	666	676	rBV	688674	1160352	42.14%	6.769%
4	8.103	804	811	818	rBV2	153560	257365	9.35%	1.501%
5	9.266	1000	1009	1017	rBV	419770	747373	27.15%	4.360%
6	10.923	1284	1291	1301	rVB	209839	368060	13.37%	2.147%
7	13.367	1698	1707	1717	rVB	1061478	1636257	59.43%	9.545%
8	13.861	1784	1791	1797	rBV2	54774	122777	4.46%	0.716%
9	14.184	1841	1846	1851	rBV3	18339	28316	1.03%	0.165%
10	14.742	1931	1941	1949	rBV	334188	534531	19.41%	3.118%
11	16.229	2187	2194	2204	rBV	1088527	1619015	58.80%	9.445%
12	17.186	2352	2357	2362	rBV4	68925	100642	3.66%	0.587%
13	17.492	2402	2409	2414	rBV	469560	710192	25.79%	4.143%
14	17.533	2414	2416	2422	rVB2	87624	113139	4.11%	0.660%
15	18.373	2554	2559	2564	rBV2	158233	219271	7.96%	1.279%
16	18.902	2646	2649	2655	rVB3	28884	43951	1.60%	0.256%
17	19.302	2711	2717	2723	rBV6	23885	47907	1.74%	0.279%
18	19.543	2753	2758	2764	rVB	277179	379880	13.80%	2.216%
19	19.637	2771	2774	2780	rBV8	35319	54619	1.98%	0.319%
20	19.783	2796	2799	2805	rVB7	18199	30154	1.10%	0.176%
21	19.872	2809	2814	2815	rBV	45946	56949	2.07%	0.332%
22	19.907	2816	2820	2826	rVB	200287	287586	10.45%	1.678%
23	20.101	2846	2853	2859	rBV	2184426	2753245	100.00%	16.061%
24	20.394	2894	2903	2911	rVB5	43659	114901	4.17%	0.670%
25	20.541	2924	2928	2935	rBV2	46213	82731	3.00%	0.483%
26	20.865	2979	2983	2986	rBV6	29851	39013	1.42%	0.228%
27	21.346	3063	3065	3071	rVB5	25636	38626	1.40%	0.225%
28	21.417	3071	3077	3087	rBV5	132184	363419	13.20%	2.120%
29	21.781	3128	3139	3145	rBV2	468230	988417	35.90%	5.766%
30	21.834	3145	3148	3155	rVB	94475	141734	5.15%	0.827%
31	22.081	3188	3190	3193	rBV4	33273	43047	1.56%	0.251%
32	22.181	3202	3207	3216	rVB6	117689	241830	8.78%	1.411%
33	22.269	3216	3222	3223	rBV4	95749	163109	5.92%	0.951%
34	22.457	3250	3254	3264	rVB5	66239	139989	5.08%	0.817%
35	22.586	3269	3276	3289	rBV3	143105	486836	17.68%	2.840%
36	22.968	3333	3341	3349	rBV2	346933	995496	36.16%	5.807%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032321\
Data File : BG048478.D
Acq On : 23 Mar 2021 20:32
Operator : CG/JU
Sample : M1555-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B2B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	24.801	3647	3653	3663	rVB2	45468	141070	5.12%	0.823%
38	25.112	3698	3706	3726	rVB2	258964	837234	30.41%	4.884%




Sum of corrected areas: 17142358

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032321\
Data File : BG048478.D
Acq On : 23 Mar 2021 20:32
Operator : CG/JU
Sample : M1555-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B2B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

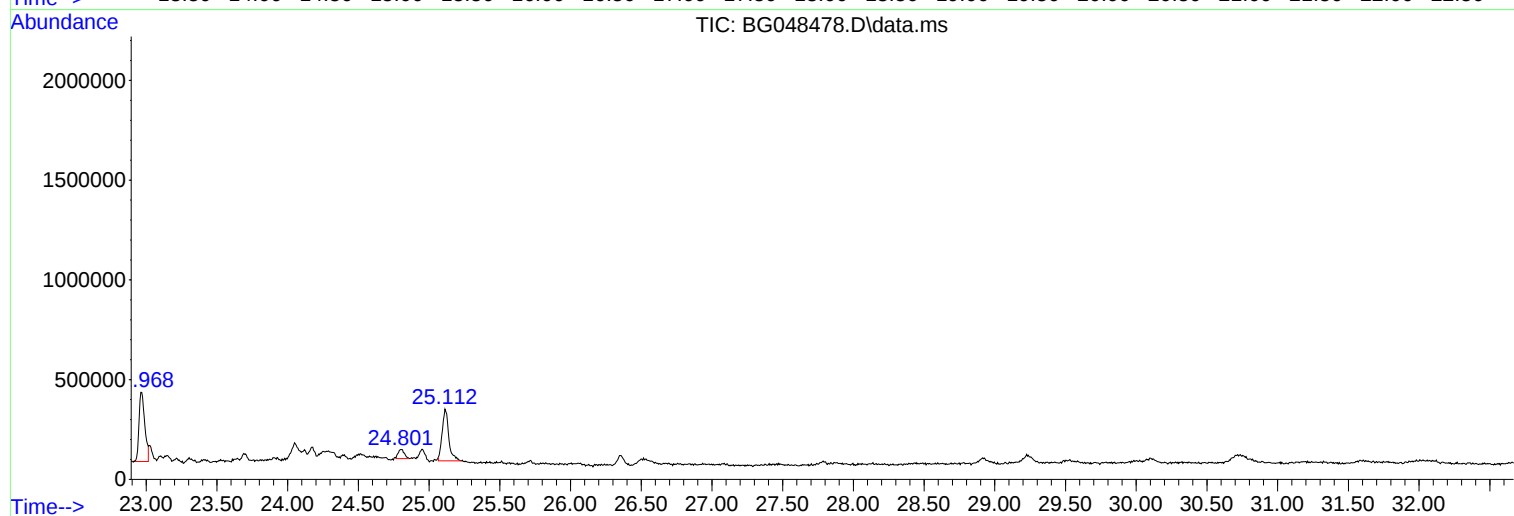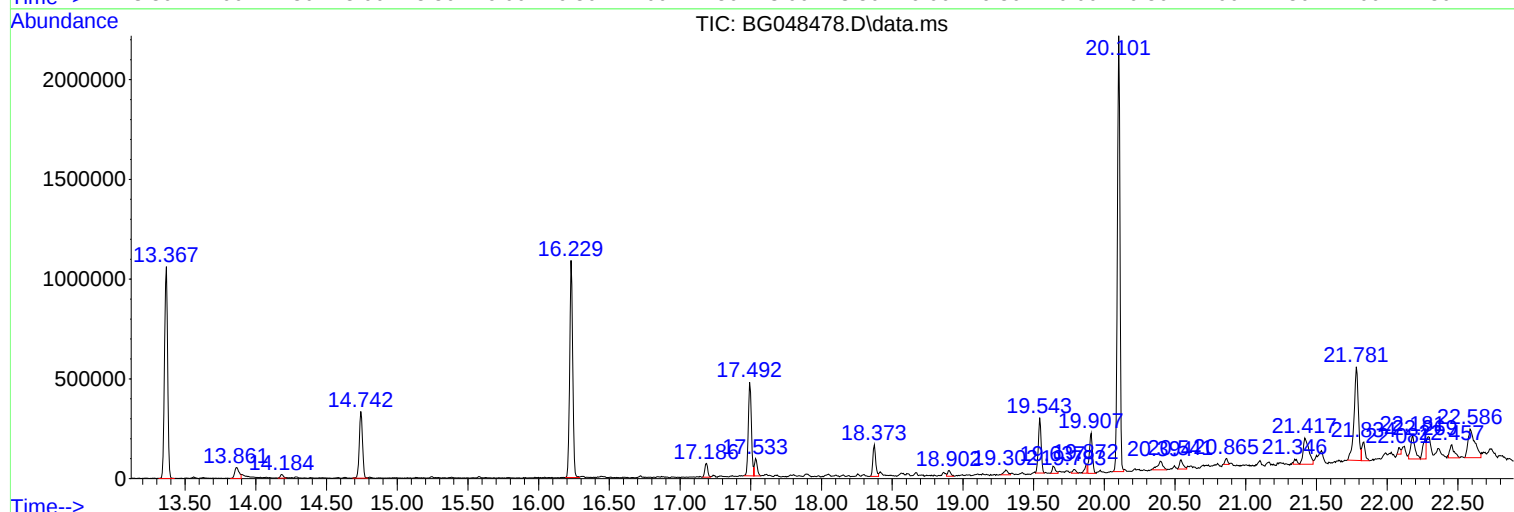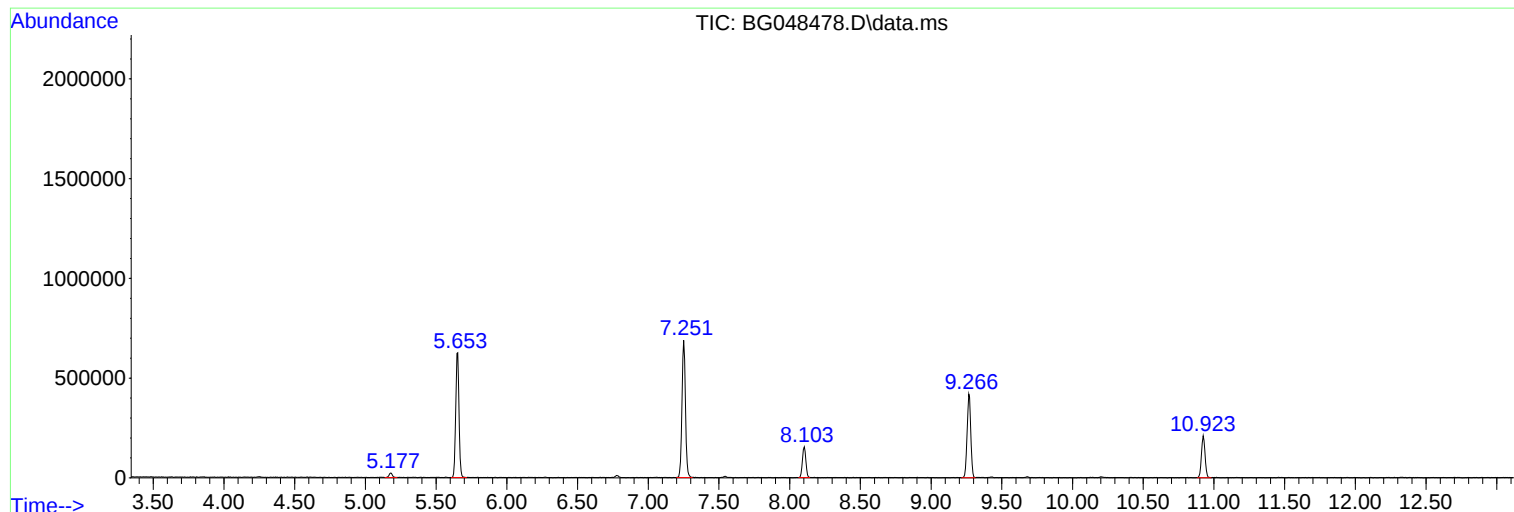

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032321\
Data File : BG048478.D
Acq On : 23 Mar 2021 20:32
Operator : CG/JU
Sample : M1555-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B2B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032321\
Data File : BG048478.D
Acq On : 23 Mar 2021 20:32
Operator : CG/JU
Sample : M1555-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B2B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------