
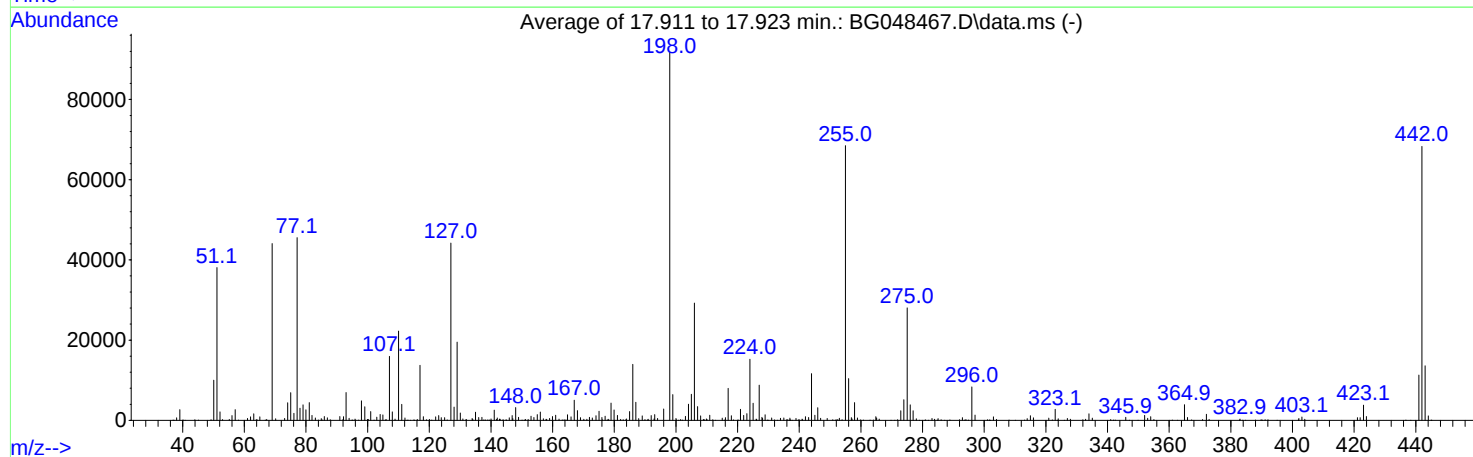


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032321\
 Data File : BG048467.D
 Acq On : 23 Mar 2021 12:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 24 12:36:47 2021

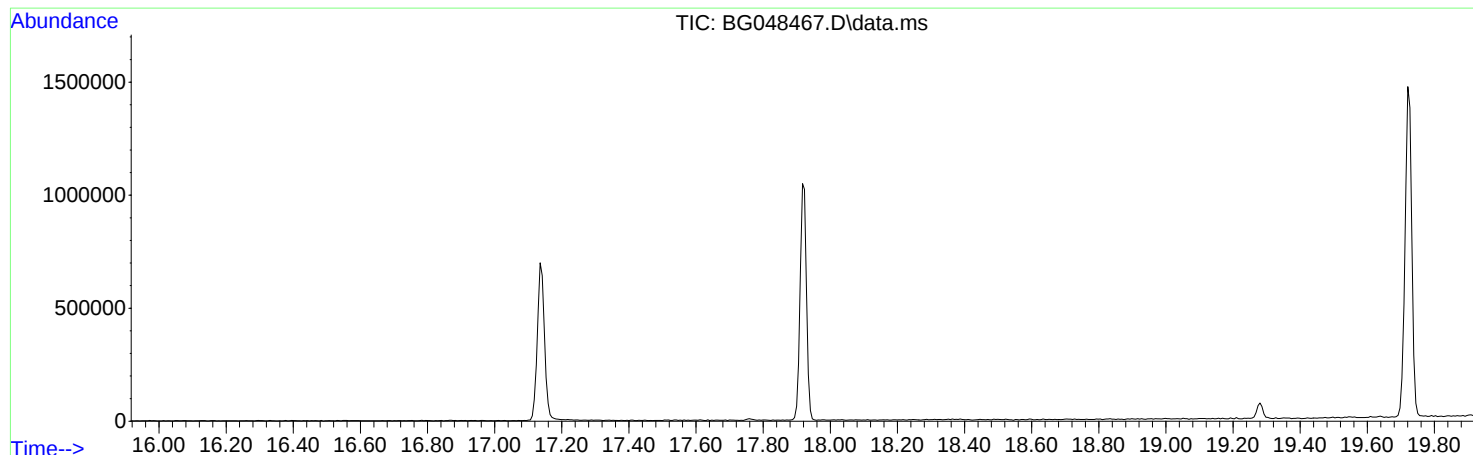




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	38091	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.1	44099	PASS
70	69	0.00	2	0.9	402	PASS
127	198	10	80	48.2	44192	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91704	PASS
199	198	5	9	7.0	6438	PASS
275	198	10	60	30.6	28061	PASS
365	198	1	100	4.3	3917	PASS
441	198	0.01	100	12.3	11292	PASS
442	198	50	100	74.5	68304	PASS
443	442	15	24	19.9	13609	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032321\
Data File : BG048467.D
Acq On : 23 Mar 2021 12:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 23 13:47:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 22 11:22:24 2021
Response via : Initial Calibration

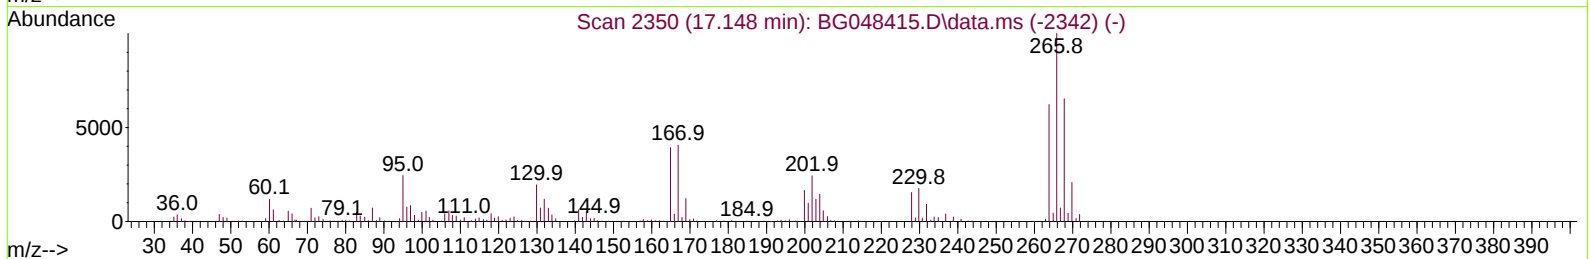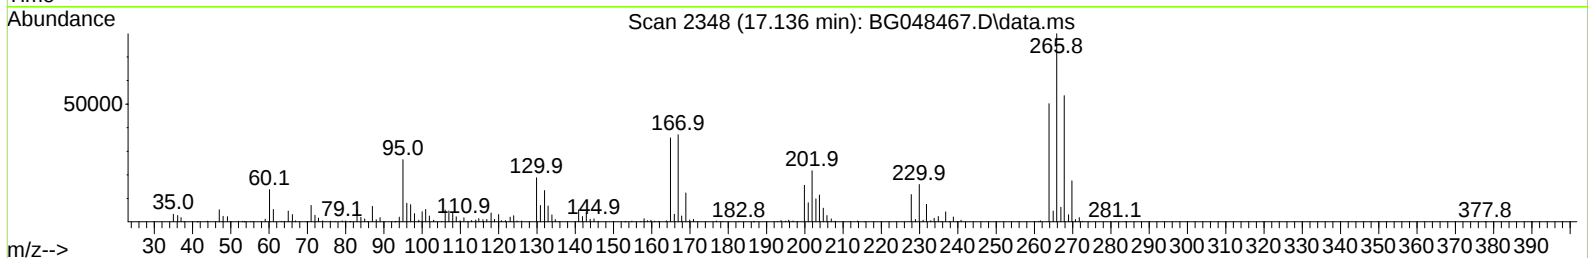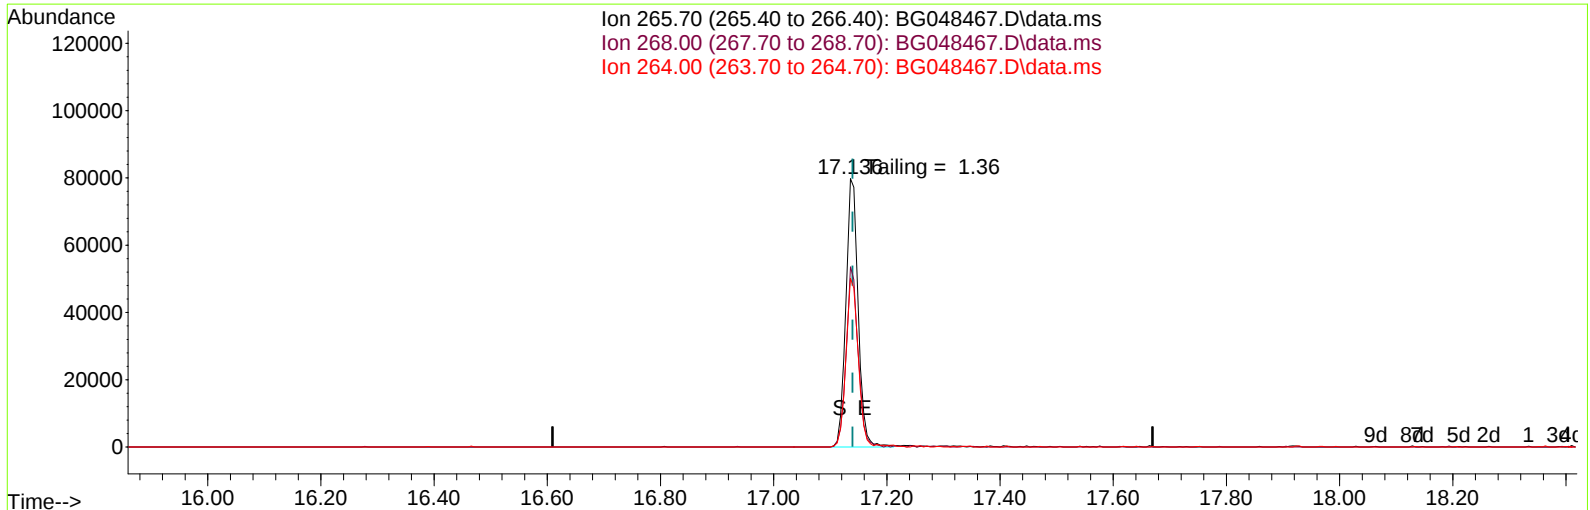

TIC: BG048467.D\data.ms

(70) Pentachlorophenol (C)

17.136min (-0.004) 201098.76 ng m




response 122680

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.11
264.00	61.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032321\
 Data File : BG048467.D
 Acq On : 23 Mar 2021 12:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 13:47:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 22 11:22:24 2021
 Response via : Initial Calibration

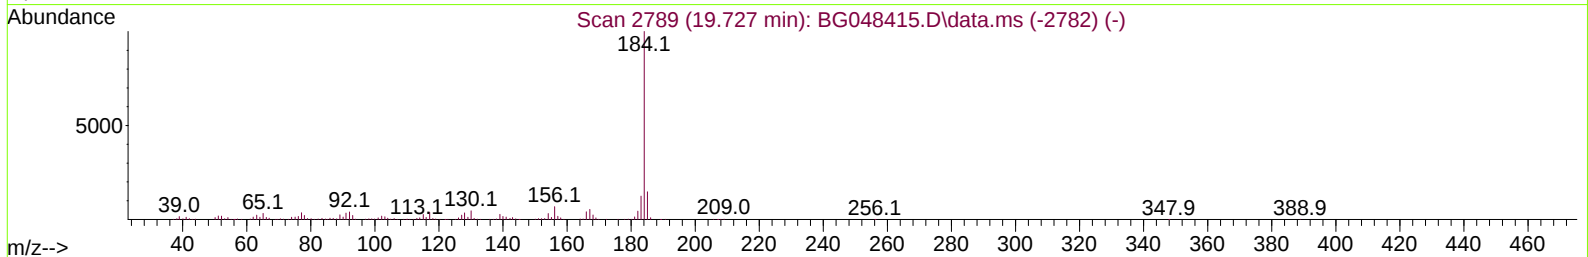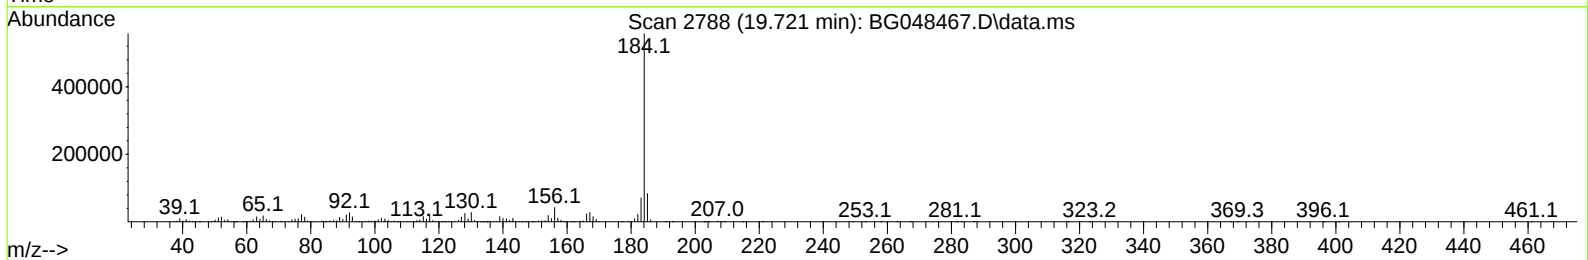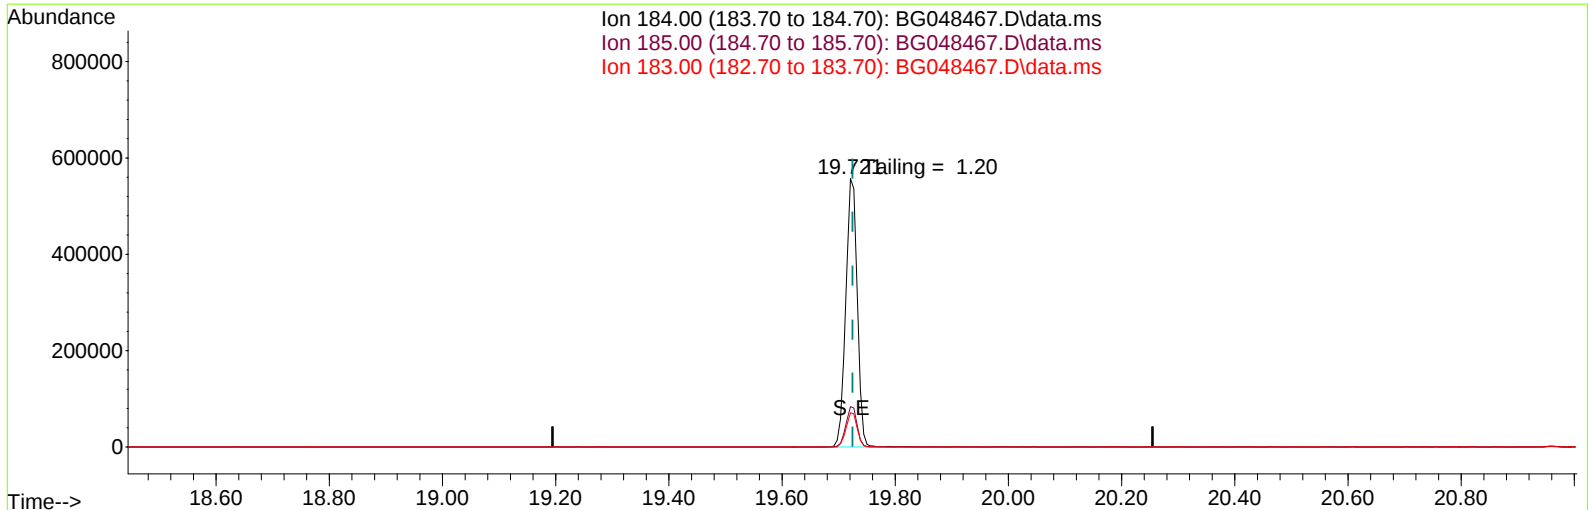

TIC: BG048467.D\data.ms

(77) Benzidine

19.721min (-0.004) 141769.99 ng m

response 789885

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.03
183.00	13.20	12.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/23/2021	BNA_G	BG048467.D
Compound Name	Response	Retention Time
DDT	390848	20.96
DDD	1181	20.51
DDE	770	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1951	392799	0.50