


Data Path : Z:\HPCHEM1\BNA_G\Data\BG032415\
 Data File : BG016094.D
 Acq On : 24 Mar 2015 9:30
 Operator : TP/IZ
 Sample : DFTPP13
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP13

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG031715.M
 Title : SVOA CALIBRATION
 Last Update : Wed Mar 25 02:11:09 2015

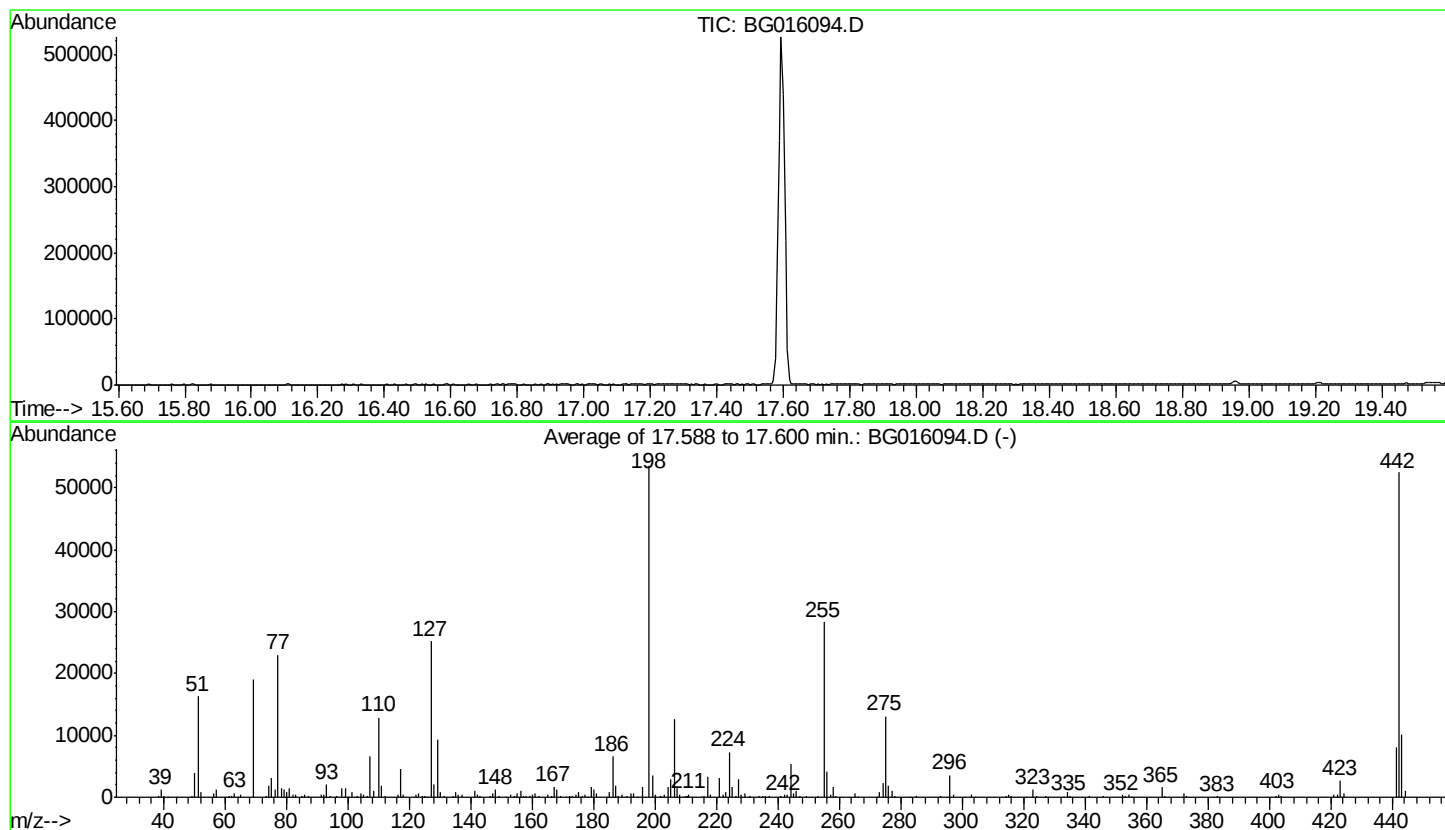

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	16329	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	19090	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	25168	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53565	PASS
199	198	5	9	6.5	3474	PASS
275	198	10	60	24.4	13064	PASS
365	198	1	100	3.0	1621	PASS
441	443	0.01	100	79.4	8011	PASS
442	198	50	100	98.2	52594	PASS
443	442	15	24	19.2	10090	PASS