


Data Path : Z:\HPCHEM1\BNA_G\Data\BG032415\
 Data File : BG016094.D
 Acq On : 24 Mar 2015 9:30
 Operator : TP/IZ
 Sample : DFTPP13
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP13

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG031715.M
 Title : SVOA CALIBRATION
 Last Update : Sat Mar 21 04:57:09 2015

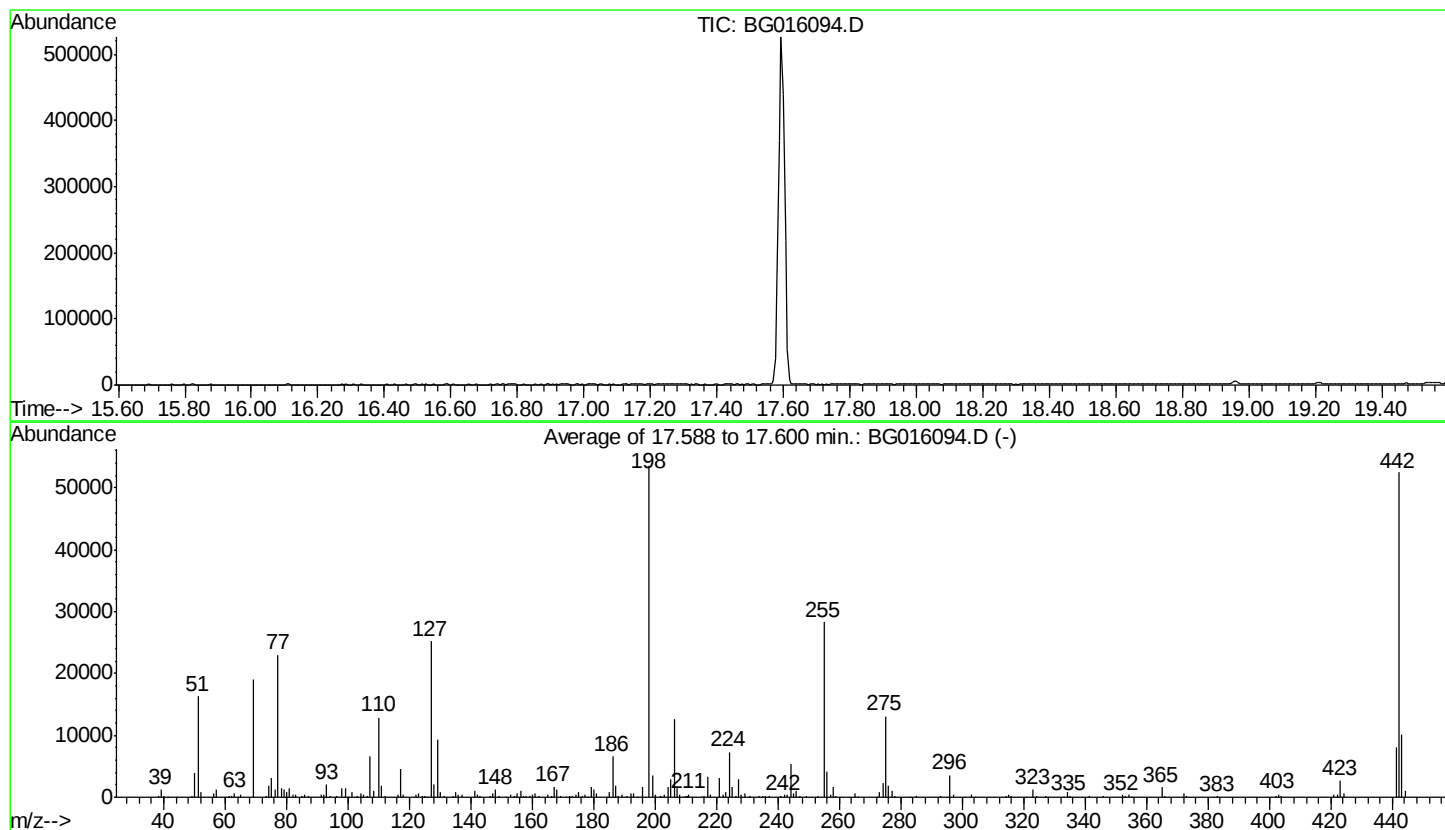

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	16329	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	19090	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	25168	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53565	PASS
199	198	5	9	6.5	3474	PASS
275	198	10	60	24.4	13064	PASS
365	198	1	100	3.0	1621	PASS
441	443	0.01	100	79.4	8011	PASS
442	198	50	100	98.2	52594	PASS
443	442	15	24	19.2	10090	PASS

m/z	Abundance
38.15	249.0
39.15	1103.0
40.15	785.0
44.15	205.0
49.15	191.0
50.15	4042.0
51.15	15951.0
52.15	766.0
56.15	529.0
57.15	1175.0
61.05	211.0
62.15	166.0
63.15	613.0
65.15	407.0
69.15	17592.0
73.35	213.0
74.15	1616.0
75.15	2710.0
76.15	1173.0
77.15	21360.0
78.15	1526.0
79.05	1204.0
80.05	919.0
81.05	1402.0
82.15	431.0
83.05	385.0
85.05	193.0
86.05	352.0
87.15	198.0
91.15	370.0
92.15	325.0
93.05	2251.0
96.15	183.0
98.05	1291.0
99.05	1219.0
101.15	771.0
103.05	262.0
104.15	528.0
105.05	535.0
107.15	5789.0
108.15	903.0
110.05	11765.0
111.05	1787.0
112.05	292.0
116.15	429.0
117.15	4350.0
118.05	424.0
122.05	414.0
123.05	524.0
124.05	236.0
125.15	295.0
127.15	22816.0
128.15	1921.0
129.05	8824.0
130.05	745.0
131.15	180.0
135.15	737.0
136.05	305.0
137.15	262.0
141.05	1083.0
141.95	320.0
142.95	208.0
146.05	245.0
147.05	685.0
148.05	1006.0
149.05	220.0
151.15	177.0
152.95	424.0
154.15	220.0
155.05	558.0
156.05	1014.0
158.05	194.0
159.05	154.0
160.15	305.0
161.05	554.0
165.05	318.0
166.15	286.0
167.05	1990.0
168.05	1205.0
169.05	224.0
171.95	178.0
173.15	214.0
173.95	333.0
175.15	766.0
176.05	221.0
177.05	315.0
179.05	1580.0
180.05	1029.0
181.05	605.0
184.15	189.0
185.15	697.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

186.15	5553.0
187.05	1470.0
188.15	208.0
189.15	244.0
191.05	248.0
192.05	555.0
193.15	409.0
196.05	1524.0
198.05	44424.0
199.05	3005.0
200.05	324.0
201.55	289.0
203.05	408.0
204.05	1315.0
205.05	2284.0
206.15	10456.0
207.05	1605.0
208.05	356.0
211.05	471.0
216.15	161.0
217.05	2930.0
217.95	391.0
221.05	2477.0
223.05	672.0
224.05	5880.0
225.05	1295.0
226.05	164.0
227.05	2338.0
228.05	389.0
229.05	557.0
231.05	234.0
235.05	188.0
236.05	199.0
237.05	165.0
242.05	365.0
243.05	307.0
244.15	4328.0
245.05	588.0
246.05	741.0
247.05	205.0
249.05	187.0
252.95	181.0
255.05	22304.0
256.05	3513.0
257.15	230.0
258.05	1296.0
259.05	167.0
265.05	563.0
273.05	669.0
274.05	1670.0
275.05	10080.0
276.05	1592.0
277.05	805.0
285.05	213.0
293.15	189.0
296.05	2550.0
297.05	343.0
303.05	335.0
314.05	171.0
315.05	318.0
316.05	177.0
323.15	1073.0
324.15	258.0
327.05	180.0
334.05	583.0
335.05	165.0
345.95	197.0
352.05	364.0
353.05	243.0
354.05	225.0
365.05	1056.0
366.05	196.0
372.05	429.0
402.05	240.0
403.05	341.0
421.05	258.0
422.05	178.0
423.05	1901.0
424.05	433.0
441.15	5475.0
442.15	35480.0
443.15	7059.0
444.05	733.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

m/z	Abundance
39.15	1436.0
40.05	625.0
41.15	154.0
44.15	349.0
50.15	4617.0
51.15	19080.0
52.15	1023.0
56.05	562.0
57.15	1495.0
61.15	240.0
62.05	196.0
63.05	926.0
65.25	410.0
69.15	23376.0
73.25	255.0
74.15	2225.0
75.15	3807.0
76.15	1332.0
77.15	27416.0
78.15	1671.0
79.05	1402.0
80.15	1118.0
81.05	1970.0
82.05	469.0
83.15	558.0
85.15	407.0
86.05	455.0
87.15	242.0
91.15	469.0
92.05	350.0
93.15	2265.0
94.05	250.0
96.05	151.0
98.15	1652.0
99.15	1674.0
100.15	157.0
101.05	967.0
103.15	410.0
104.05	732.0
105.15	490.0
106.15	264.0
107.15	8026.0
108.15	1502.0
110.15	15145.0
111.05	2085.0
112.05	200.0
116.05	425.0
117.15	5107.0
118.05	419.0
122.05	363.0
123.05	851.0
124.05	356.0
124.95	338.0
127.15	29632.0
128.05	2463.0
129.05	11152.0
130.05	954.0
131.15	173.0
134.05	334.0
135.15	771.0
136.05	389.0
137.15	513.0
141.05	1368.0
142.05	488.0
143.05	440.0
146.05	260.0
147.05	587.0
148.05	1511.0
149.05	370.0
153.05	423.0
154.15	323.0
155.15	776.0
156.15	1246.0
157.15	346.0
158.05	250.0
159.15	274.0
160.05	285.0
161.05	609.0
162.05	191.0
165.05	516.0
166.05	503.0
167.15	2592.0
168.05	1405.0
169.15	196.0
171.05	183.0
172.05	167.0
173.05	256.0
174.05	630.0
175.05	1131.0
176.05	347.0
177.05	438.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

178.05	255.0
179.05	2084.0
180.05	1391.0
181.05	734.0
185.05	956.0
186.15	7814.0
187.15	1943.0
188.15	302.0
188.95	446.0
191.05	235.0
192.15	775.0
193.05	620.0
194.05	176.0
196.05	1899.0
198.05	62960.0
199.05	3911.0
200.05	373.0
201.45	181.0
202.25	157.0
203.05	342.0
204.05	1985.0
205.05	3679.0
206.15	15132.0
207.15	2133.0
208.15	697.0
210.05	288.0
210.65	371.0
211.05	585.0
212.15	170.0
214.95	150.0
215.95	248.0
217.05	3822.0
218.05	696.0
221.05	3553.0
222.05	635.0
223.05	1088.0
224.05	8886.0
225.05	2295.0
226.15	341.0
227.05	3095.0
228.05	467.0
229.05	643.0
231.05	254.0
233.95	196.0
235.05	271.0
236.05	199.0
237.15	241.0
241.15	259.0
242.15	457.0
243.15	354.0
244.15	6261.0
245.05	841.0
246.05	1236.0
247.05	198.0
249.05	194.0
253.05	198.0
255.05	33600.0
256.05	4668.0
257.05	435.0
258.05	1836.0
258.95	265.0
265.05	814.0
266.05	214.0
272.05	191.0
273.05	1227.0
274.05	2982.0
275.05	15734.0
276.05	2245.0
277.05	1168.0
277.95	258.0
283.15	158.0
285.15	294.0
293.05	390.0
296.05	4375.0
297.05	485.0
303.05	421.0
304.05	189.0
314.05	323.0
315.05	389.0
316.05	211.0
320.95	203.0
323.15	1264.0
324.15	319.0
327.05	318.0
328.05	172.0
333.05	221.0
334.15	947.0
335.05	295.0
341.15	161.0
346.05	247.0
352.15	400.0
353.15	315.0
354.05	600.0
365.05	1900.0
366.05	325.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

372.15	793.0
373.05	166.0
383.15	294.0
402.05	423.0
402.95	492.0
403.95	197.0
421.15	497.0
422.05	384.0
423.15	3139.0
424.15	631.0
441.15	8905.0
442.15	60088.0
443.15	11849.0
444.05	1260.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

m/z	Abundance
38.15	224.0
39.15	932.0
40.05	694.0
44.15	291.0
49.15	224.0
50.15	3385.0
51.15	13956.0
52.15	821.0
56.15	527.0
57.15	963.0
61.05	198.0
62.15	312.0
63.15	655.0
64.15	164.0
65.25	351.0
69.15	16303.0
74.15	1811.0
75.15	2515.0
76.15	937.0
77.15	20384.0
78.15	1468.0
79.15	1183.0
80.05	760.0
81.05	1215.0
82.15	362.0
83.05	357.0
85.15	162.0
86.05	250.0
87.25	182.0
91.15	257.0
92.15	339.0
93.15	1611.0
94.15	180.0
96.15	150.0
98.15	1184.0
99.15	1236.0
101.05	659.0
103.05	160.0
104.05	541.0
105.15	411.0
106.05	211.0
107.15	6070.0
108.15	898.0
110.05	11622.0
111.05	1625.0
112.15	179.0
116.15	362.0
117.05	4027.0
118.05	320.0
122.05	493.0
123.05	678.0
124.15	281.0
125.15	231.0
126.05	248.0
127.05	23056.0
128.15	1600.0
129.05	8202.0
130.05	675.0
134.05	265.0
135.05	818.0
136.05	332.0
137.05	344.0
141.15	901.0
142.05	392.0
142.95	288.0
146.15	331.0
147.05	643.0
148.15	1190.0
149.05	265.0
153.05	345.0
154.05	224.0
155.15	634.0
156.05	932.0
157.05	188.0
158.05	312.0
159.05	183.0
160.15	395.0
161.05	718.0
162.05	166.0
165.05	484.0
166.15	461.0
167.05	2368.0
168.05	1210.0
169.05	183.0
172.05	162.0
173.05	294.0
174.05	441.0
175.15	838.0
176.15	319.0
177.05	473.0
179.05	1552.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

180.05	1138.0
181.05	407.0
185.15	832.0
186.15	6468.0
187.05	1922.0
188.15	225.0
189.05	371.0
191.05	191.0
192.05	490.0
193.05	678.0
196.05	1426.0
198.05	53312.0
199.05	3506.0
200.05	311.0
201.55	244.0
203.05	269.0
204.15	1877.0
205.05	2852.0
206.15	12099.0
207.15	1581.0
208.05	384.0
209.05	185.0
209.95	221.0
211.05	505.0
214.95	165.0
216.05	254.0
217.05	3183.0
218.15	387.0
221.05	3031.0
221.95	521.0
222.95	693.0
224.05	7150.0
225.15	1529.0
226.05	273.0
227.05	3004.0
228.05	541.0
229.05	715.0
231.05	276.0
233.95	221.0
237.15	323.0
240.95	157.0
242.05	348.0
243.05	416.0
244.15	5603.0
245.05	697.0
246.05	924.0
246.95	230.0
249.05	246.0
252.95	177.0
255.05	28840.0
256.05	4191.0
257.05	423.0
258.05	1772.0
259.05	268.0
265.05	535.0
273.05	913.0
274.05	2456.0
275.05	13379.0
276.05	1768.0
277.05	940.0
278.05	202.0
285.05	188.0
292.95	309.0
296.05	3687.0
297.05	511.0
303.15	460.0
313.95	162.0
315.05	525.0
323.15	1322.0
324.15	186.0
326.95	311.0
334.15	1045.0
335.05	227.0
341.15	233.0
346.05	287.0
352.05	415.0
353.05	326.0
354.05	504.0
355.15	171.0
365.05	1908.0
365.95	253.0
372.05	797.0
373.05	230.0
382.95	199.0
402.05	276.0
403.05	462.0
404.05	166.0
421.05	456.0
422.05	493.0
423.05	2922.0
424.05	603.0
441.15	9654.0
442.15	62216.0
443.15	11364.0
444.15	1129.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

Scan 2531 (17.558 min): BG016094.D
DFTPP13

m/z	Abundance
40.15	587.0
44.15	218.0
166.15	176.0
167.15	554.0
207.05	223.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13