

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032416\
 Data File : BG021483.D
 Acq On : 24 Mar 2016 13:33
 Operator : UM/SJ
 Sample : H1909-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T37

Quant Time: Mar 25 01:03:58 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 25 01:02:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	8822	20.00	ng/ul	0.00
18) Naphthalene-d8	10.87	136	44485	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	30239	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.42	188	76397	20.00	ng/ul	0.00
78) Chrysene-d12	21.66	240	85634	20.00	ng/ul	0.00
86) Perylene-d12	24.87	264	82650	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	679	3.45	ng/uL	0.00
5) Phenol-d5	7.34	99	12794	15.34	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.39	67	9916	20.07	ng/ul	0.01
9) 2-Chlorophenol-d4	7.64	132	11749	18.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	12175	17.04	ng/ul	0.00
19) Nitrobenzene-d5	9.23	128	6278	18.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.96	143	6935	18.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	12354	18.12	ng/ul	0.01
29) 4-Chloroaniline-d4	11.01	131	16551	18.56	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	50020	19.87	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	58046	18.70	ng/ul	0.00
52) 4-Nitrophenol-d4	15.09	143	3761	9.35	ng/ul	0.02
58) Fluorene-d10	15.67	176	43387	19.11	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	5418	10.73	ng/ul	0.00
71) Anthracene-d10	17.51	188	71389	19.07	ng/ul	0.00
79) Pyrene-d10	19.79	212	81201	20.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.65	264	84105	22.05	ng/ul	-0.01


Target Compounds						Qvalue
45) Dimethylphthalate	14.13	163	14379	5.50	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032416\
Data File : BG021483.D
Acq On : 24 Mar 2016 13:33
Operator : UM/SJ
Sample : H1909-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T37

Quant Time: Mar 25 01:03:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 25 01:02:38 2016
Response via : Initial Calibration

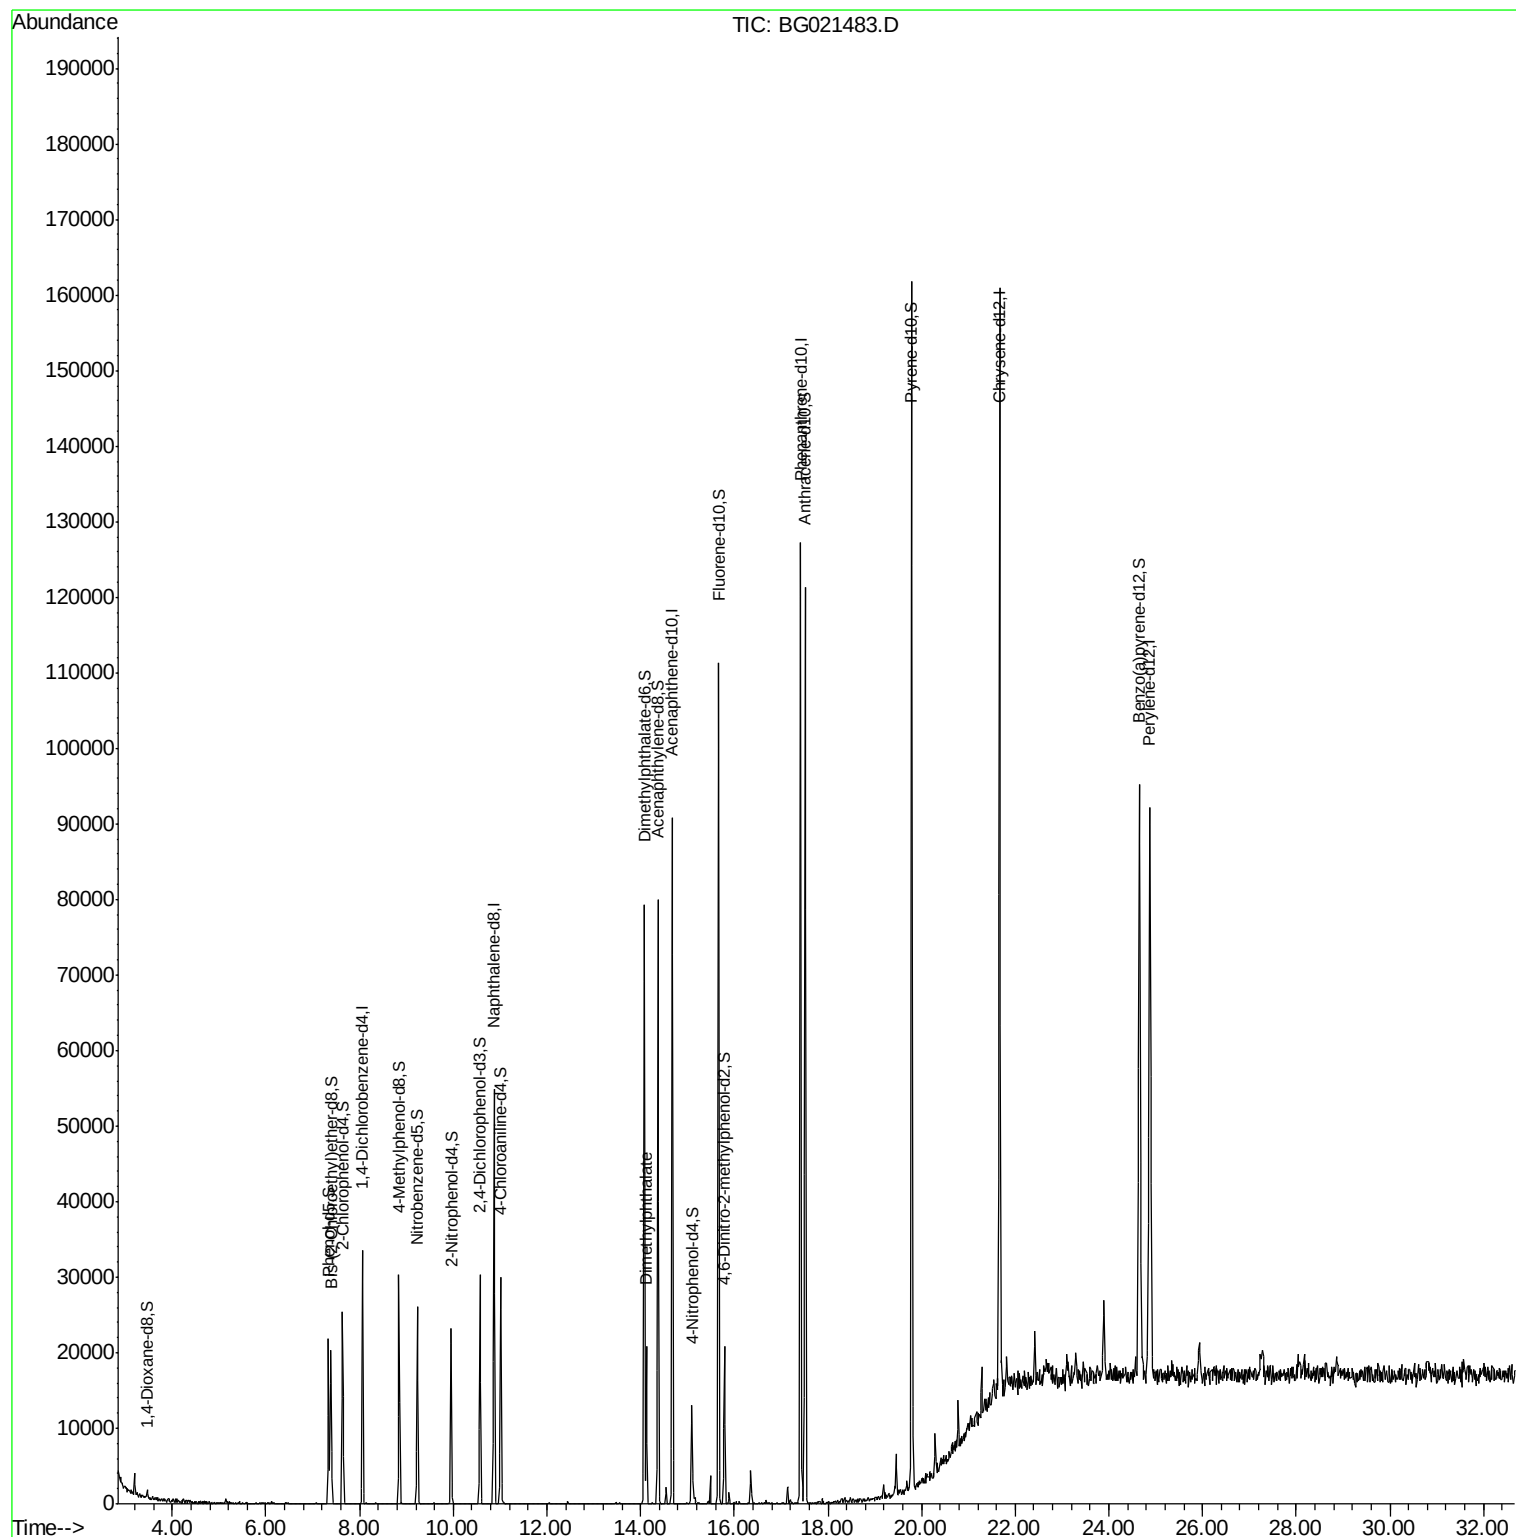

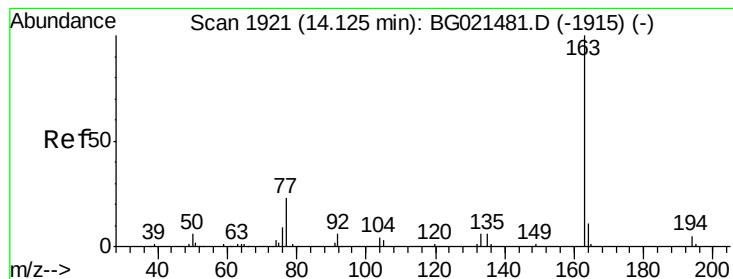

#45

Dimethylphthalate

Concen: 5.50 ng/ul

RT: 14.13 min Scan# 1921

Delta R.T. 0.00 min

Lab File: BG021483.D


Acq: 24 Mar 2016 13:33

Instrument :

BNA_G

ClientSampleId :

A4T37

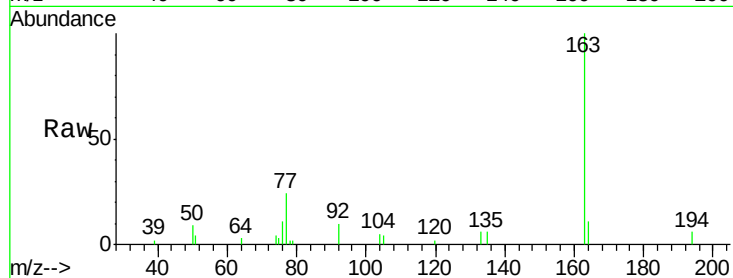


Tgt Ion:163 Resp: 14379

Ion Ratio Lower Upper

163 100

194 5.6 3.9 5.9

164 11.1 8.7 13.1

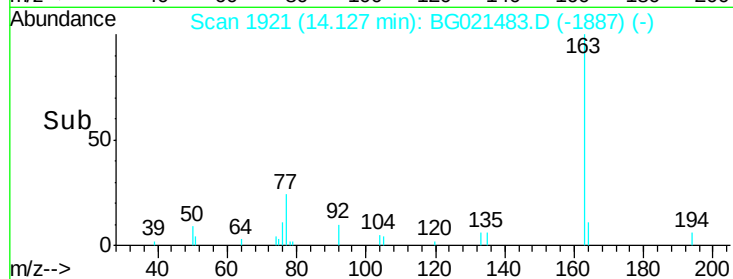

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

