

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032416\
 Data File : BG021488.D
 Acq On : 24 Mar 2016 17:04
 Operator : UM/SJ
 Sample : H1909-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T44

Quant Time: Mar 25 01:55:28 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 25 01:20:42 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	10273	20.00	ng/ul	0.00
18) Naphthalene-d8	10.87	136	49050	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	32130	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.42	188	79889	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	91323	20.00	ng/ul	0.00
86) Perylene-d12	24.88	264	86719	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.46	96	865	3.78	ng/uL	0.00
5) Phenol-d5	7.33	99	25405	26.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	17622	30.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	20591	27.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	23101	27.77	ng/ul	0.00
19) Nitrobenzene-d5	9.23	128	11104	30.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.96	143	12864	30.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	21990	29.24	ng/ul	0.00
29) 4-Chloroaniline-d4	11.01	131	30496	31.02	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	85923	32.12	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	103312	31.33	ng/ul	0.00
52) 4-Nitrophenol-d4	15.08	143	8287	19.38	ng/ul	0.00
58) Fluorene-d10	15.67	176	76148	31.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	12003	22.74	ng/ul	0.00
71) Anthracene-d10	17.52	188	125914	32.16	ng/ul	0.00
79) Pyrene-d10	19.79	212	147935	34.74	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.66	264	152919	38.21	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.13	163	36360	13.08	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032416\
Data File : BG021488.D
Acq On : 24 Mar 2016 17:04
Operator : UM/SJ
Sample : H1909-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T44

Quant Time: Mar 25 01:55:28 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 25 01:20:42 2016
Response via : Initial Calibration

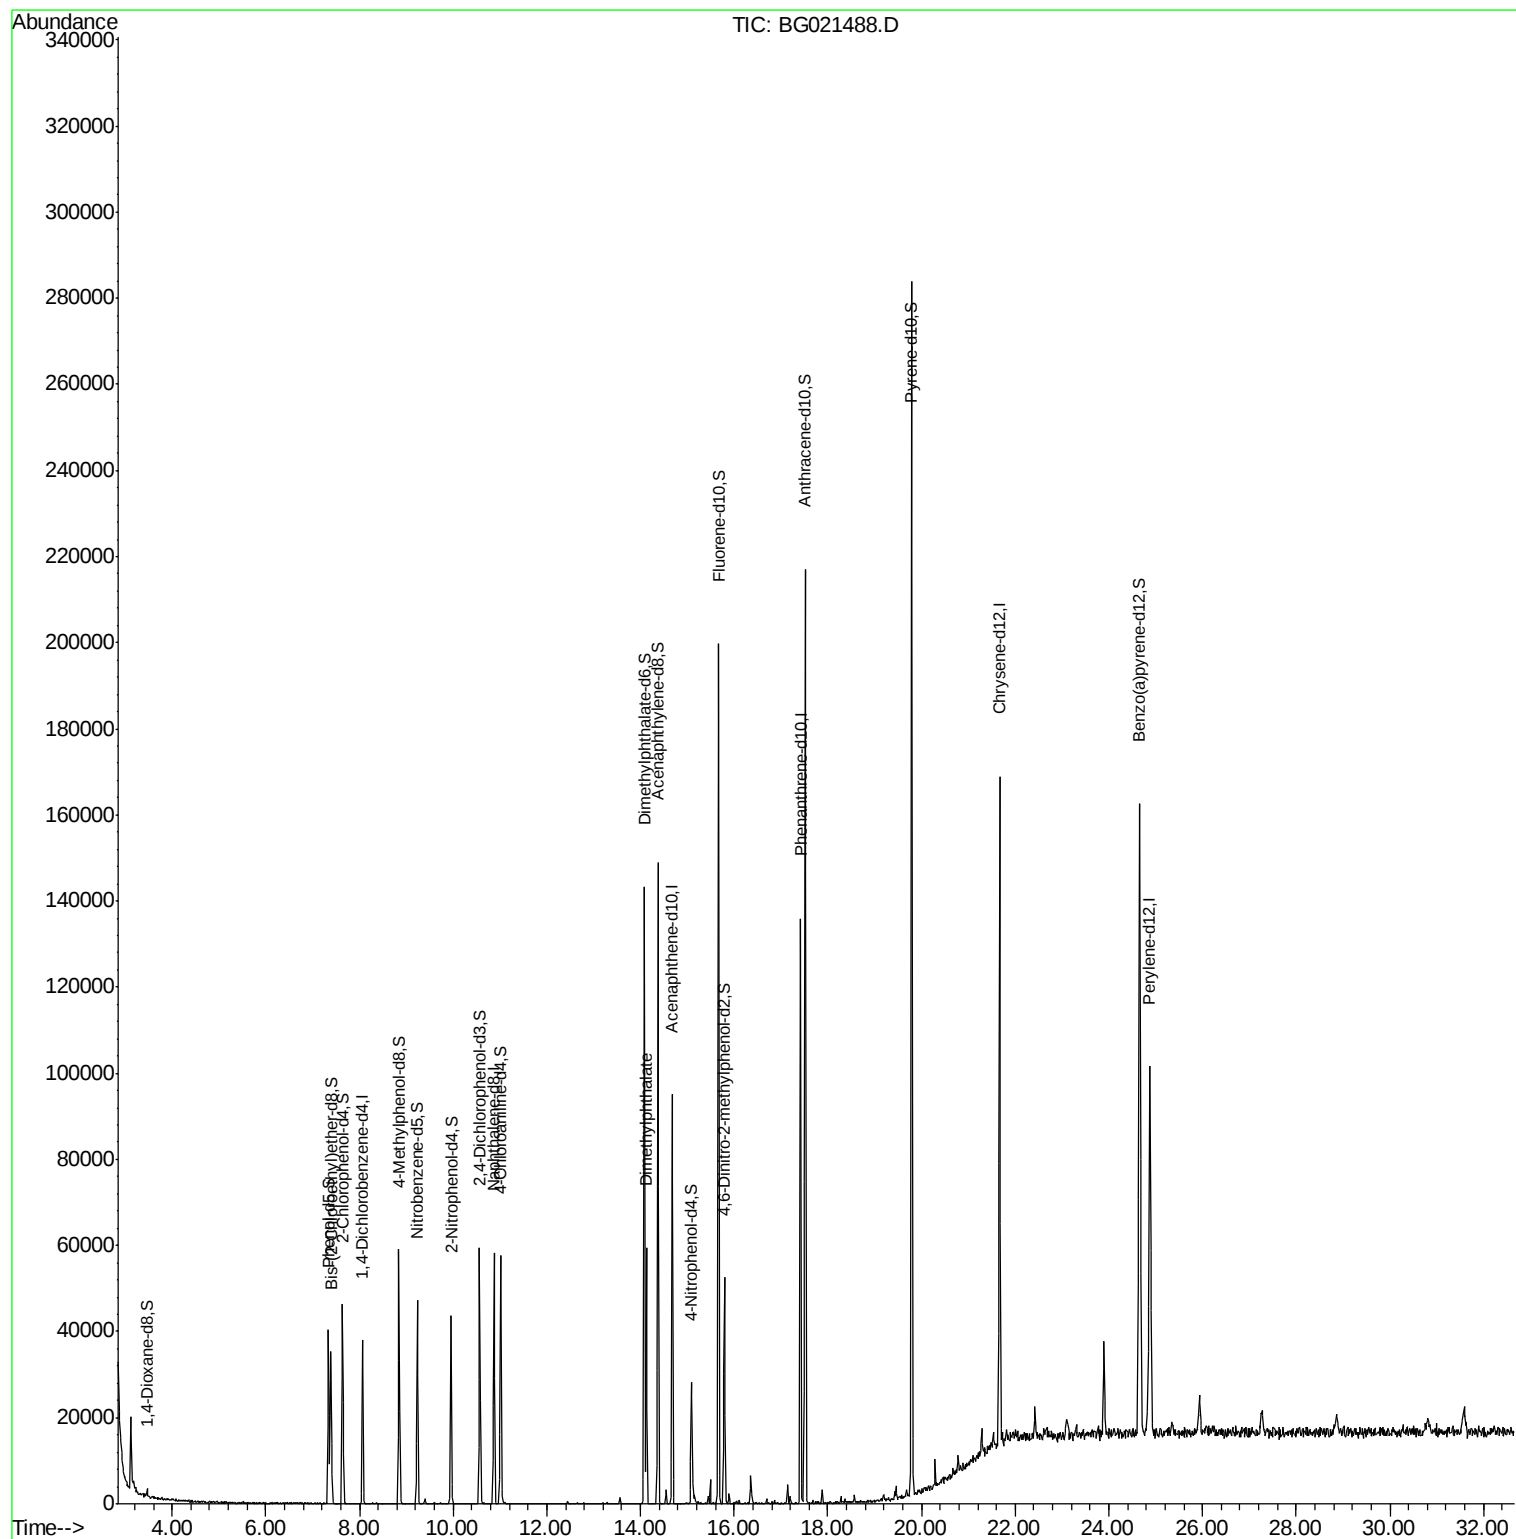

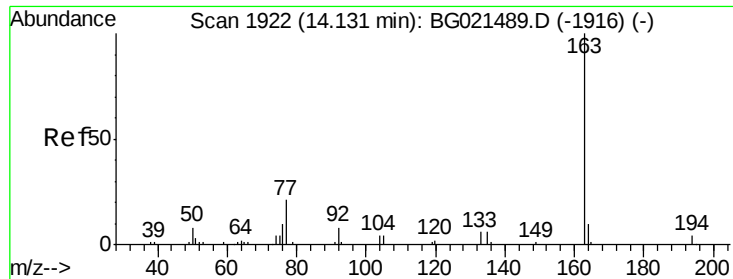

#45
 Dimethylphthalate
 Concen: 13.08 ng/ul
 RT: 14.13 min Scan# 1921
 Delta R.T. -0.00 min
 Lab File: BG021488.D
 Acq: 24 Mar 2016 17:04

Instrument :
 BNA_G
 ClientSampleId :
 A4T44

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.9	5.9
164	9.8	8.7	13.1

