

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032416\
 Data File : BG021484.D
 Acq On : 24 Mar 2016 14:13
 Operator : UM/SJ
 Sample : H1909-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4T38

Quant Time: Mar 25 01:04:03 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 25 01:02:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	8590	20.00	ng/ul	0.01
18) Naphthalene-d8	10.87	136	41756	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	28484	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.42	188	73289	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	81566	20.00	ng/ul	0.00
86) Perylene-d12	24.88	264	77712	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	646	3.37	ng/uL	0.01
5) Phenol-d5	7.34	99	15705	19.34	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.39	67	10781	22.41	ng/ul	0.01
9) 2-Chlorophenol-d4	7.64	132	12862	20.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	14231	20.46	ng/ul	0.00
19) Nitrobenzene-d5	9.24	128	7251	23.15	ng/ul	0.01
22) 2-Nitrophenol-d4	9.95	143	7766	21.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	13771	21.51	ng/ul	0.01
29) 4-Chloroaniline-d4	11.02	131	19374	23.15	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	57751	24.35	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	65472	22.40	ng/ul	0.00
52) 4-Nitrophenol-d4	15.09	143	5654	14.91	ng/ul	0.02
58) Fluorene-d10	15.66	176	49818	23.30	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	7652	15.80	ng/ul	0.00
71) Anthracene-d10	17.52	188	84286	23.47	ng/ul	0.00
79) Pyrene-d10	19.79	212	94710	24.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.65	264	98060	27.34	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.13	163	14196	5.76	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032416\
Data File : BG021484.D
Acq On : 24 Mar 2016 14:13
Operator : UM/SJ
Sample : H1909-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4T38

Quant Time: Mar 25 01:04:03 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 25 01:02:38 2016
Response via : Initial Calibration

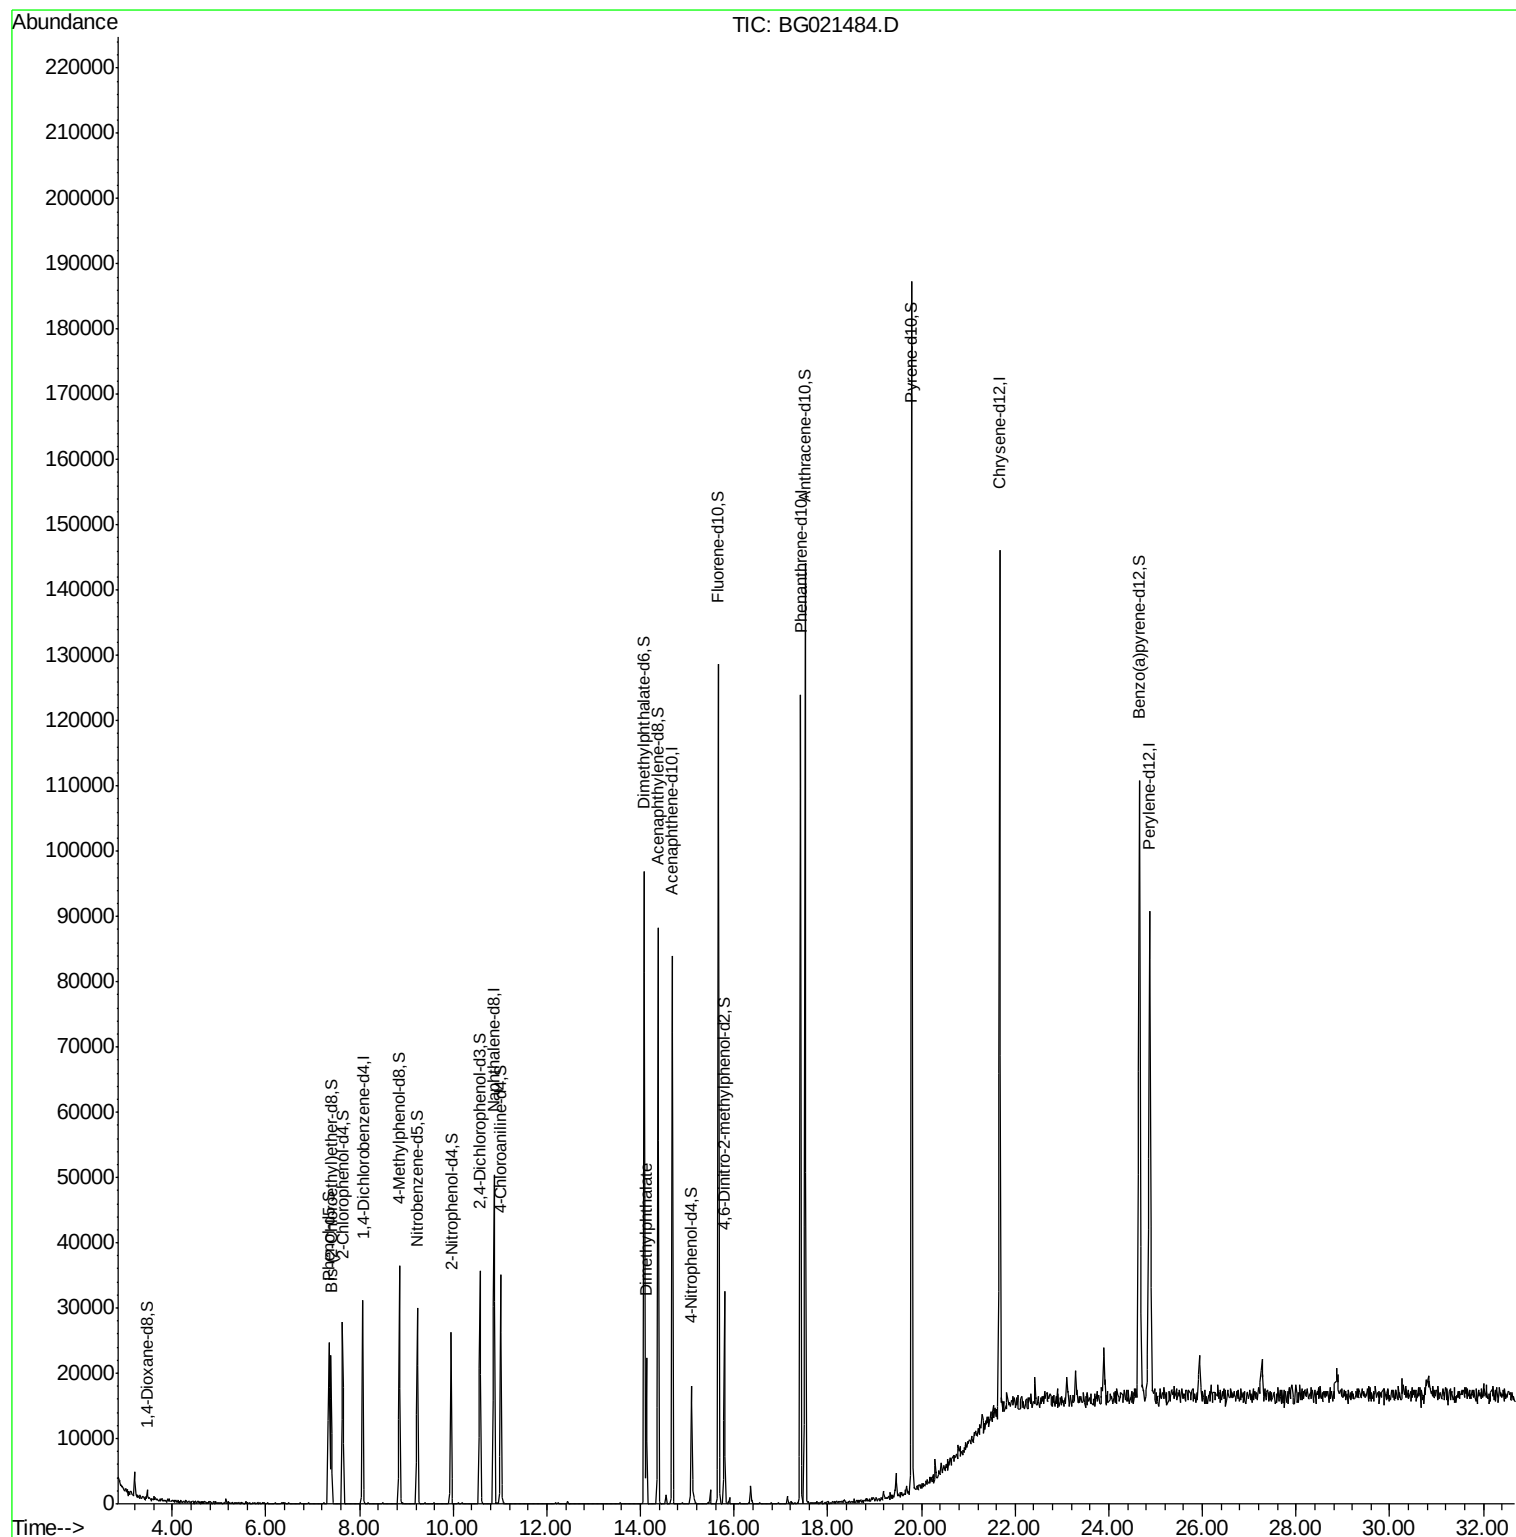

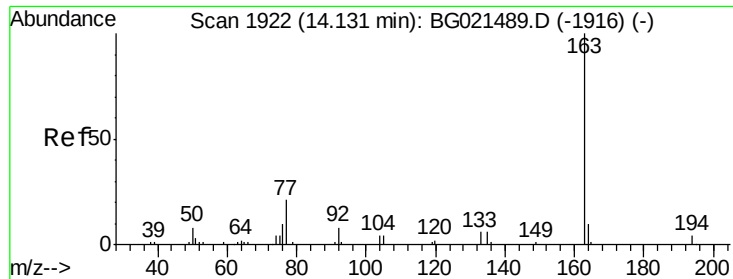

#45
 Dimethylphthalate
 Concen: 5.76 ng/ul
 RT: 14.13 min Scan# 1921
 Delta R.T. 0.00 min
 Lab File: BG021484.D
 Acq: 24 Mar 2016 14:13

Instrument :
 BNA_G
 ClientSampleId :
 A4T38

Tot Ion	Ratio	Lower	Upper
163	100		
194	5.2	3.9	5.9
164	10.8	8.7	13.1

